

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF063021\
Data File : FF008709.D
Signal(s) : FID2B.ch
Acq On : 30 Jun 2021 16:33
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jul 01 01:17:26 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF062321.M
Quant Title :
QLast Update : Thu Jun 24 08:07:11 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.746	2801156	24.578 ug/ml
Target Compounds			
13) N-TRIACONTANE	17.799	116502	0.972 ug/ml
14) N-DOTRIACONTANE	18.630	165082	1.409 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF063021\
Data File : FF008709.D
Signal(s) : FID2B.ch
Acq On : 30 Jun 2021 16:33
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jul 01 01:17:26 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF062321.M
Quant Title :
QLast Update : Thu Jun 24 08:07:11 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

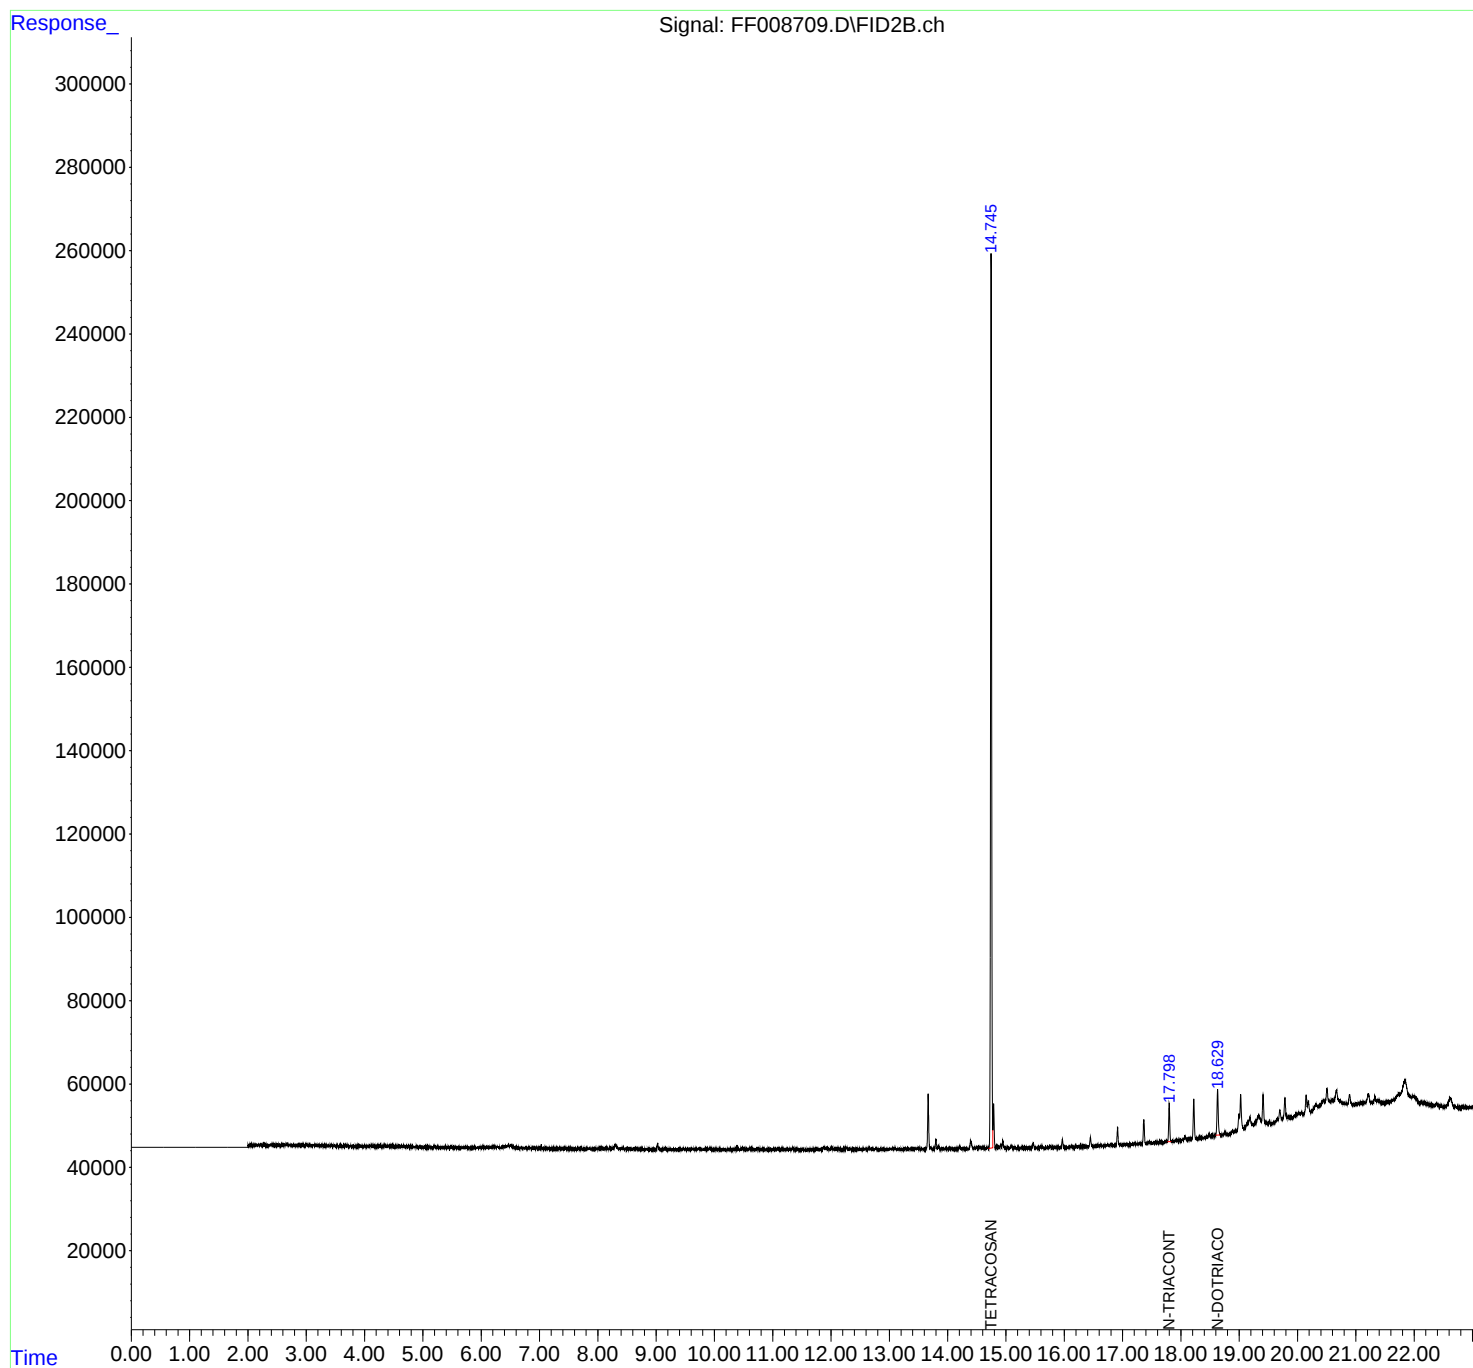


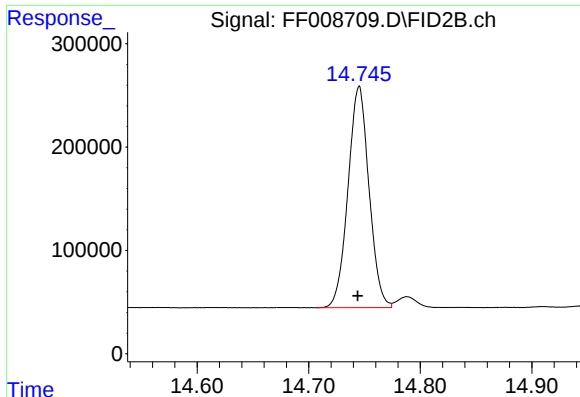

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.746 min
Delta R.T.: 0.002 min
Response: 2801156
Conc: 24.58 ug/ml

Instrument :
FID_F
ClientSampleId :

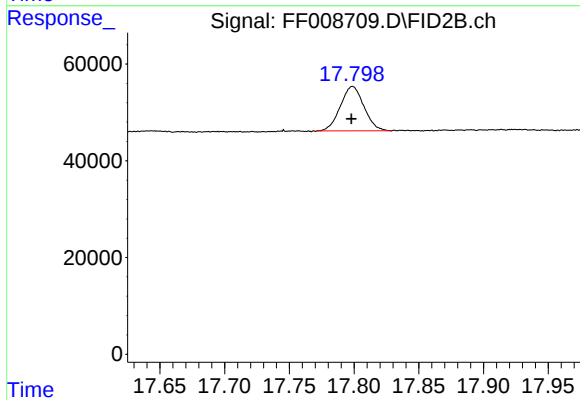

#13 N-TRIACONTANE

R.T.: 17.799 min
Delta R.T.: 0.000 min
Response: 116502
Conc: 0.97 ug/ml

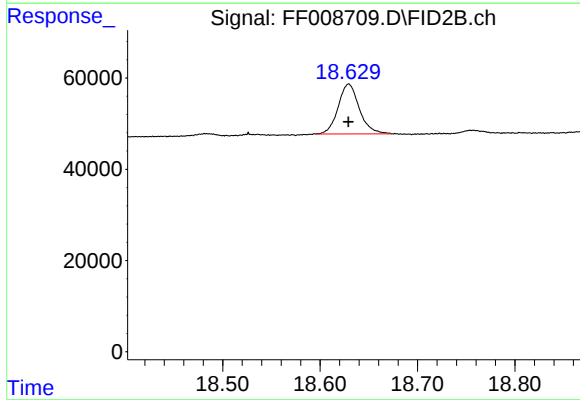

#14 N-DOTRIACONTANE

R.T.: 18.630 min
Delta R.T.: 0.000 min
Response: 165082
Conc: 1.41 ug/ml