

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF063022\
Data File : FF010936.D
Signal(s) : FID2B.ch
Acq On : 30 Jun 2022 15:50
Operator : AJ\MA
Sample : RT MARKER
Misc :
ALS Vial : 4 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Jul 01 01:44:27 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF063022.M
Quant Title :
QLast Update : Fri Jul 01 01:40:42 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
3) N-DODECANE	6.536	1624395	14.586 ug/ml
12) N-OCTACOSANE	16.989	1597817	15.310 ug/ml
13) N-TRIACONTANE	17.874	188217	1.793 ug/ml
14) N-DOTRIACONTANE	18.706	311905	2.906 ug/ml
15) N-TETRATRIACONTANE	19.487	230996	2.369 ug/ml
16) N-HEXATRIACONTANE	20.225	145542	1.693 ug/ml
17) N-OCTATRIACONTANE	20.879f	20827	0.278 ug/ml
18) N-TETRACONTANE	21.763	211177	2.478 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF063022\
Data File : FF010936.D
Signal(s) : FID2B.ch
Acq On : 30 Jun 2022 15:50
Operator : AJ\MA
Sample : RT MARKER
Misc :
ALS Vial : 4 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Jul 01 01:44:27 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF063022.M
Quant Title :
QLast Update : Fri Jul 01 01:40:42 2022
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

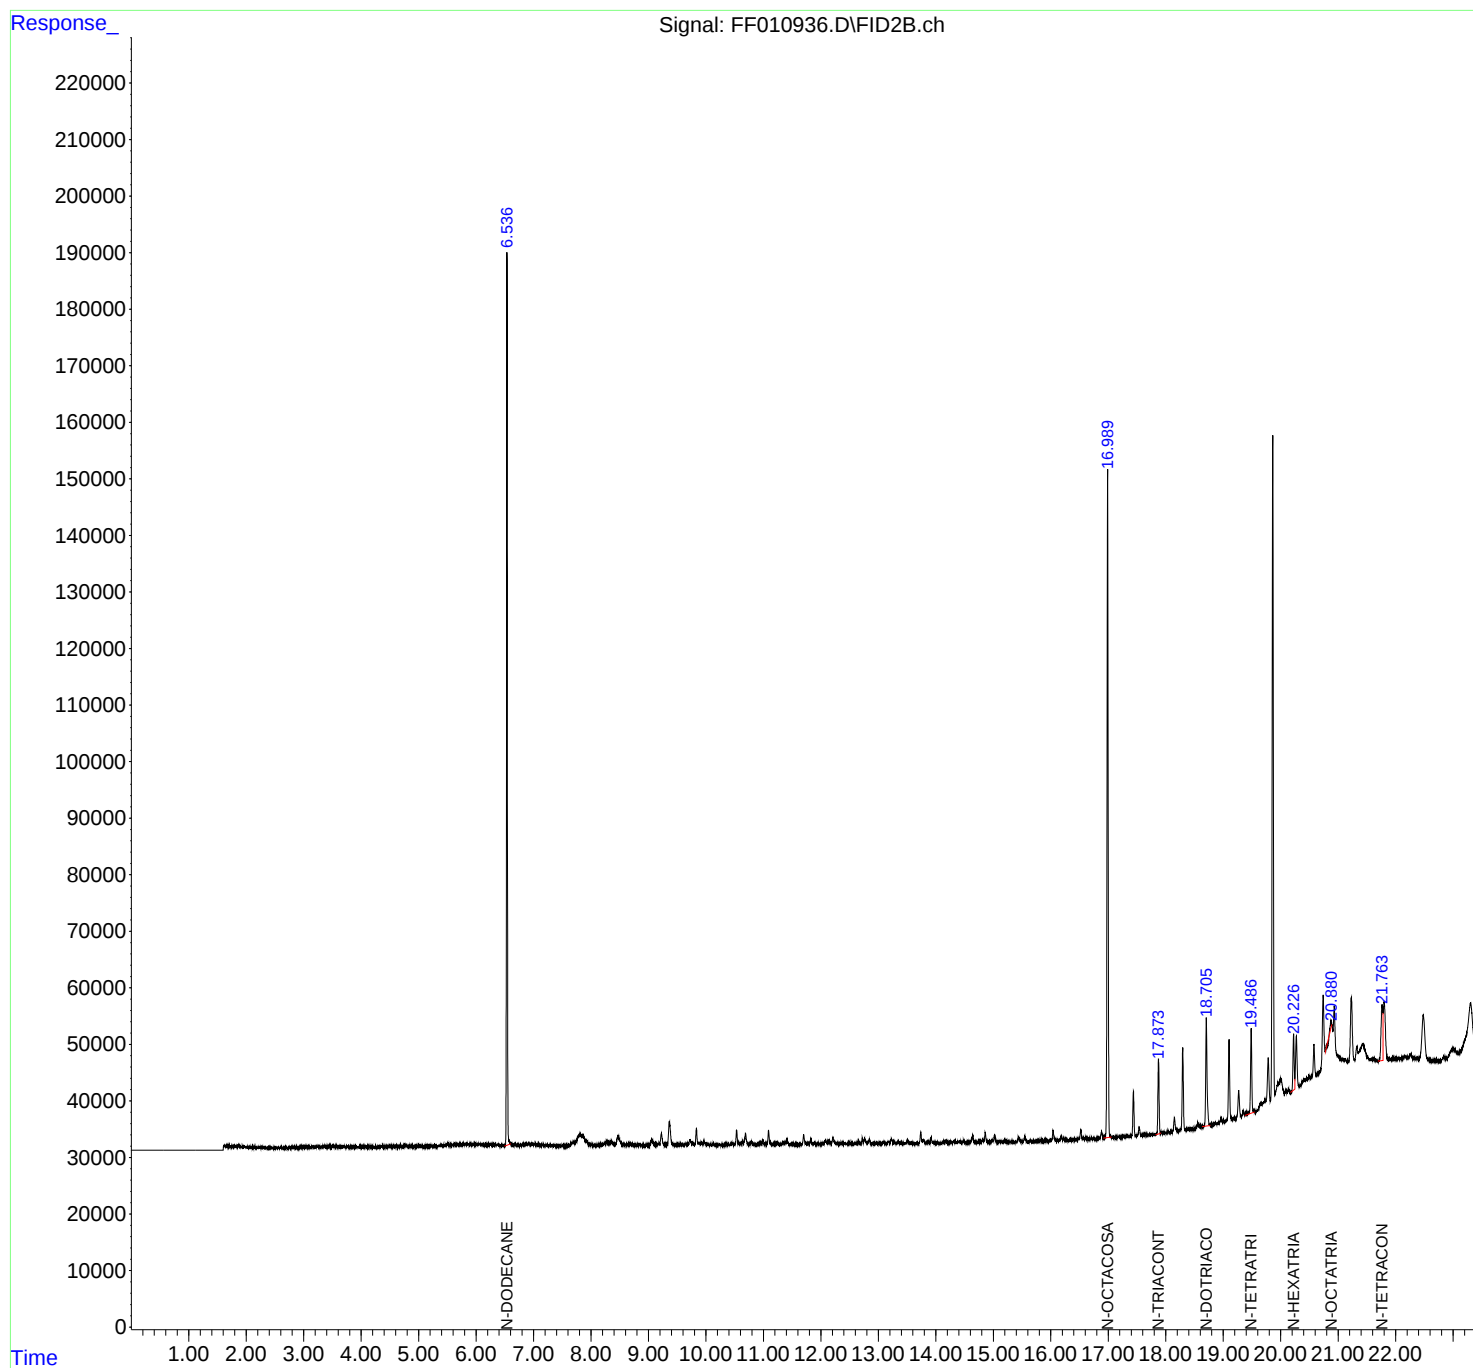

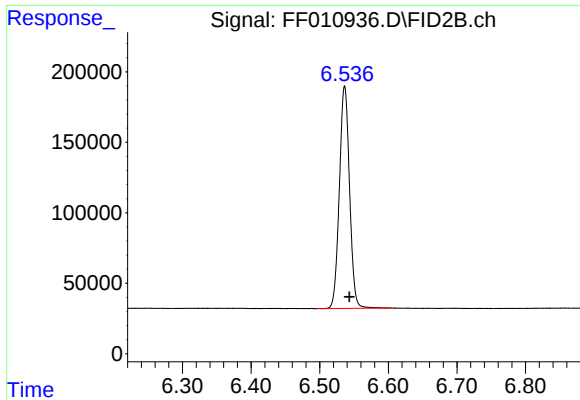


#3 N-DODECANE

R.T.: 6.536 min
Delta R.T.: -0.007 min
Response: 1624395
Conc: 14.59 ug/ml

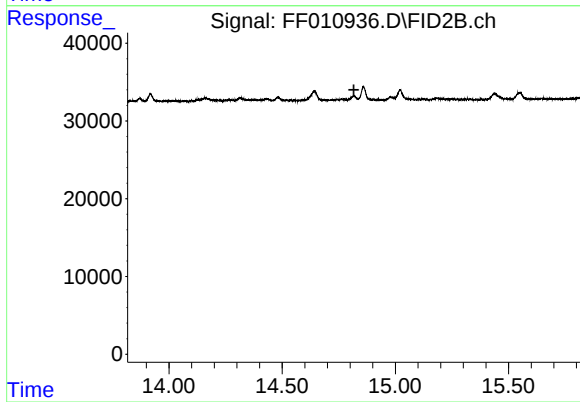


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T.: 14.817 min
Response: 0
Conc: N.D.

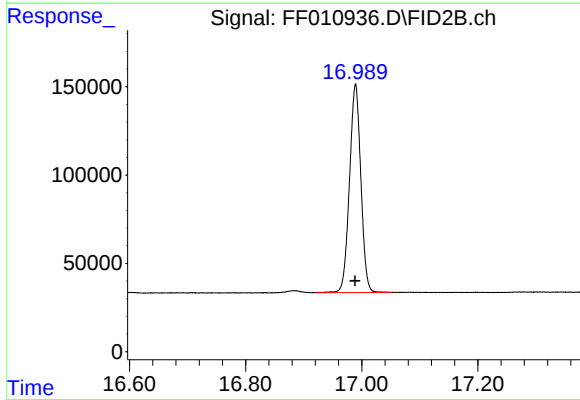


#12 N-OCTACOSANE

R.T.: 16.989 min
Delta R.T.: 0.000 min
Response: 1597817
Conc: 15.31 ug/ml

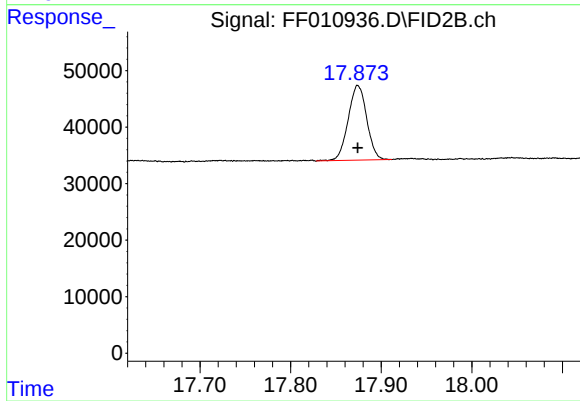


#13 N-TRIACONTANE

R.T.: 17.874 min
Delta R.T.: 0.000 min
Response: 188217
Conc: 1.79 ug/ml

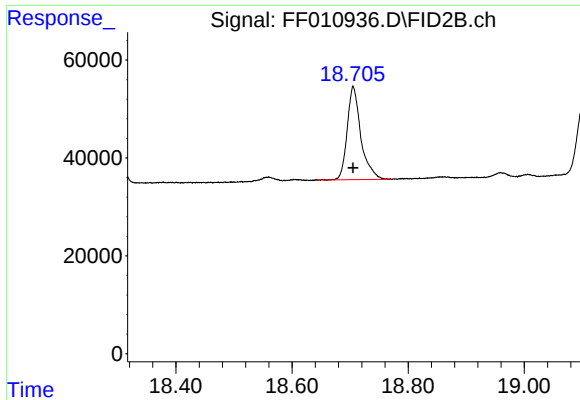


#14 N-DOTRIACONTANE

R.T.: 18.706 min
Delta R.T.: 0.000 min
Response: 311905
Conc: 2.91 ug/ml

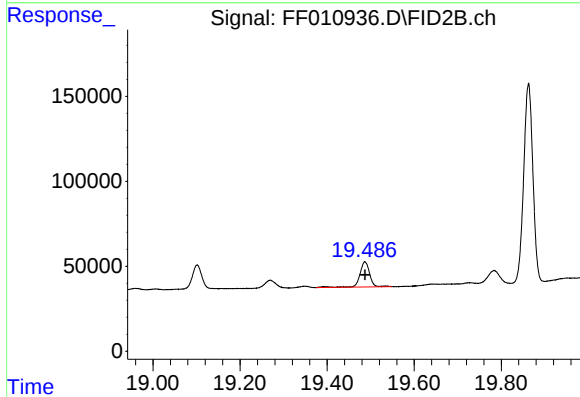


#15 N-TETRATRIACONTANE

R.T.: 19.487 min
Delta R.T.: 0.000 min
Response: 230996
Conc: 2.37 ug/ml

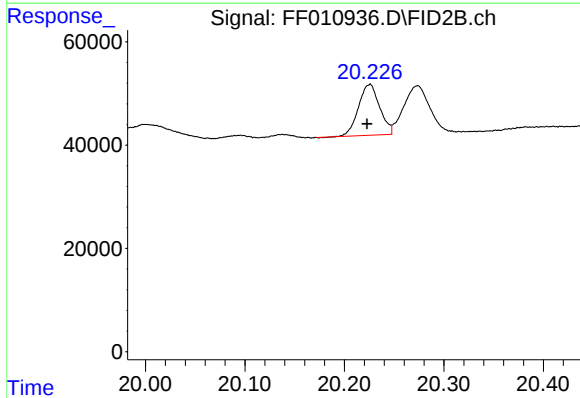


#16 N-HEXATRIACONTANE

R.T.: 20.225 min
Delta R.T.: 0.002 min
Response: 145542
Conc: 1.69 ug/ml

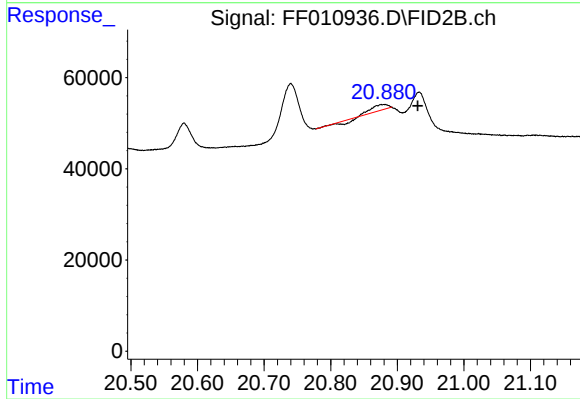

#17 N-OCTATRIACONTANE

R.T.: 20.879 min
Delta R.T.: -0.052 min
Response: 20827
Conc: 0.28 ug/ml

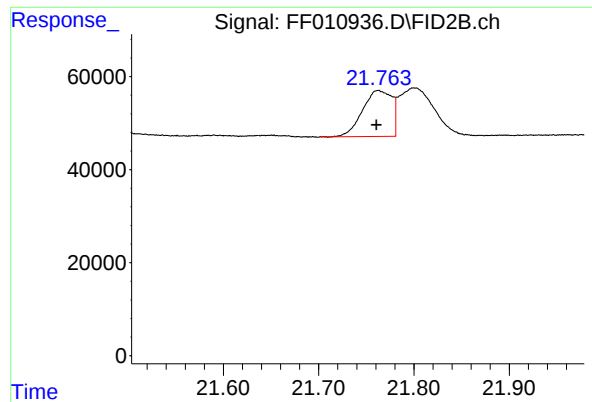

#18 N-TETRACONTANE

R.T.: 21.763 min
Delta R.T.: 0.002 min
Response: 211177
Conc: 2.48 ug/ml