

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF063022\
Data File : FF010937.D
Signal(s) : FID2B.ch
Acq On : 30 Jun 2022 16:20
Operator : AJ\MA
Sample : PB145894BL
Misc :
ALS Vial : 54 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Jul 01 01:44:38 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF063022.M
Quant Title :
QLast Update : Fri Jul 01 01:40:42 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.817	2720001	28.995 ug/ml
Target Compounds			
16) N-HEXATRIACONTANE	20.272	116267	1.352 ug/ml
18) N-TETRACONTANE	21.797	225299	2.644 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF063022\
Data File : FF010937.D
Signal(s) : FID2B.ch
Acq On : 30 Jun 2022 16:20
Operator : AJ\MA
Sample : PB145894BL
Misc :
ALS Vial : 54 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Jul 01 01:44:38 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF063022.M
Quant Title :
QLast Update : Fri Jul 01 01:40:42 2022
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

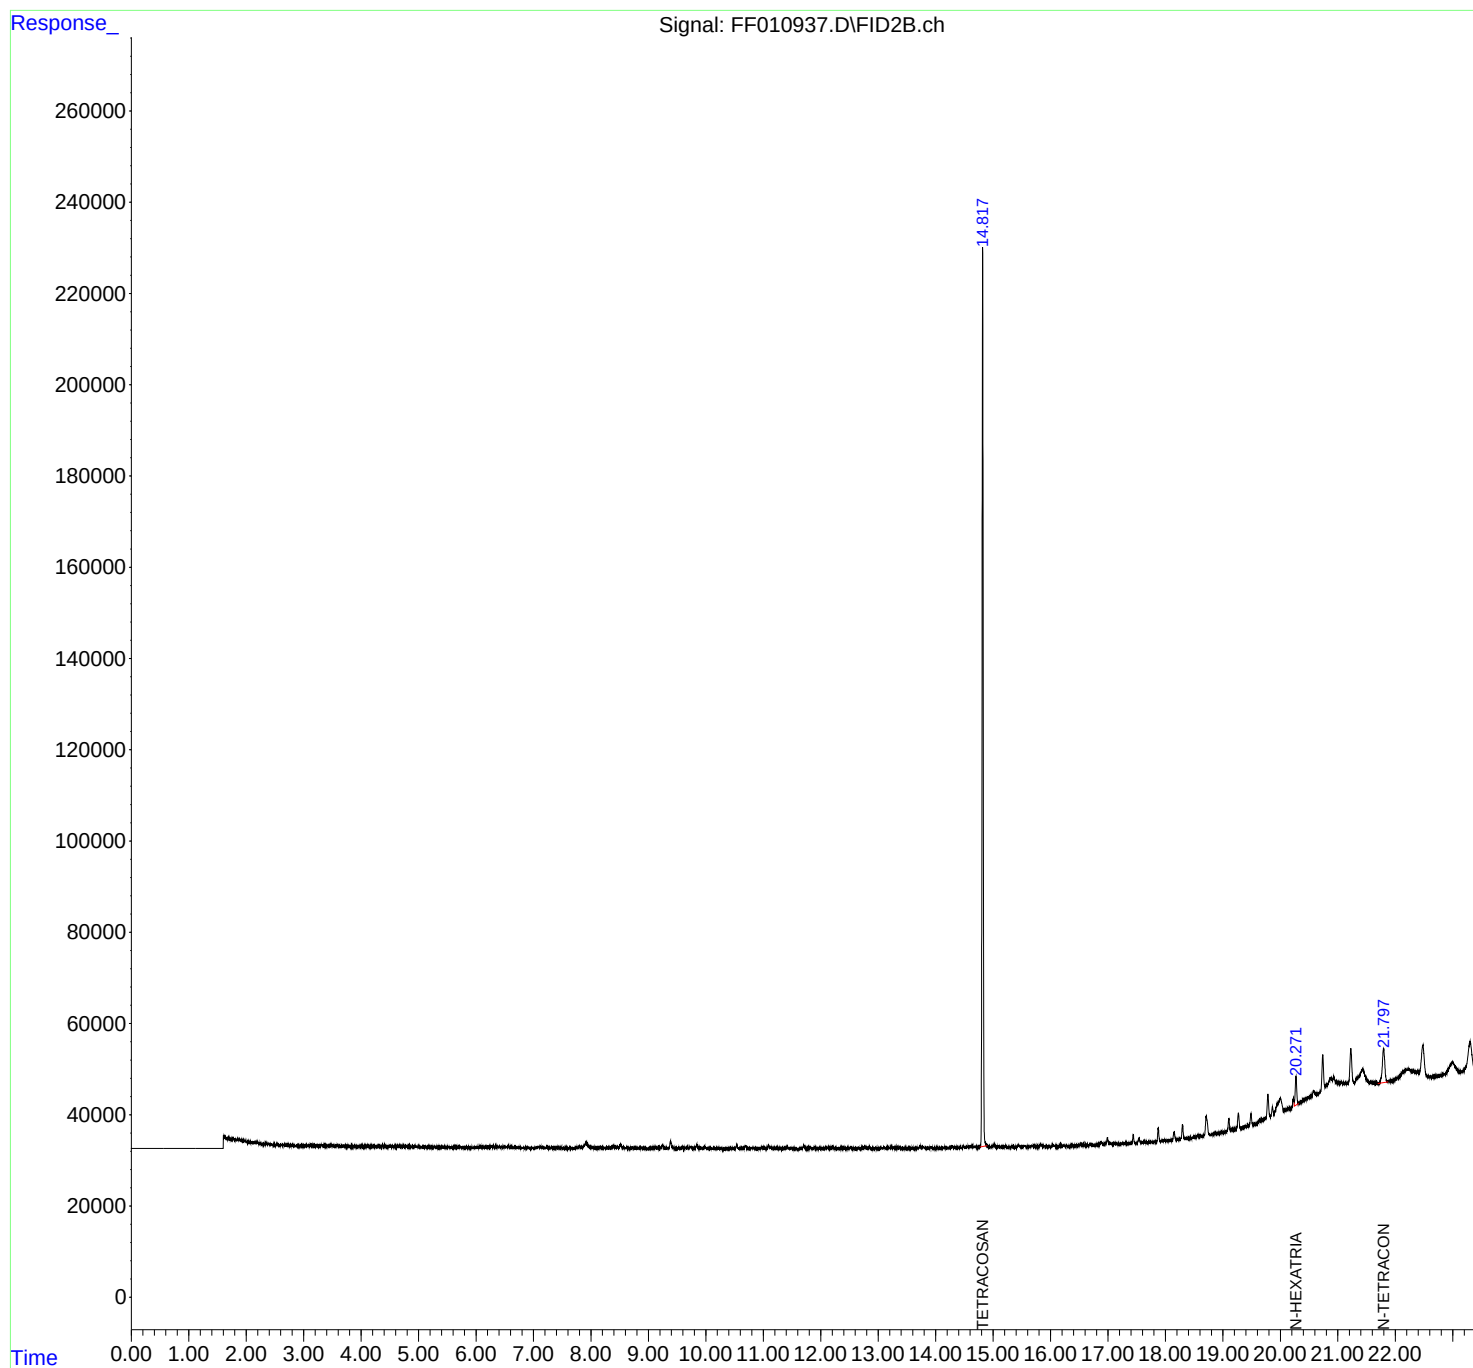

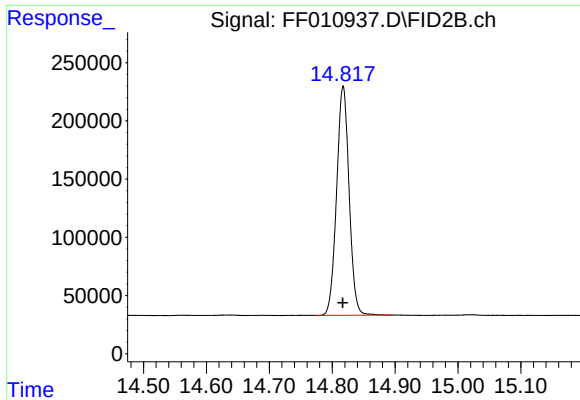


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.817 min
Delta R.T.: 0.000 min
Response: 2720001
Conc: 28.99 ug/ml

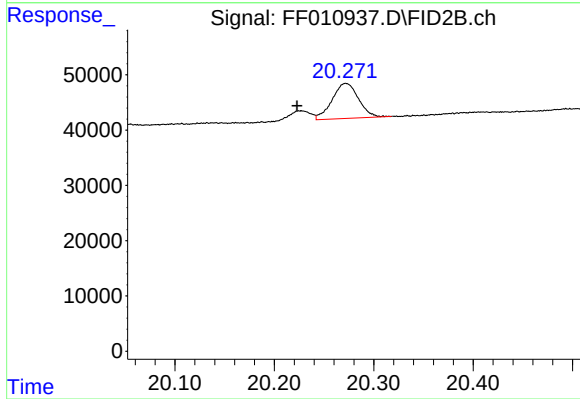

#16 N-HEXATRIACONTANE

R.T.: 20.272 min
Delta R.T.: 0.049 min
Response: 116267
Conc: 1.35 ug/ml

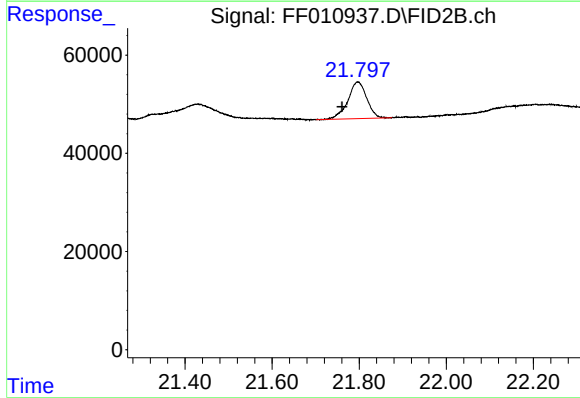

#18 N-TETRACONTANE

R.T.: 21.797 min
Delta R.T.: 0.036 min
Response: 225299
Conc: 2.64 ug/ml