

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_F\Data\FF063025\  
Data File : FF016034.D  
Signal(s) : FID2B.ch  
Acq On : 30 Jun 2025 10:41  
Operator : YP\AJ  
Sample : RT MARKER  
Misc :  
ALS Vial : 54 Sample Multiplier: 1

Instrument :  
FID\_F  
ClientSampleId :  
RT MARKER

Integration File: autoint1.e  
Quant Time: Jul 01 03:14:04 2025  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_F\Method\FF061325.M  
Quant Title :  
QLast Update : Fri Jun 13 15:23:30 2025  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1uL  
Signal Phase : Rxi-1ms  
Signal Info : 20mx0.18mmx0.18um

| Compound                    |              | R.T.   | Response | Conc Units   |
|-----------------------------|--------------|--------|----------|--------------|
| -----                       |              |        |          |              |
| System Monitoring Compounds |              |        |          |              |
| Target Compounds            |              |        |          |              |
| 3)                          | N-DODECANE   | 6.795  | 2459391  | 18.470 ug/ml |
| 12)                         | N-OCTACOSANE | 17.274 | 2241117  | 16.976 ug/ml |
| -----                       |              |        |          |              |

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_F\Data\FF063025\  
Data File : FF016034.D  
Signal(s) : FID2B.ch  
Acq On : 30 Jun 2025 10:41  
Operator : YP\AJ  
Sample : RT MARKER  
Misc :  
ALS Vial : 54 Sample Multiplier: 1

Instrument :  
FID\_F  
ClientSampleId :  
RT MARKER

Integration File: autoint1.e  
Quant Time: Jul 01 03:14:04 2025  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_F\Method\FF061325.M  
Quant Title :  
QLast Update : Fri Jun 13 15:23:30 2025  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1uL  
Signal Phase : Rxi-1ms  
Signal Info : 20mx0.18mmx0.18um

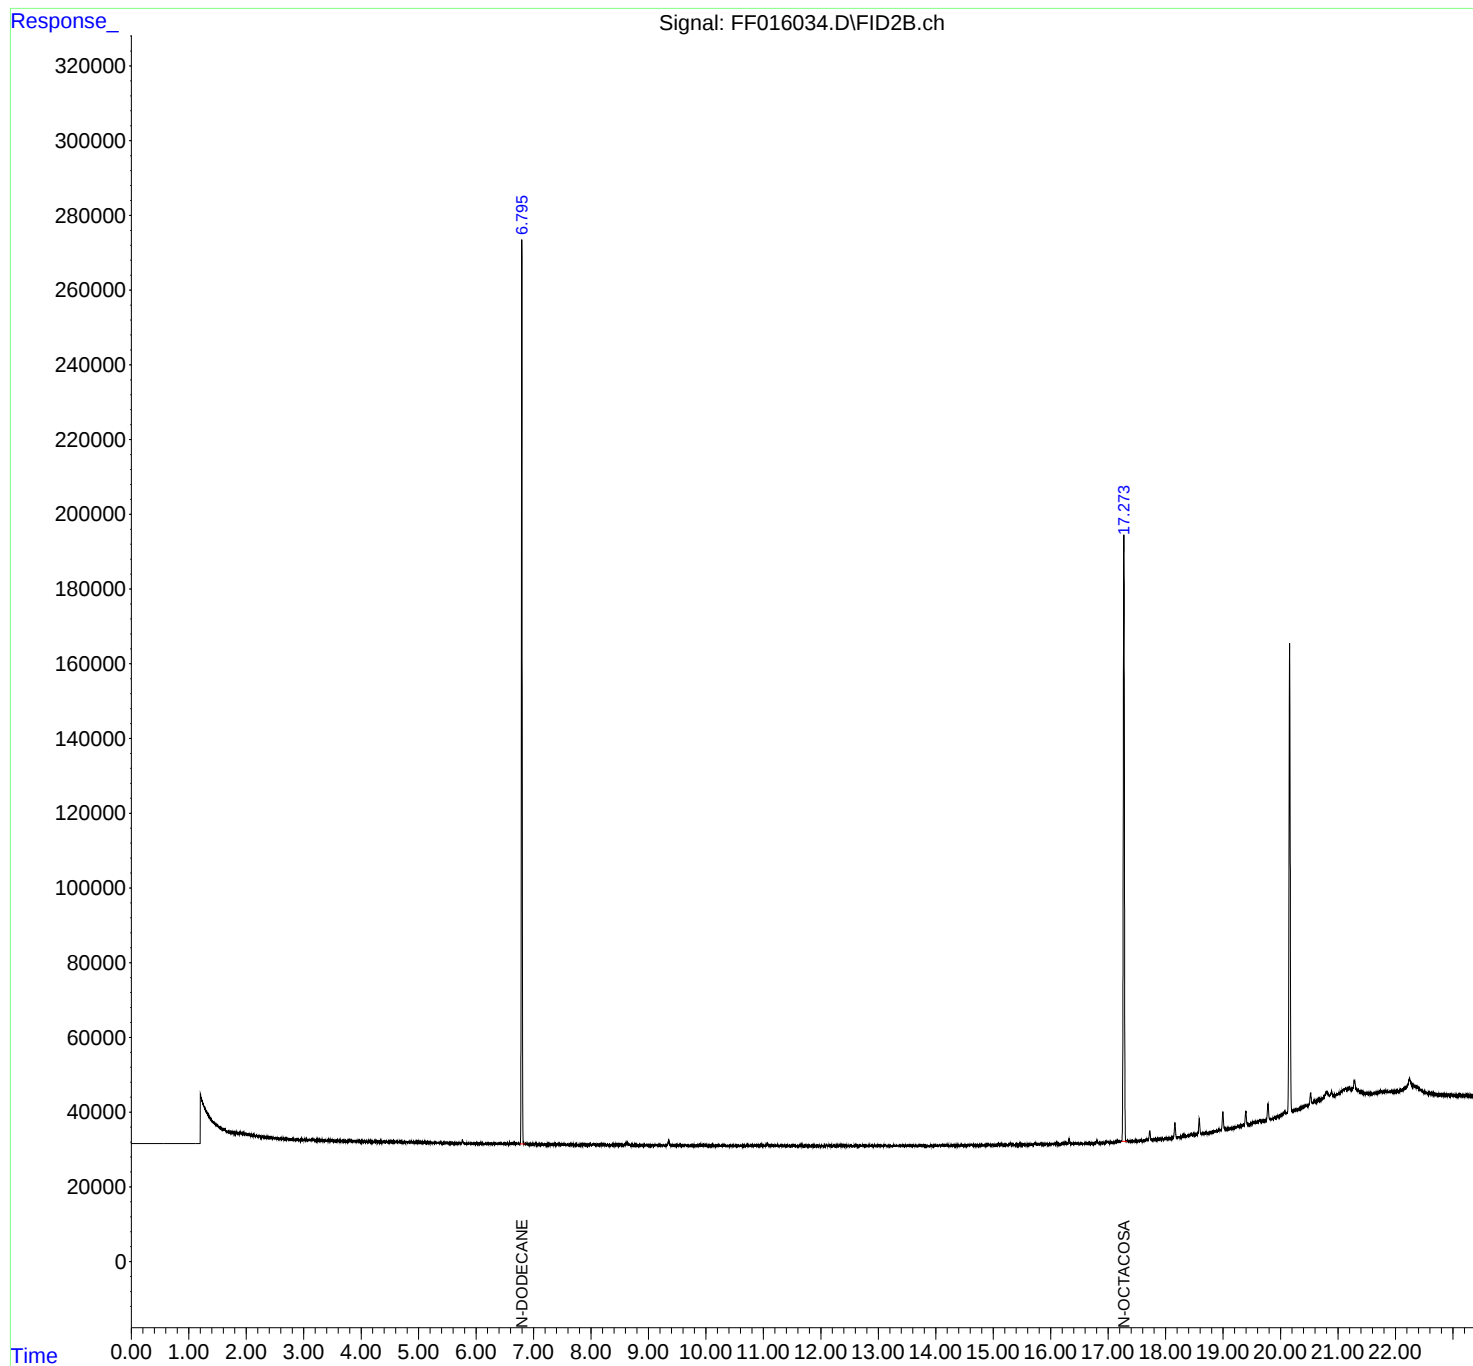


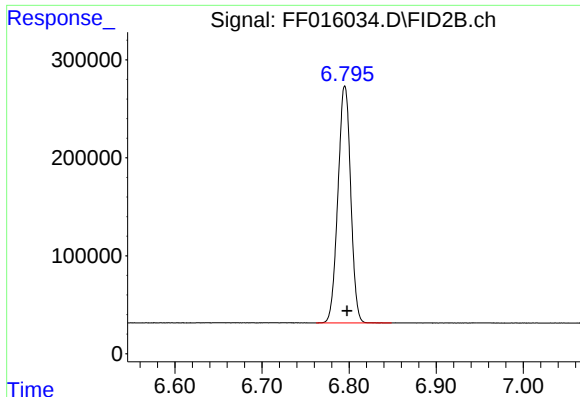

#3 N-DODECANE


R.T.: 6.795 min  
Delta R.T.: -0.003 min  
Response: 2459391  
Conc: 18.47 ug/ml

Instrument :  
FID\_F  
ClientSampleId :  
RT MARKER

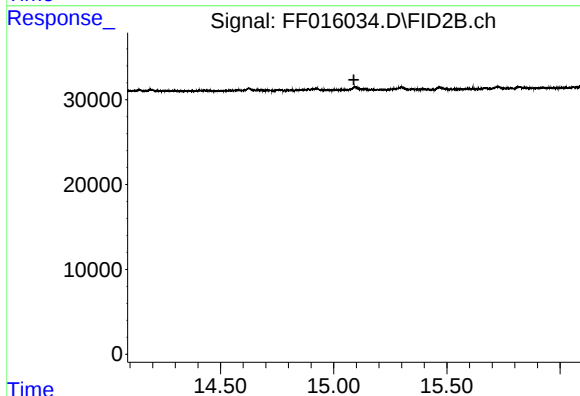

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min  
Exp R.T. : 15.089 min  
Response: 0  
Conc: N.D.

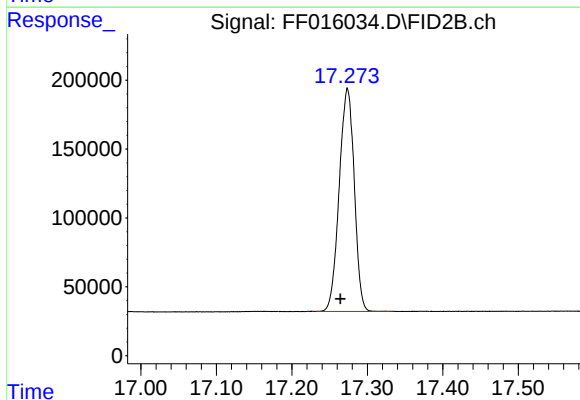

#12 N-OCTACOSANE

R.T.: 17.274 min  
Delta R.T.: 0.010 min  
Response: 2241117  
Conc: 16.98 ug/ml