

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF070119\
Data File : FF004879.D
Signal(s) : FID2B.ch
Acq On : 01 Jul 2019 08:58
Operator : DD\AJ
Sample : MECL2
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
MECL2

Integration File: autoint1.e
Quant Time: Jul 02 01:48:34 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF062619.M
Quant Title :
QLast Update : Wed Jun 26 14:27:24 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
14) N-DOTRIACONTANE	18.626	87530	0.769 ug/ml
16) N-HEXATRIACONTANE	20.123	955421	9.227 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF070119\
Data File : FF004879.D
Signal(s) : FID2B.ch
Acq On : 01 Jul 2019 08:58
Operator : DD\AJ
Sample : MECL2
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
MECL2

Integration File: autoint1.e
Quant Time: Jul 02 01:48:34 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF062619.M
Quant Title :
QLast Update : Wed Jun 26 14:27:24 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

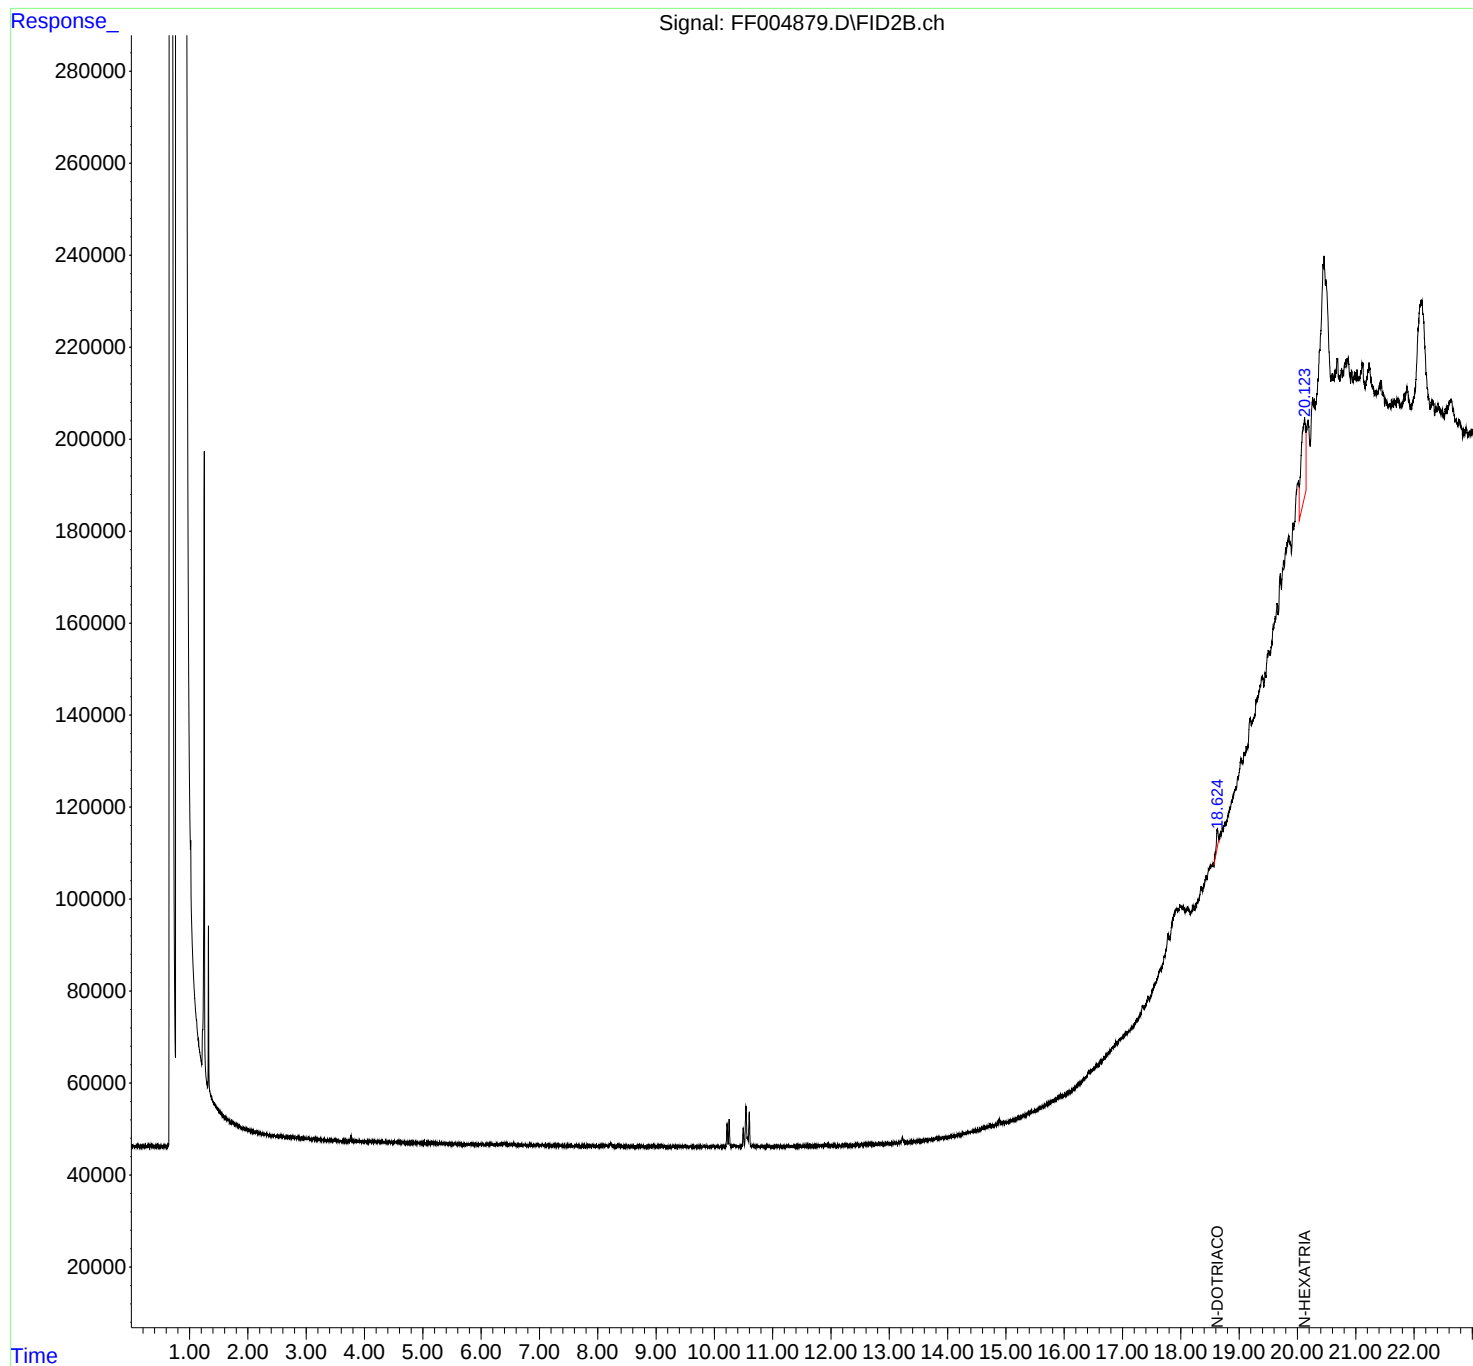


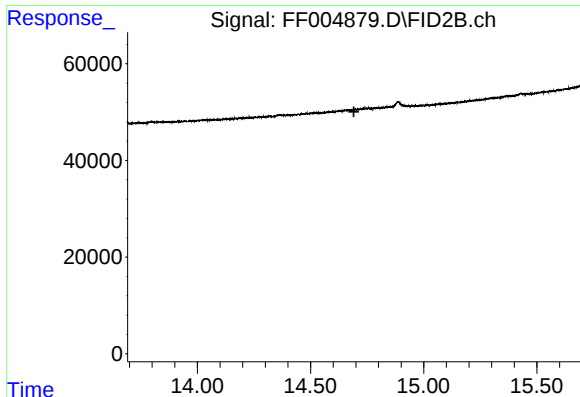

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 0.000 min
Exp R.T.: 14.692 min
Response: 0
Conc: N.D.

Instrument :
FID_F
ClientSampleId :
MECL2

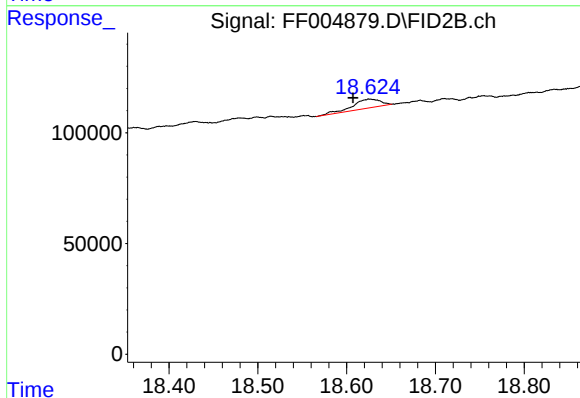

#14 N-DOTRIACONTANE

R.T.: 18.626 min
Delta R.T.: 0.019 min
Response: 87530
Conc: 0.77 ug/ml

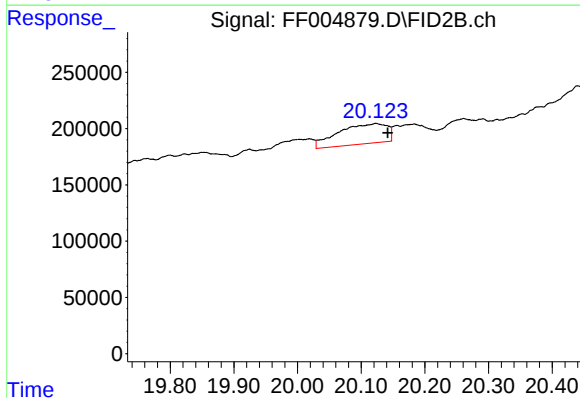

#16 N-HEXATRIACONTANE

R.T.: 20.123 min
Delta R.T.: -0.018 min
Response: 955421
Conc: 9.23 ug/ml