

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF070119\
 Data File : FF004882.D
 Signal(s) : FID2B.ch
 Acq On : 01 Jul 2019 10:29
 Operator : DD\AJ
 Sample : RT MARKER
 Misc :
 ALS Vial : 54 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :
 RT MARKER

Integration File: autoint1.e
 Quant Time: Jul 02 01:49:18 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF062619.M
 Quant Title :
 QLast Update : Wed Jun 26 14:27:24 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds

3)	N-DODECANE	6.431	6127870	48.296 ug/ml
12)	N-OCTACOSANE	16.891	5955567	53.394 ug/ml
13)	N-TRIACONTANE	17.783	250028	2.226 ug/ml
14)	N-DOTRIACONTANE	18.626	327051	2.872 ug/ml
15)	N-TETRATRIACONTANE	19.416	216845	1.998 ug/ml
16)	N-HEXATRIACONTANE	20.167	1184117	11.435 ug/ml
17)	N-OCTATRIACONTANE	20.927	1637487	17.168 ug/ml
18)	N-TETRACONTANE	21.869f	429778	3.697 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF070119\
Data File : FF004882.D
Signal(s) : FID2B.ch
Acq On : 01 Jul 2019 10:29
Operator : DD\AJ
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
RT MARKER

Integration File: autoint1.e
Quant Time: Jul 02 01:49:18 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF062619.M
Quant Title :
QLast Update : Wed Jun 26 14:27:24 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

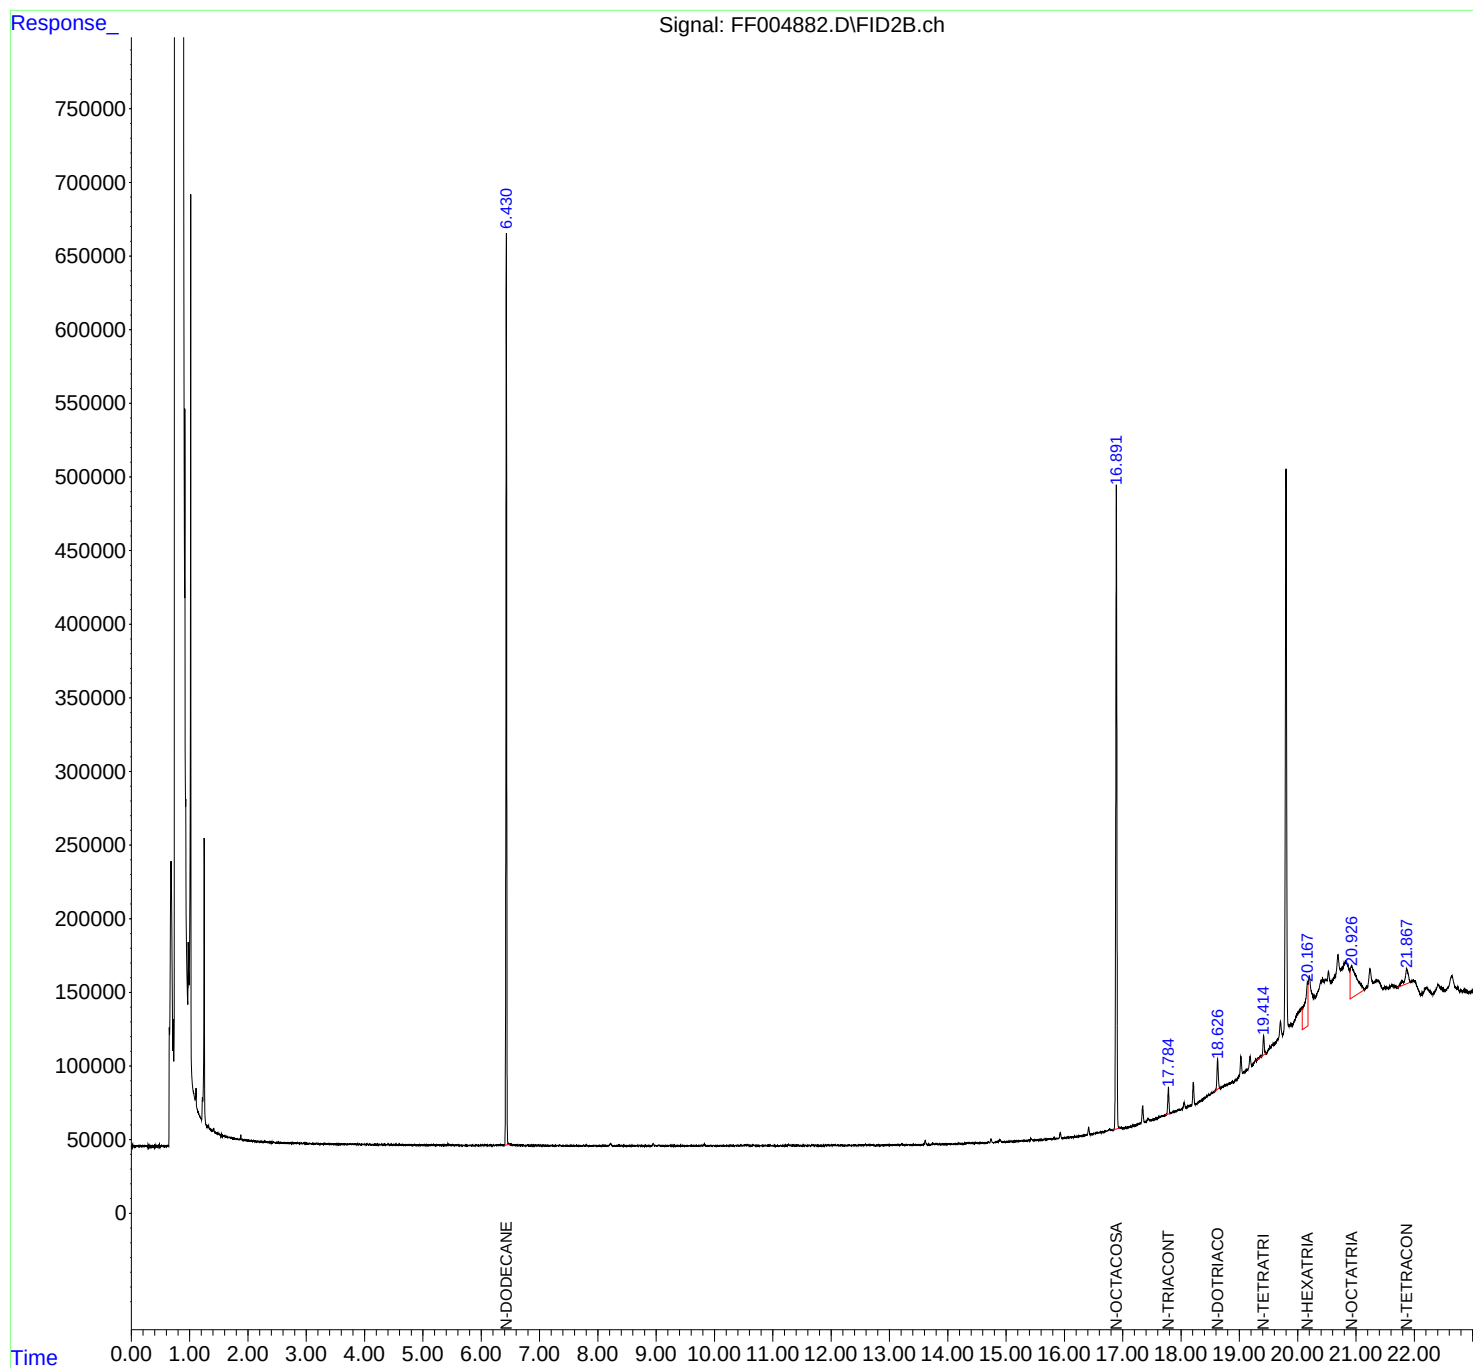


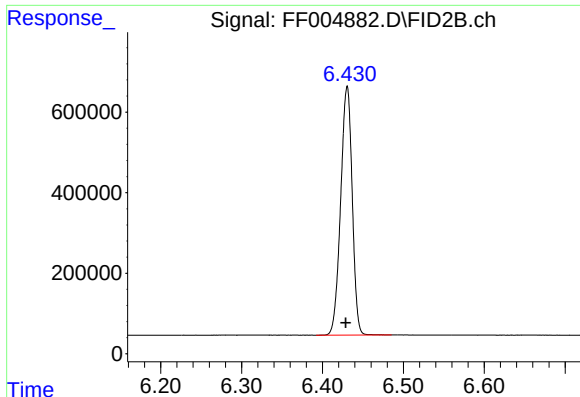

#3 N-DODECANE


R.T.: 6.431 min
Delta R.T.: 0.002 min
Response: 6127870
Conc: 48.30 ug/ml

Instrument :
FID_F
ClientSampleId :
RT MARKER

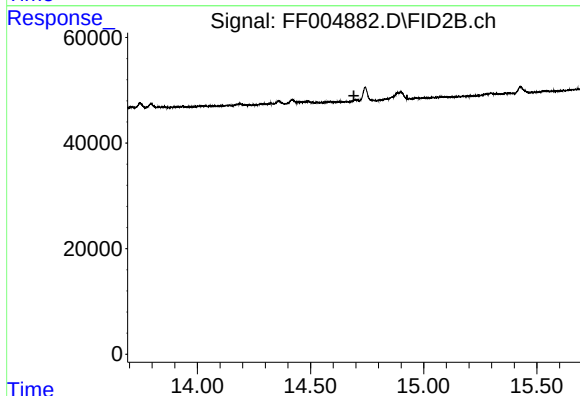


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.692 min
Response: 0
Conc: N.D.

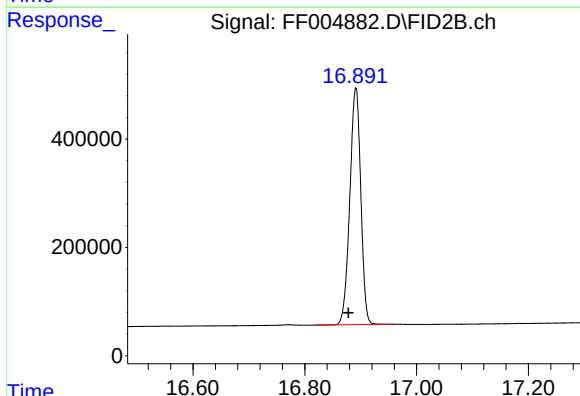


#12 N-OCTACOSANE

R.T.: 16.891 min
Delta R.T.: 0.014 min
Response: 5955567
Conc: 53.39 ug/ml

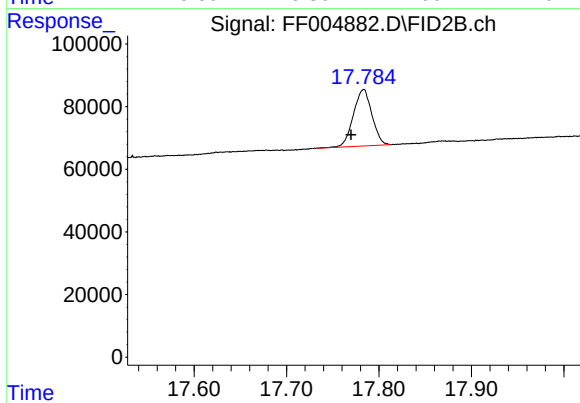

#13 N-TRIACONTANE


R.T.: 17.783 min
Delta R.T.: 0.014 min
Response: 250028
Conc: 2.23 ug/ml

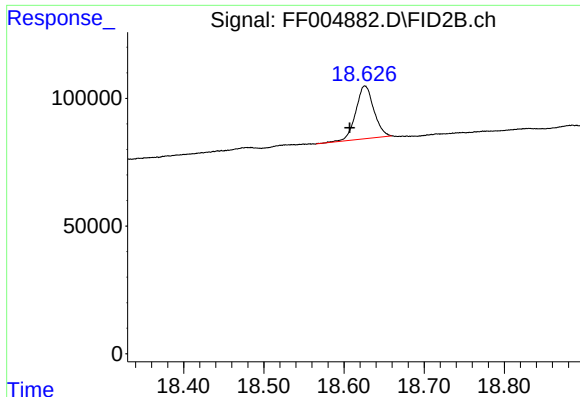

#14 N-DOTRIACONTANE


R.T.: 18.626 min
Delta R.T.: 0.019 min
Response: 327051
Conc: 2.87 ug/ml

Instrument :
FID_F
ClientSampleId :
RT MARKER

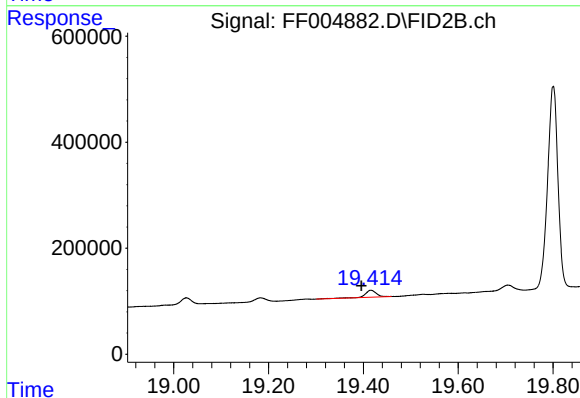


#15 N-TETRATRIACONTANE

R.T.: 19.416 min
Delta R.T.: 0.020 min
Response: 216845
Conc: 2.00 ug/ml

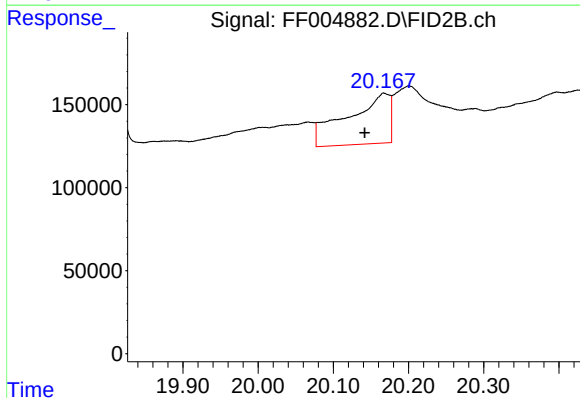


#16 N-HEXATRIACONTANE

R.T.: 20.167 min
Delta R.T.: 0.026 min
Response: 1184117
Conc: 11.44 ug/ml

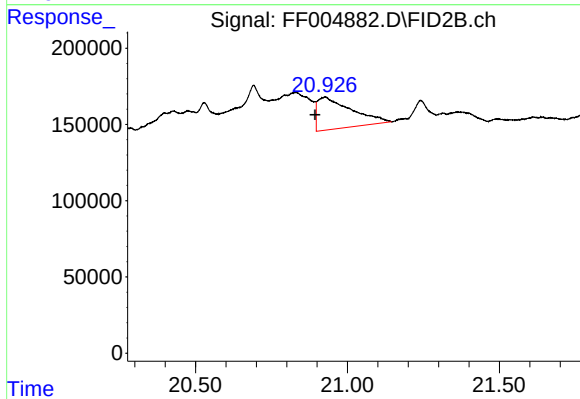

#17 N-OCTATRIACONTANE

R.T.: 20.927 min
Delta R.T.: 0.034 min
Response: 1637487
Conc: 17.17 ug/ml

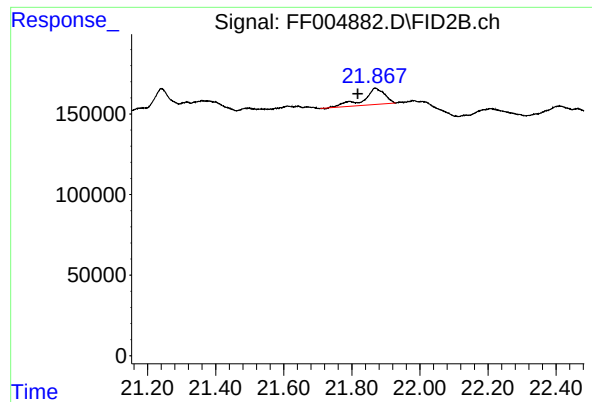

#18 N-TETRACONTANE

R.T.: 21.869 min
Delta R.T.: 0.051 min
Response: 429778
Conc: 3.70 ug/ml

Instrument :
FID_F
ClientSampleId :
RT MARKER