

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF070119\
 Data File : FF004894.D
 Signal(s) : FID2B.ch
 Acq On : 01 Jul 2019 20:35
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 52 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :
 I.BLK

Integration File: autoint1.e
 Quant Time: Jul 02 01:52:15 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF062619.M
 Quant Title :
 QLast Update : Wed Jun 26 14:27:24 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.693	2179467	22.409 ug/ml
Target Compounds			
14) N-DOTRIACONTANE	18.613	174759	1.534 ug/ml
16) N-HEXATRIACONTANE	20.151	17062	0.165 ug/ml
18) N-TETRACONTANE	21.862	267151	2.298 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF070119\
Data File : FF004894.D
Signal(s) : FID2B.ch
Acq On : 01 Jul 2019 20:35
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
I.BLK

Integration File: autoint1.e
Quant Time: Jul 02 01:52:15 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF062619.M
Quant Title :
QLast Update : Wed Jun 26 14:27:24 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

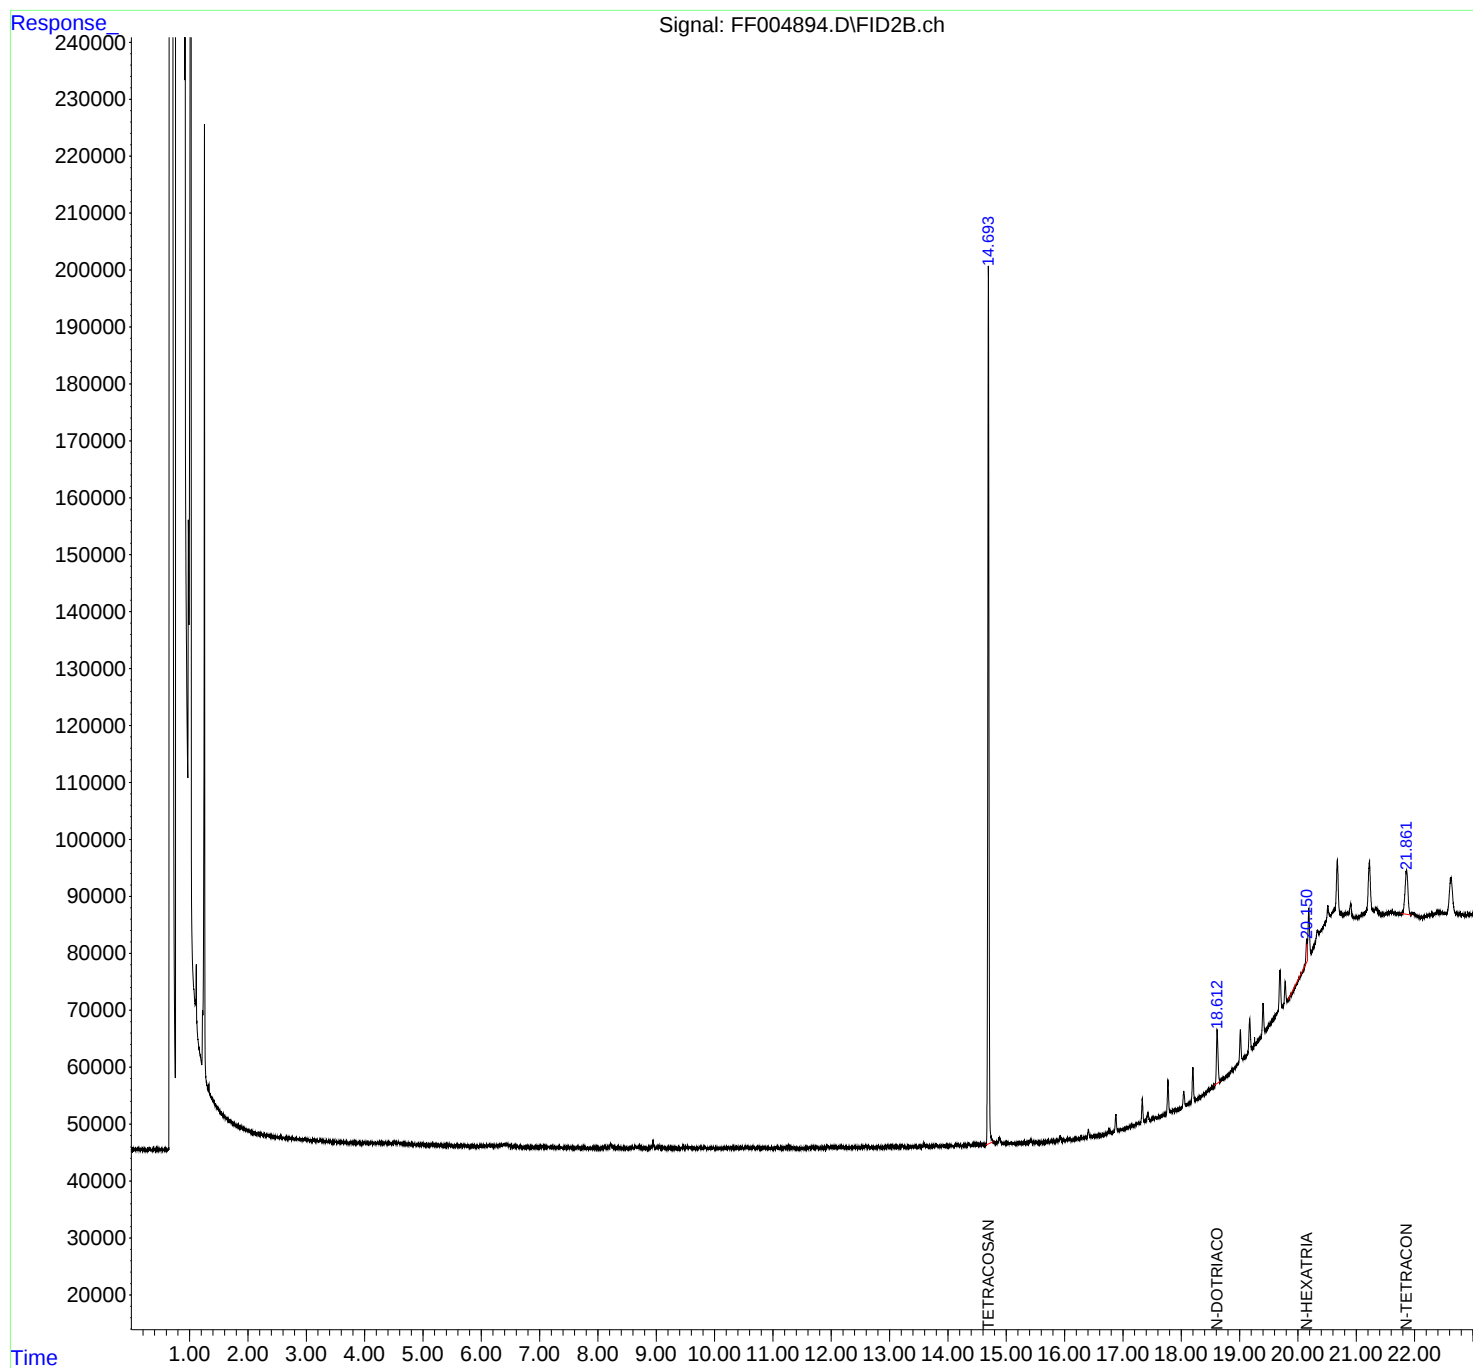


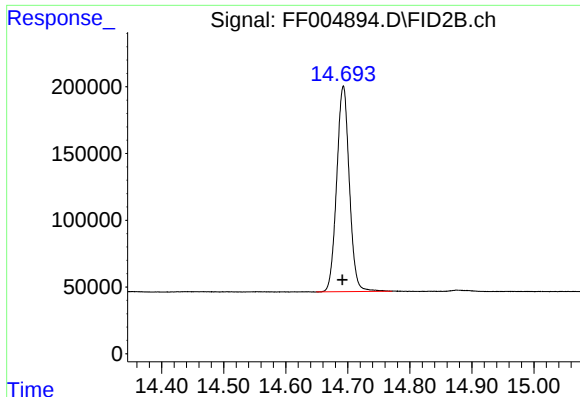

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.693 min
Delta R.T.: 0.001 min
Response: 2179467
Conc: 22.41 ug/ml

Instrument :
FID_F
ClientSampleId :
I.BLK

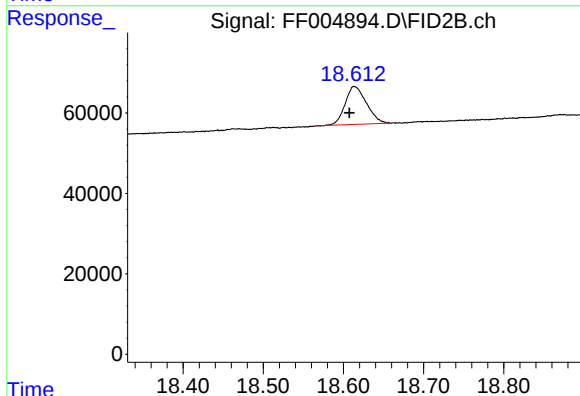


#14 N-DOTRIACONTANE

R.T.: 18.613 min
Delta R.T.: 0.006 min
Response: 174759
Conc: 1.53 ug/ml

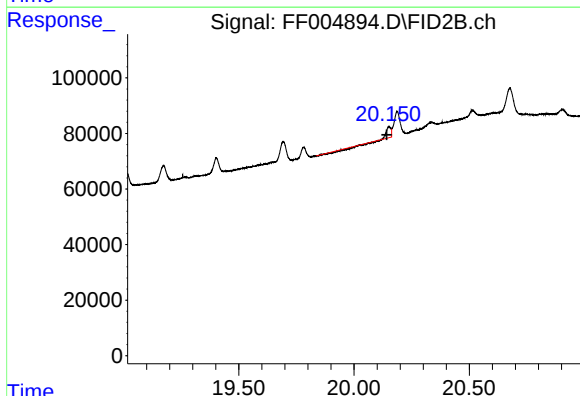

#16 N-HEXATRIACONTANE

R.T.: 20.151 min
Delta R.T.: 0.010 min
Response: 17062
Conc: 0.16 ug/ml

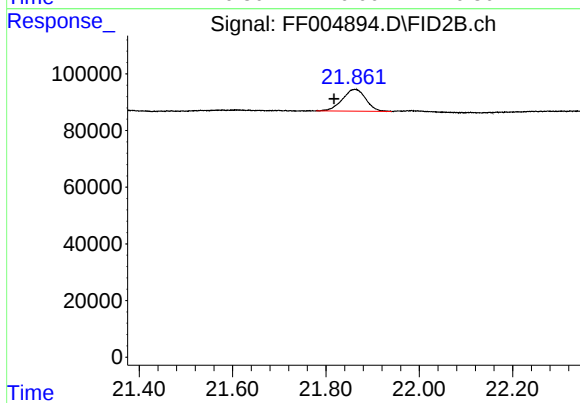

#18 N-TETRACONTANE

R.T.: 21.862 min
Delta R.T.: 0.045 min
Response: 267151
Conc: 2.30 ug/ml