

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF070119\
 Data File : FF004898.D
 Signal(s) : FID2B.ch
 Acq On : 01 Jul 2019 22:34
 Operator : DD\AJ
 Sample : K3569-02
 Misc :
 ALS Vial : 68 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :
 LT-8

Integration File: autoint1.e
 Quant Time: Jul 02 01:53:14 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF062619.M
 Quant Title :
 QLast Update : Wed Jun 26 14:27:24 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.691	2281874	23.462 ug/ml
Target Compounds			
4) N-TETRADECANE	8.280f	170881	1.366 ug/ml
8) N-DOCOSANE	13.786	129804	1.154 ug/ml
10) N-TETRACOSANE	14.894	429326	3.857 ug/ml
11) N-HEXACOSANE	15.920	669663	6.055 ug/ml
12) N-OCTACOSANE	16.876	882673	7.914 ug/ml
13) N-TRIACONTANE	17.769	806191	7.176 ug/ml
14) N-DOTRIACONTANE	18.608	525028	4.610 ug/ml
16) N-HEXATRIACONTANE	20.183	165375	1.597 ug/ml
18) N-TETRACONTANE	21.857	928903	7.991 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF070119\
Data File : FF004898.D
Signal(s) : FID2B.ch
Acq On : 01 Jul 2019 22:34
Operator : DD\AJ
Sample : K3569-02
Misc :
ALS Vial : 68 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
LT-8

Integration File: autoint1.e
Quant Time: Jul 02 01:53:14 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF062619.M
Quant Title :
QLast Update : Wed Jun 26 14:27:24 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

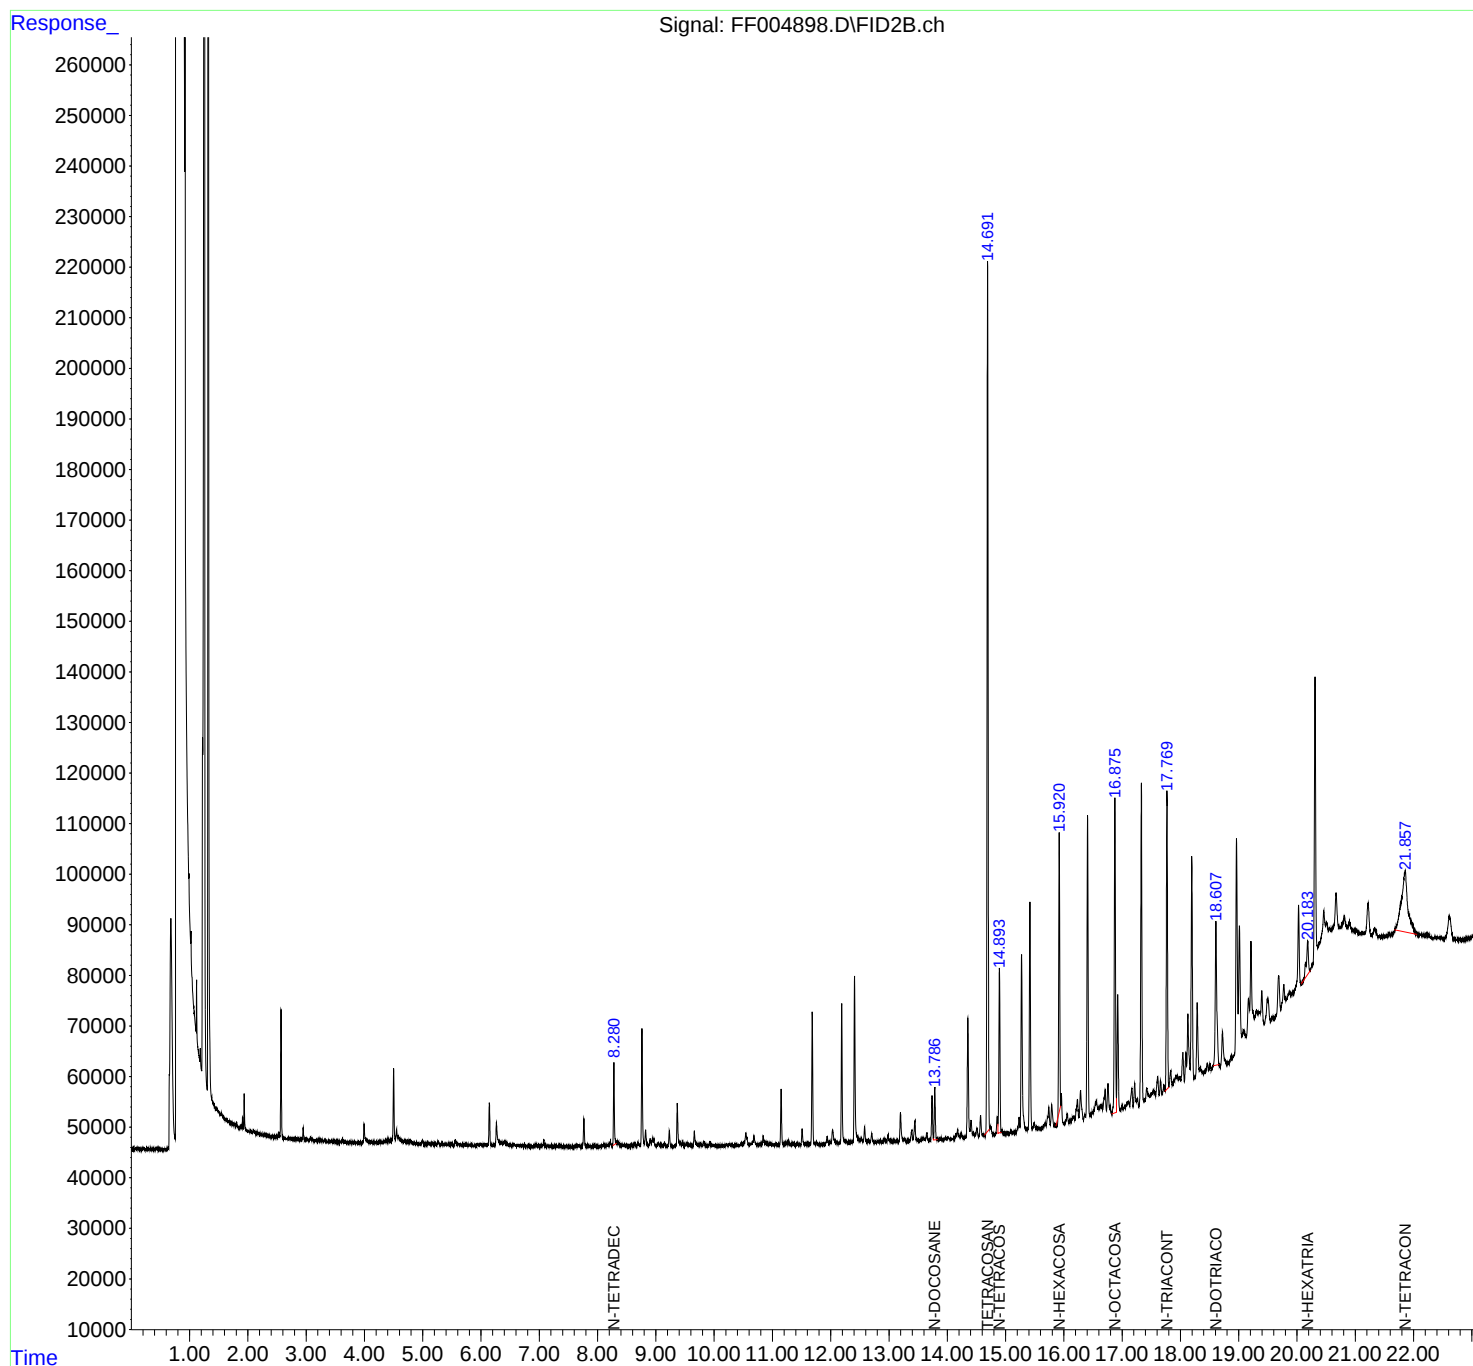


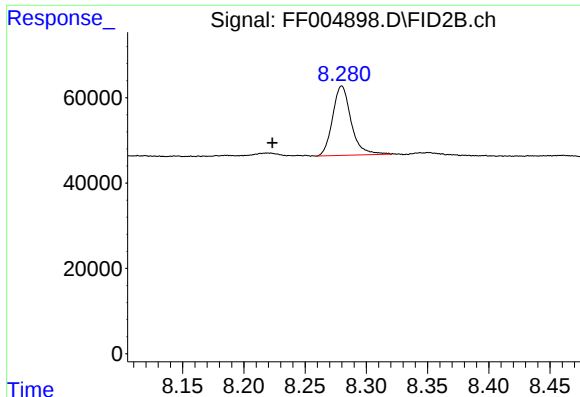

#4 N-TETRADECANE


R.T.: 8.280 min
Delta R.T.: 0.057 min
Response: 170881
Conc: 1.37 ug/ml

Instrument :
FID_F
ClientSampleId :
LT-8

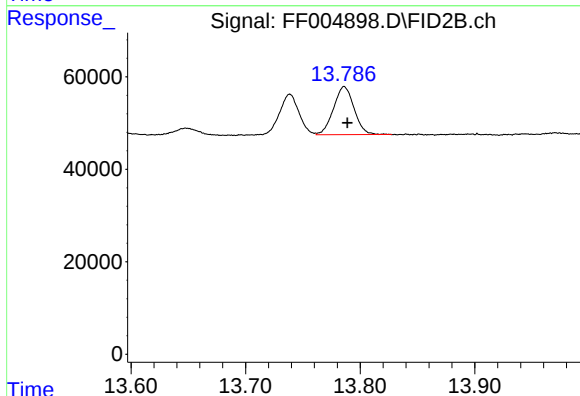


#8 N-DOCOSANE

R.T.: 13.786 min
Delta R.T.: -0.003 min
Response: 129804
Conc: 1.15 ug/ml

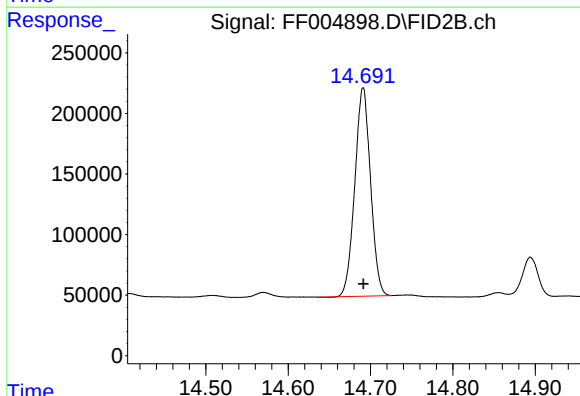


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.691 min
Delta R.T.: 0.000 min
Response: 2281874
Conc: 23.46 ug/ml

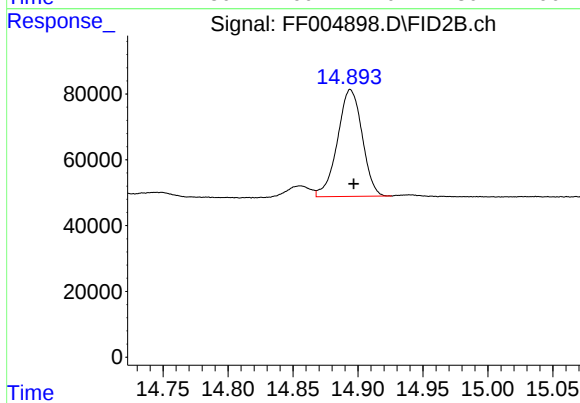

#10 N-TETRACOSANE


R.T.: 14.894 min
Delta R.T.: -0.002 min
Response: 429326
Conc: 3.86 ug/ml

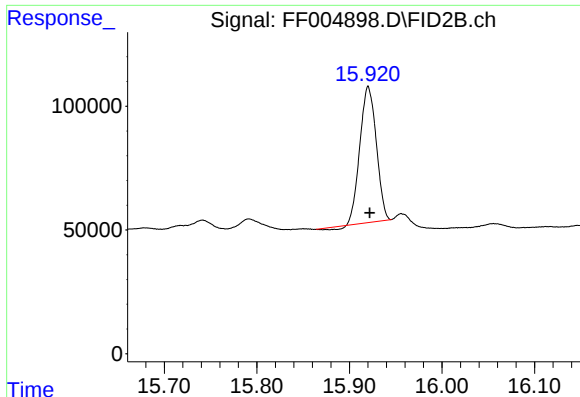

#11 N-HEXACOSANE


R.T.: 15.920 min
Delta R.T.: -0.002 min
Response: 669663
Conc: 6.05 ug/ml

Instrument :
FID_F
ClientSampleId :
LT-8

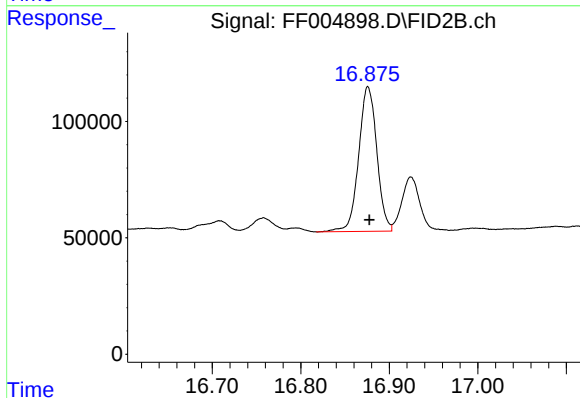


#12 N-OCTACOSANE

R.T.: 16.876 min
Delta R.T.: -0.002 min
Response: 882673
Conc: 7.91 ug/ml

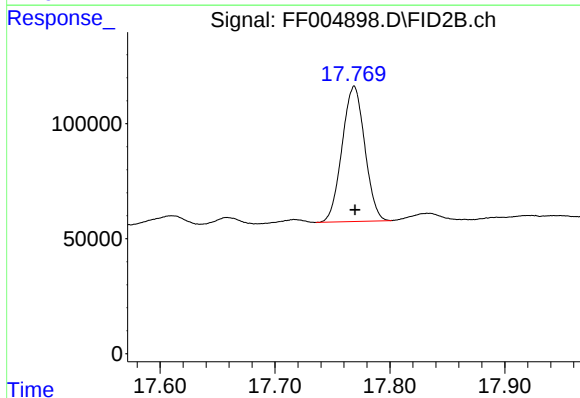


#13 N-TRIACONTANE

R.T.: 17.769 min
Delta R.T.: 0.000 min
Response: 806191
Conc: 7.18 ug/ml

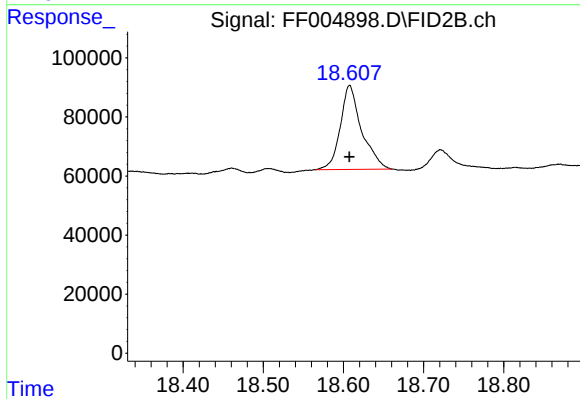

#14 N-DOTRIACONTANE


R.T.: 18.608 min
Delta R.T.: 0.000 min
Response: 525028
Conc: 4.61 ug/ml

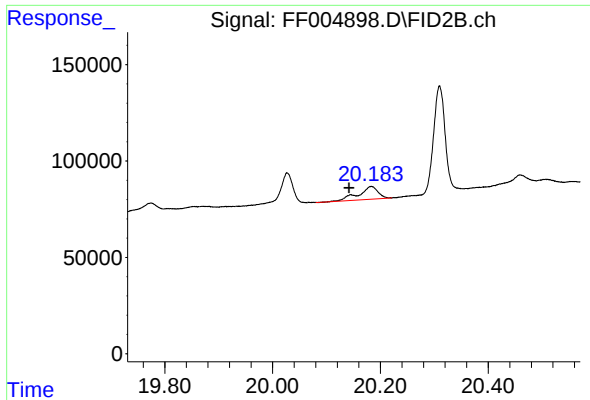

#16 N-HEXATRIACONTANE

R.T.: 20.183 min
Delta R.T.: 0.042 min
Response: 165375
Conc: 1.60 ug/ml

Instrument :
FID_F
ClientSampleId :
LT-8

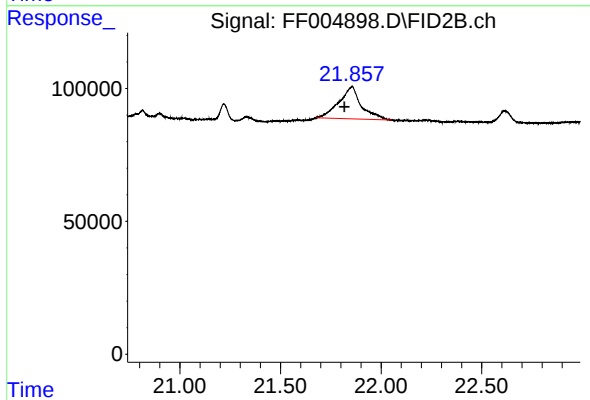

#18 N-TETRACONTANE

R.T.: 21.857 min
Delta R.T.: 0.039 min
Response: 928903
Conc: 7.99 ug/ml