

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF070119\
Data File : FF004903.D
Signal(s) : FID2B.ch
Acq On : 02 Jul 2019 01:02
Operator : DD\AJ
Sample : K3569-07
Misc :
ALS Vial : 73 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
LT-5

Integration File: autoint1.e
Quant Time: Jul 02 01:54:20 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF062619.M
Quant Title :
QLast Update : Wed Jun 26 14:27:24 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
9) S	TETRACOSANE-d50 (SURR...	14.690	2010092	20.667 ug/ml
Target Compounds				
11)	N-HEXACOSANE	15.956	89124	0.806 ug/ml
14)	N-DOTRIACONTANE	18.615	203189	1.784 ug/ml
16)	N-HEXATRIACONTANE	20.179	330269	3.189 ug/ml
18)	N-TETRACONTANE	21.851	368804	3.172 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF070119\
Data File : FF004903.D
Signal(s) : FID2B.ch
Acq On : 02 Jul 2019 01:02
Operator : DD\AJ
Sample : K3569-07
Misc :
ALS Vial : 73 Sample Multiplier: 1

Instrument :
FID_F
ClientSampled :
LT-5

Integration File: autoint1.e
Quant Time: Jul 02 01:54:20 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF062619.M
Quant Title :
QLast Update : Wed Jun 26 14:27:24 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

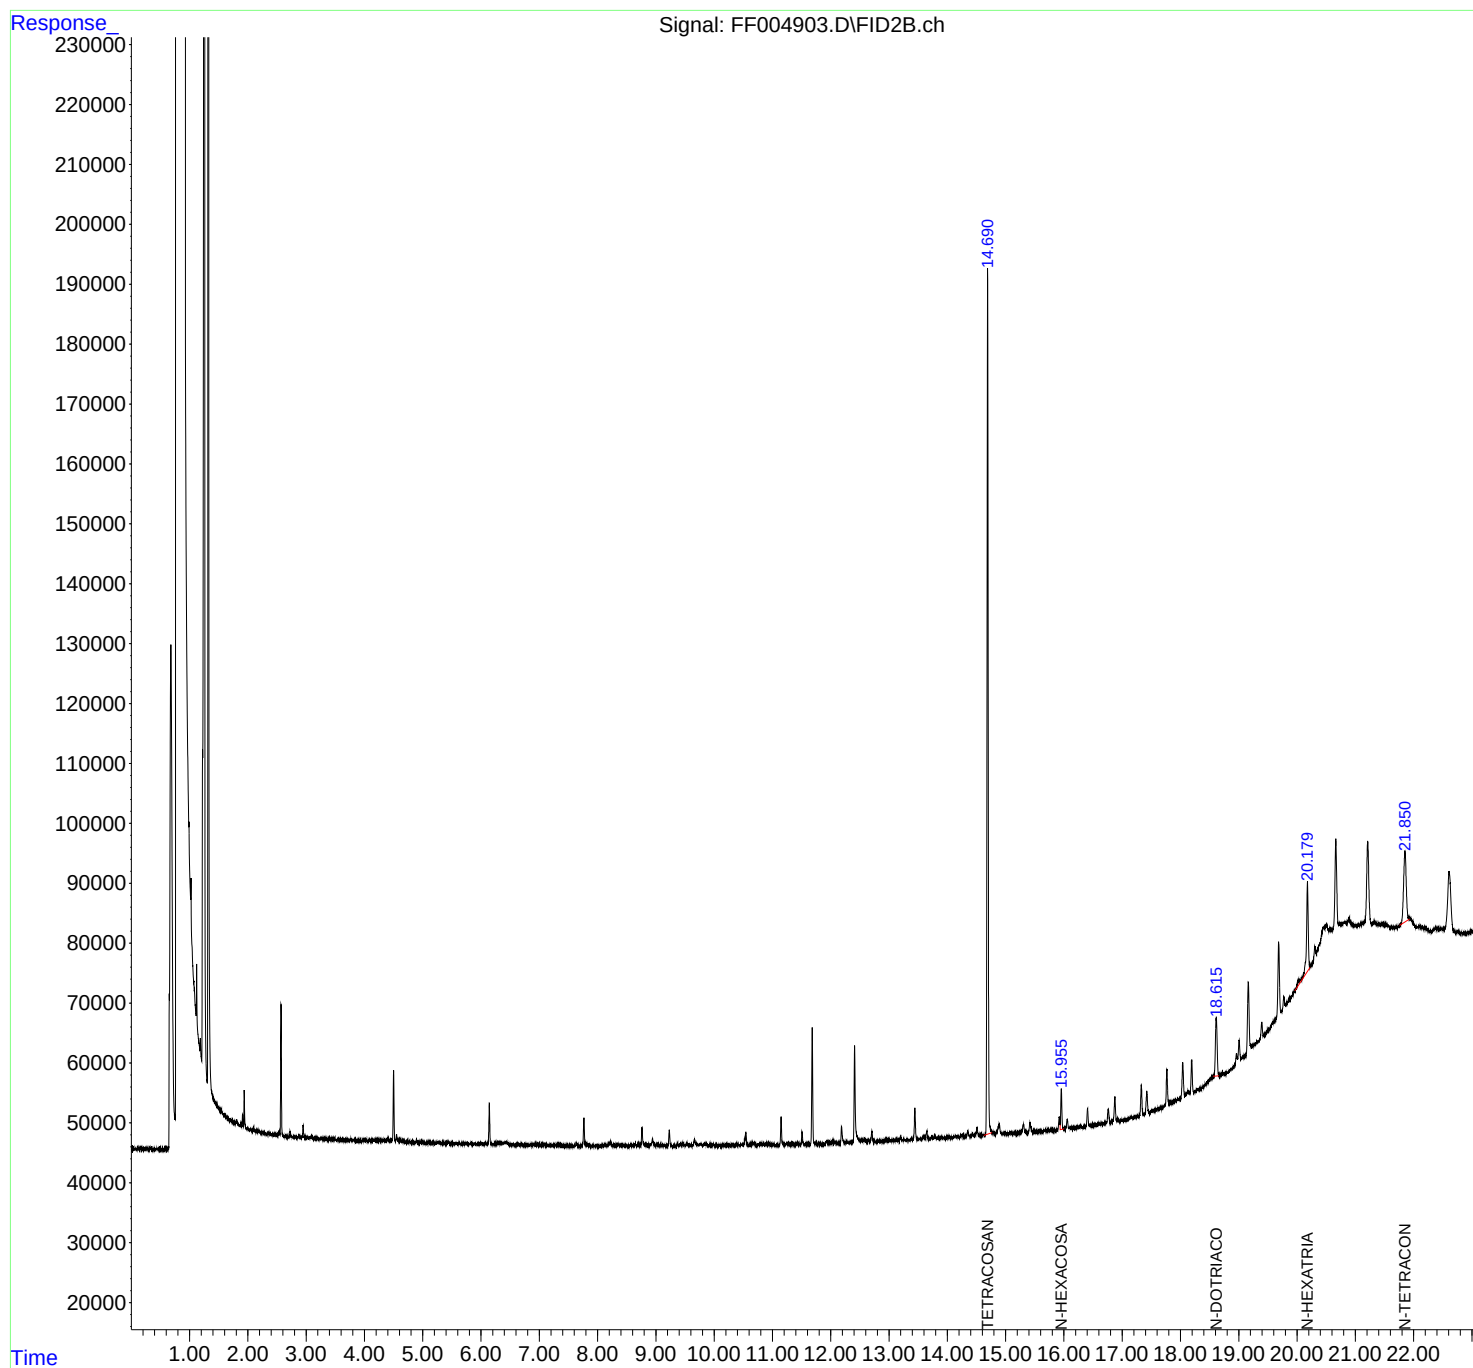


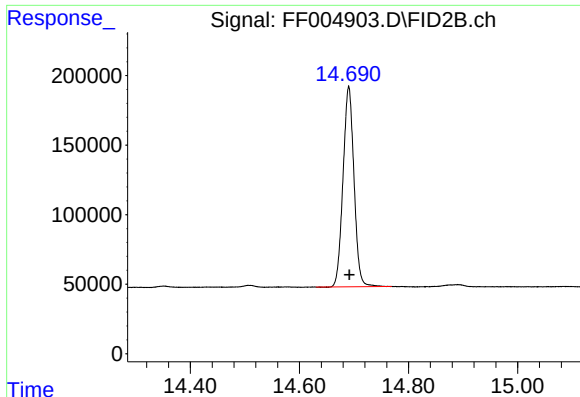

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.690 min
Delta R.T.: -0.001 min
Response: 2010092
Conc: 20.67 ug/ml

Instrument :
FID_F
ClientSampleId :
LT-5

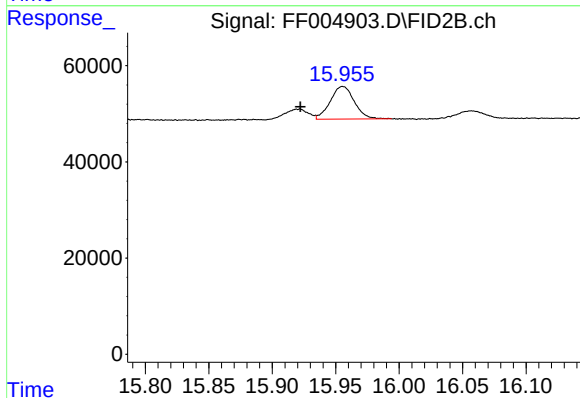


#11 N-HEXACOSANE

R.T.: 15.956 min
Delta R.T.: 0.034 min
Response: 89124
Conc: 0.81 ug/ml

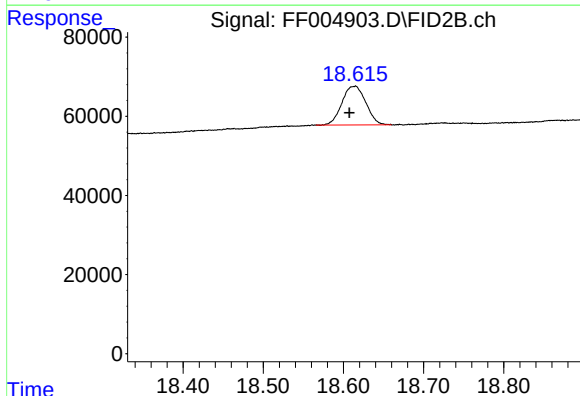


#14 N-DOTRIACONTANE

R.T.: 18.615 min
Delta R.T.: 0.007 min
Response: 203189
Conc: 1.78 ug/ml

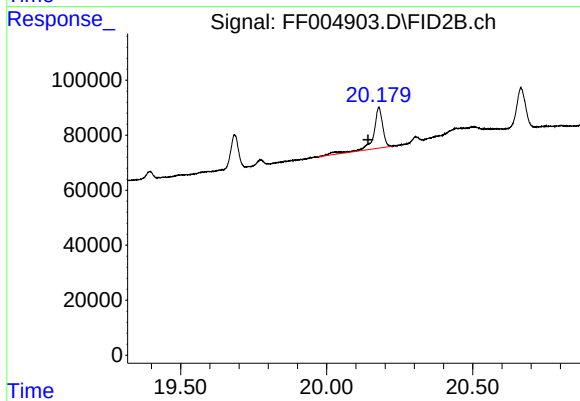

#16 N-HEXATRIACONTANE

R.T.: 20.179 min
Delta R.T.: 0.037 min
Response: 330269
Conc: 3.19 ug/ml

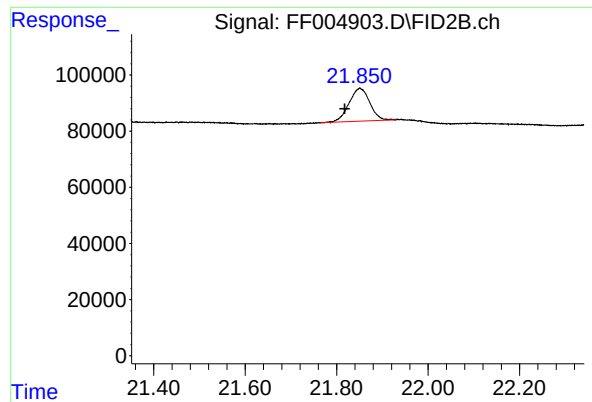

#18 N-TETRACONTANE

R.T.: 21.851 min
Delta R.T.: 0.033 min
Response: 368804
Conc: 3.17 ug/ml

Instrument :
FID_F
ClientSampleId :
LT-5