

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF070119\
 Data File : FF004909.D
 Signal(s) : FID2B.ch
 Acq On : 02 Jul 2019 03:59
 Operator : DD\AJ
 Sample : K3570-02
 Misc :
 ALS Vial : 79 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :
 ERM-16R

Integration File: autoint1.e
 Quant Time: Jul 02 08:18:42 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF062619.M
 Quant Title :
 QLast Update : Wed Jun 26 14:27:24 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.689	2123129	21.830 ug/ml
Target Compounds			
3) N-DODECANE	6.440	228691	1.802 ug/ml
4) N-TETRADECANE	8.197	267441	2.137 ug/ml
5) N-HEXADECANE	9.829	339118	2.746 ug/ml
11) N-HEXACOSANE	15.918	83231	0.753 ug/ml
12) N-OCTACOSANE	16.873	268734	2.409 ug/ml
13) N-TRIACONTANE	17.764	353931	3.151 ug/ml
14) N-DOTRIACONTANE	18.603	265212	2.329 ug/ml
16) N-HEXATRIACONTANE	20.178	152095	1.469 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF070119\
Data File : FF004909.D
Signal(s) : FID2B.ch
Acq On : 02 Jul 2019 03:59
Operator : DD\AJ
Sample : K3570-02
Misc :
ALS Vial : 79 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
ERM-16R

Integration File: autoint1.e
Quant Time: Jul 02 08:18:42 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF062619.M
Quant Title :
QLast Update : Wed Jun 26 14:27:24 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

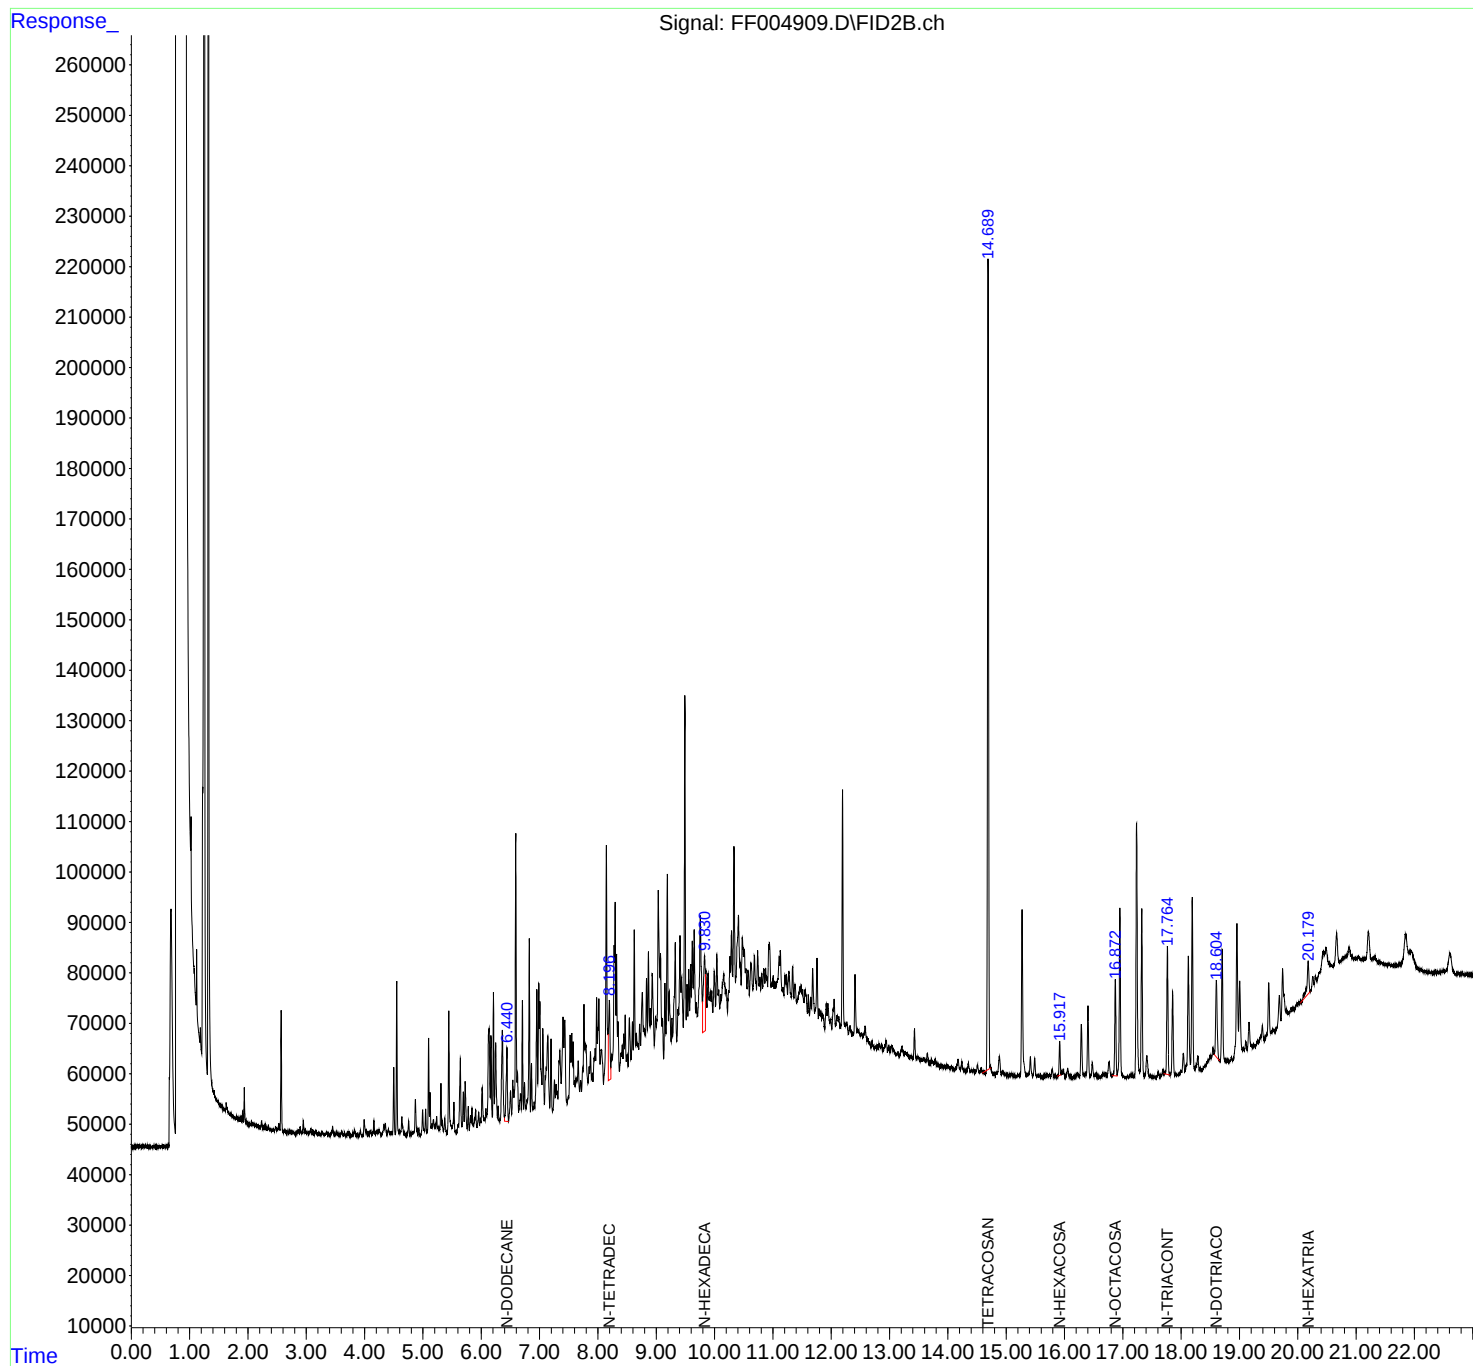


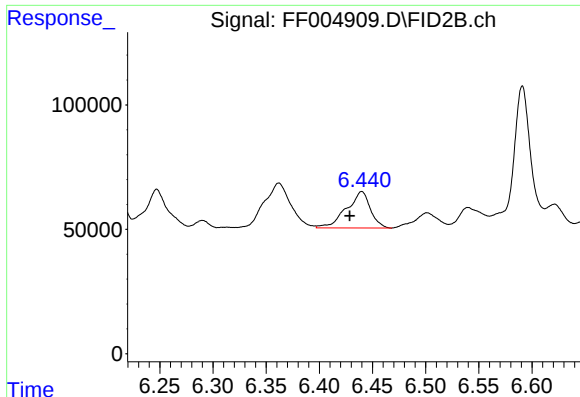

#3 N-DODECANE


R.T.: 6.440 min
Delta R.T.: 0.011 min
Response: 228691
Conc: 1.80 ug/ml

Instrument :
FID_F
ClientSampleId :
ERM-16R

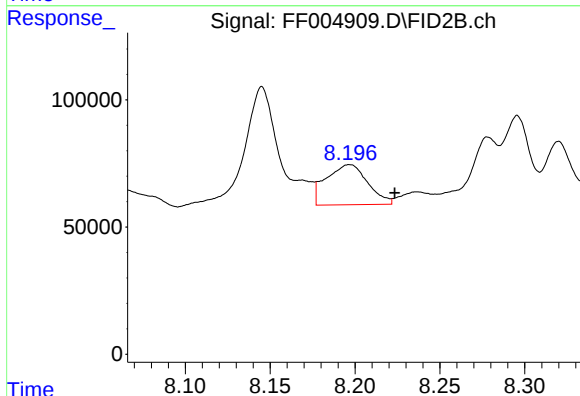


#4 N-TETRADECANE

R.T.: 8.197 min
Delta R.T.: -0.027 min
Response: 267441
Conc: 2.14 ug/ml

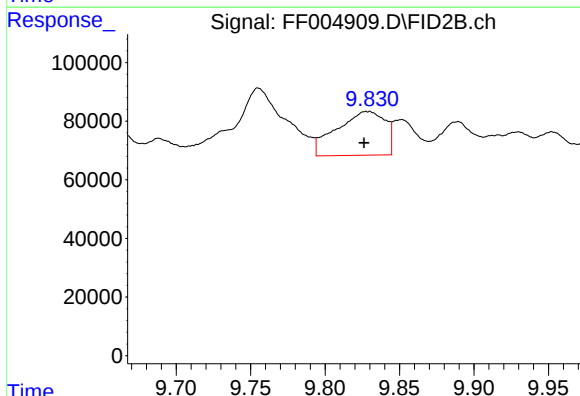


#5 N-HEXADECANE

R.T.: 9.829 min
Delta R.T.: 0.002 min
Response: 339118
Conc: 2.75 ug/ml

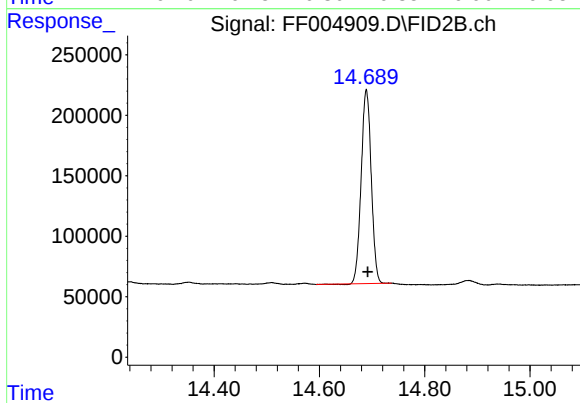

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.689 min
Delta R.T.: -0.002 min
Response: 2123129
Conc: 21.83 ug/ml

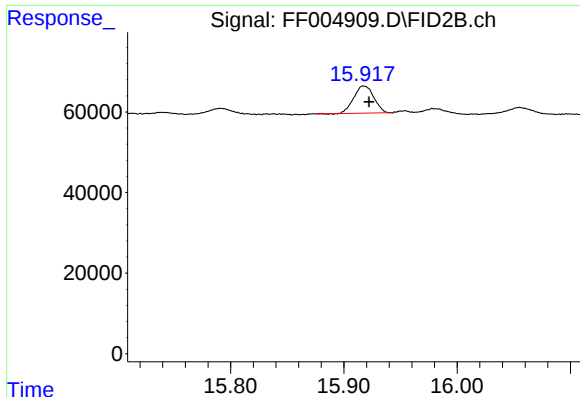

#11 N-HEXACOSANE


R.T.: 15.918 min
Delta R.T.: -0.004 min
Response: 83231
Conc: 0.75 ug/ml

Instrument :
FID_F
ClientSampleId :
ERM-16R

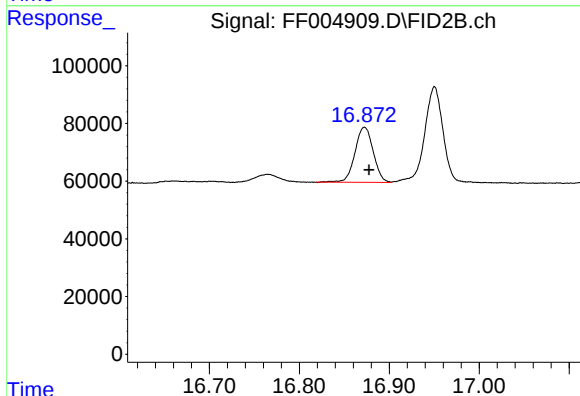


#12 N-OCTACOSANE

R.T.: 16.873 min
Delta R.T.: -0.005 min
Response: 268734
Conc: 2.41 ug/ml

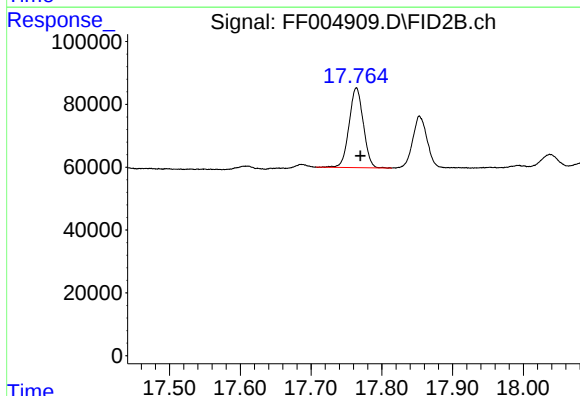


#13 N-TRIACONTANE

R.T.: 17.764 min
Delta R.T.: -0.006 min
Response: 353931
Conc: 3.15 ug/ml

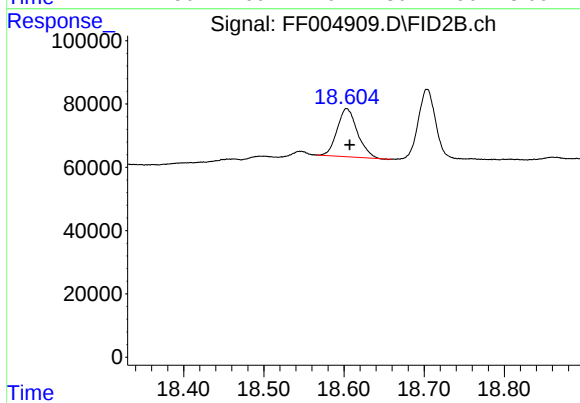

#14 N-DOTRIACONTANE

R.T.: 18.603 min
Delta R.T.: -0.004 min
Response: 265212
Conc: 2.33 ug/ml

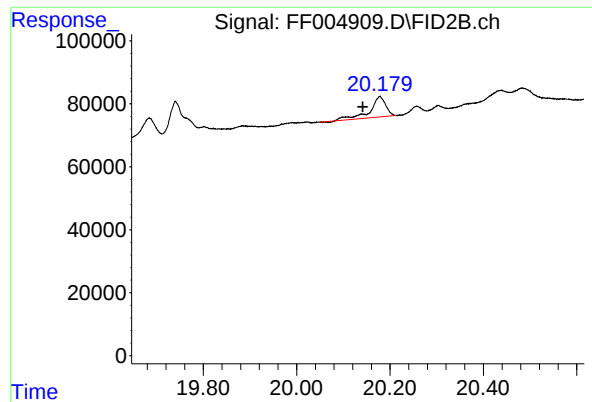

#16 N-HEXATRIACONTANE

R.T.: 20.178 min
Delta R.T.: 0.037 min
Response: 152095
Conc: 1.47 ug/ml

Instrument :
FID_F
ClientSampleId :
ERM-16R