

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF070119\
 Data File : FF004917.D
 Signal(s) : FID2B.ch
 Acq On : 02 Jul 2019 11:02
 Operator : DD\AJ
 Sample : K3569-01RE
 Misc :
 ALS Vial : 85 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :
 ERM-1RE

Integration File: autoint1.e
 Quant Time: Jul 02 14:43:01 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF062619.M
 Quant Title :
 QLast Update : Wed Jun 26 14:27:24 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
9) S	TETRACOSANE-d50 (SURR...	14.688	2712134	27.886 ug/ml
Target Compounds				
4)	N-TETRADECANE	8.277f	89957	0.719 ug/ml
8)	N-DOCOSANE	13.782	168369	1.496 ug/ml
10)	N-TETRACOSANE	14.890	529589	4.758 ug/ml
11)	N-HEXACOSANE	15.917	910648	8.233 ug/ml
12)	N-OCTACOSANE	16.874	993237	8.905 ug/ml
13)	N-TRIACONTANE	17.767	885259	7.880 ug/ml
14)	N-DOTRIACONTANE	18.607	585270	5.139 ug/ml
15)	N-TETRATRIACONTANE	19.399	156436	1.441 ug/ml
16)	N-HEXATRIACONTANE	20.148	72444	0.700 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF070119\
Data File : FF004917.D
Signal(s) : FID2B.ch
Acq On : 02 Jul 2019 11:02
Operator : DD\AJ
Sample : K3569-01RE
Misc :
ALS Vial : 85 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
ERM-1RE

Integration File: autoint1.e
Quant Time: Jul 02 14:43:01 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF062619.M
Quant Title :
QLast Update : Wed Jun 26 14:27:24 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

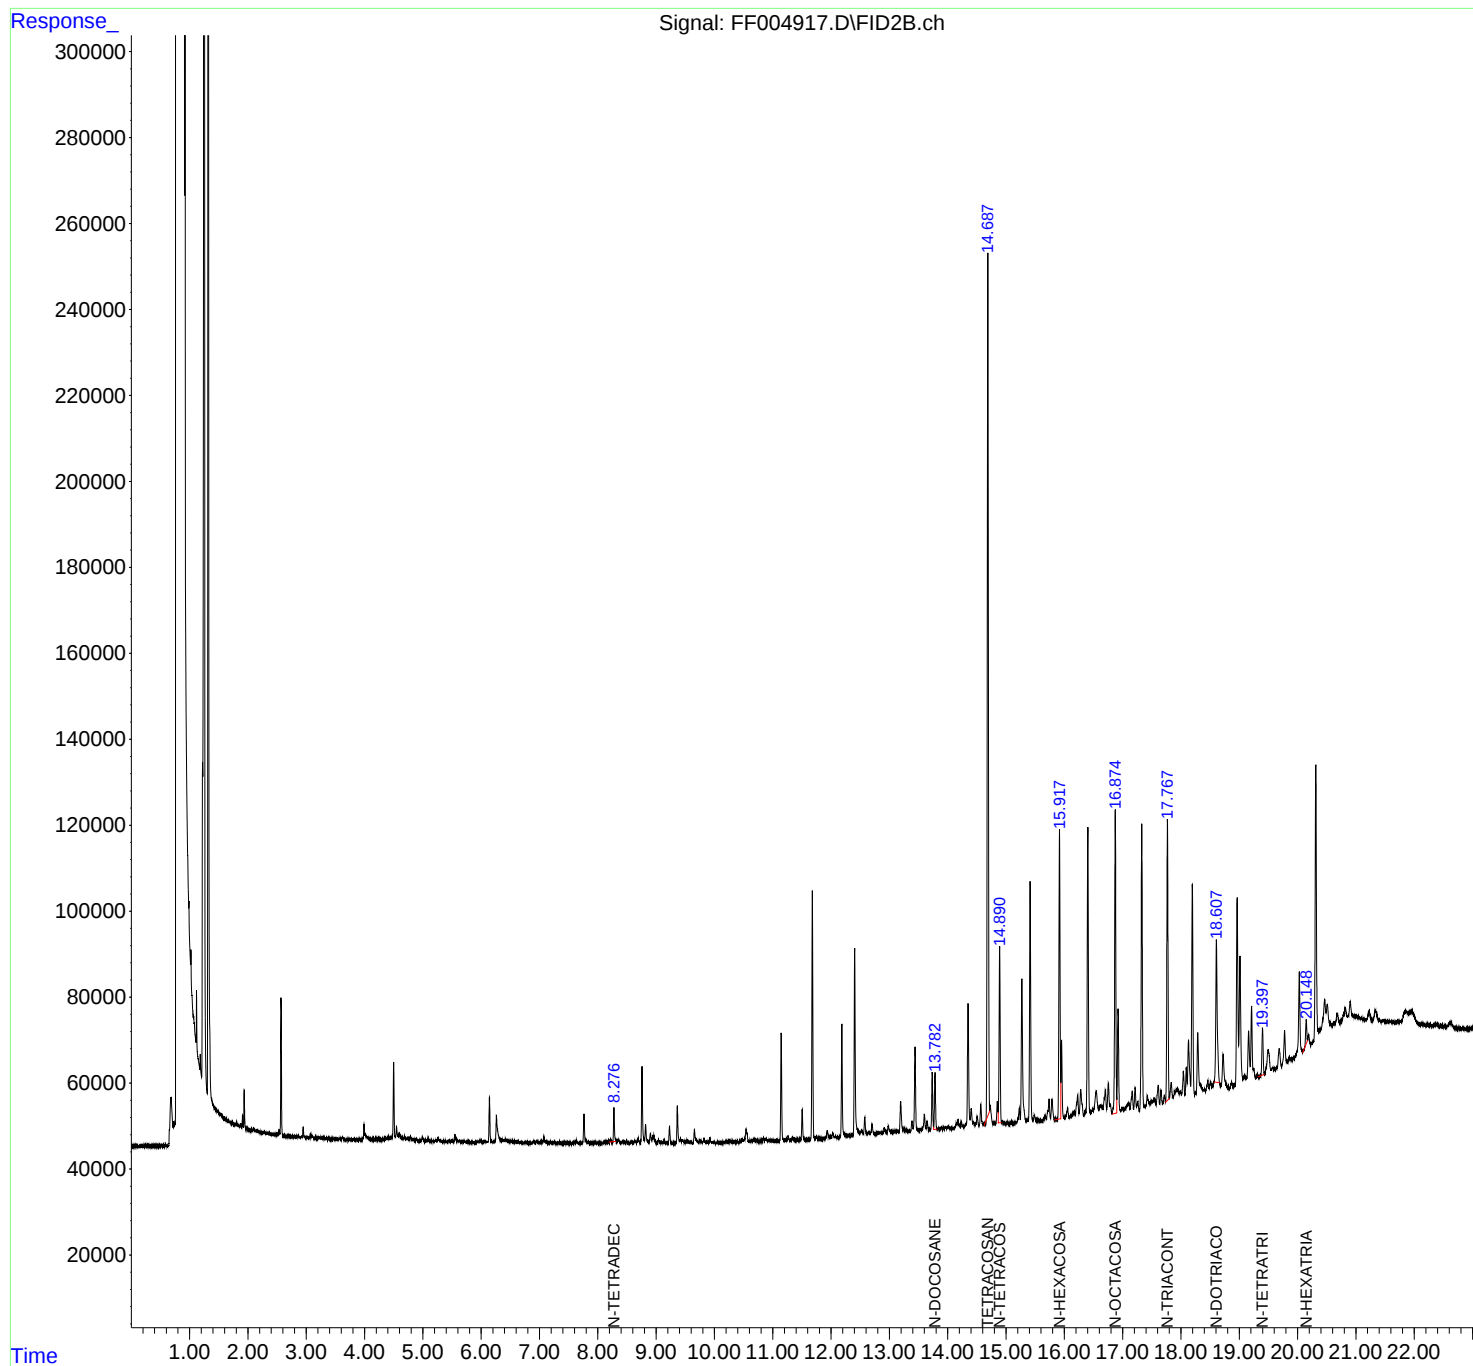


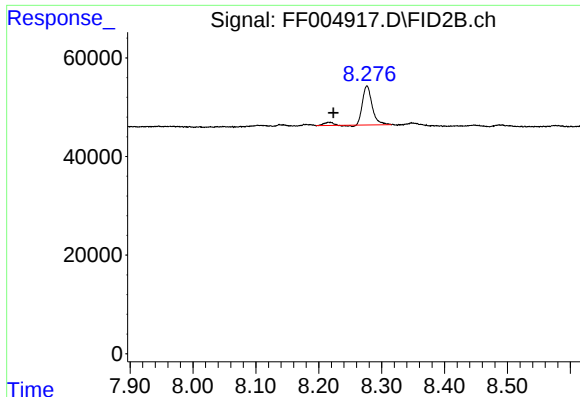

#4 N-TETRADECANE


R.T.: 8.277 min
Delta R.T.: 0.053 min
Response: 89957
Conc: 0.72 ug/ml

Instrument :
FID_F
ClientSampleId :
ERM-1RE

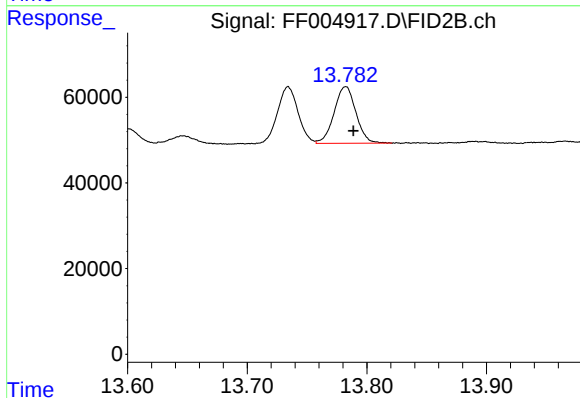


#8 N-DOCOSANE

R.T.: 13.782 min
Delta R.T.: -0.006 min
Response: 168369
Conc: 1.50 ug/ml

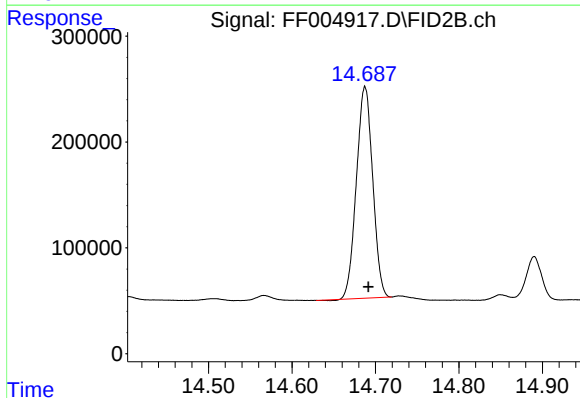


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.688 min
Delta R.T.: -0.004 min
Response: 2712134
Conc: 27.89 ug/ml

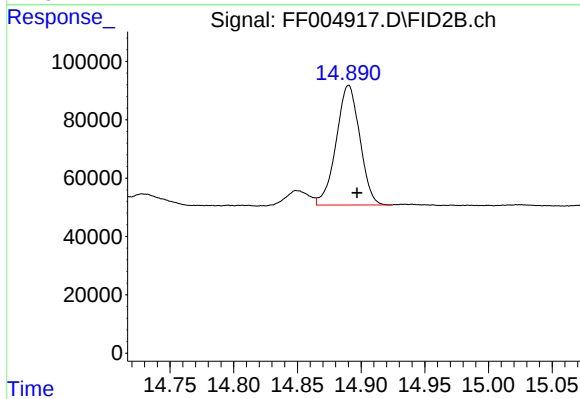

#10 N-TETRACOSANE


R.T.: 14.890 min
Delta R.T.: -0.006 min
Response: 529589
Conc: 4.76 ug/ml

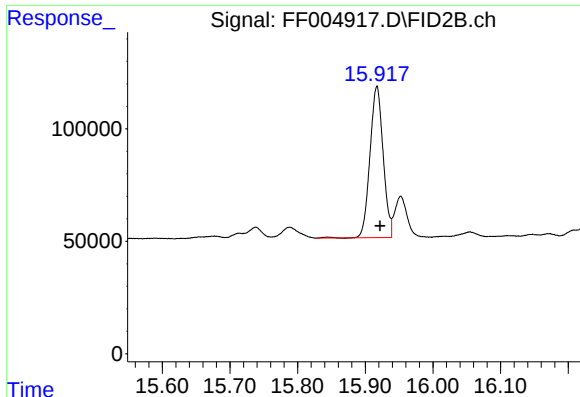

#11 N-HEXACOSANE


R.T.: 15.917 min
Delta R.T.: -0.005 min
Response: 910648
Conc: 8.23 ug/ml

Instrument :
FID_F
ClientSampleId :
ERM-1RE

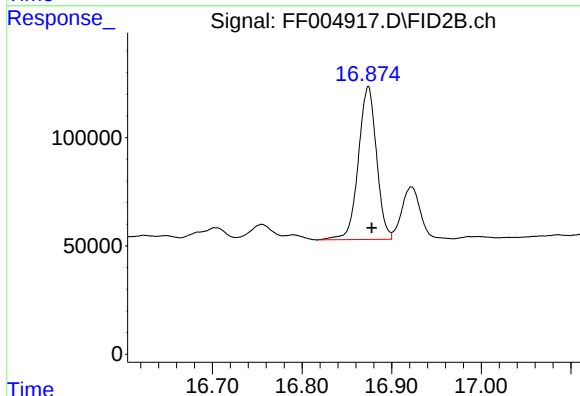


#12 N-OCTACOSANE

R.T.: 16.874 min
Delta R.T.: -0.004 min
Response: 993237
Conc: 8.90 ug/ml

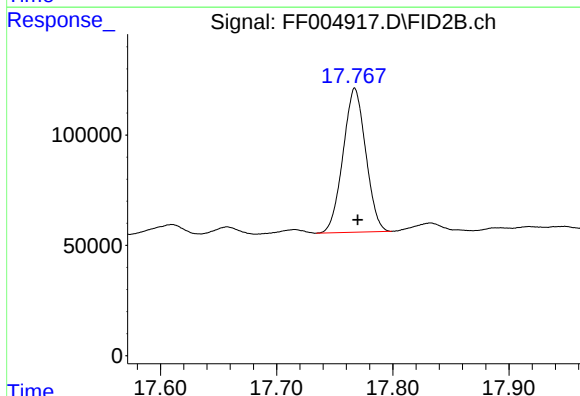


#13 N-TRIACONTANE

R.T.: 17.767 min
Delta R.T.: -0.002 min
Response: 885259
Conc: 7.88 ug/ml

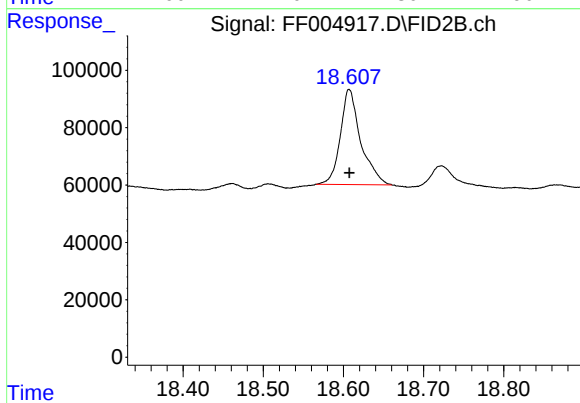

#14 N-DOTRIACONTANE


R.T.: 18.607 min
Delta R.T.: 0.000 min
Response: 585270
Conc: 5.14 ug/ml

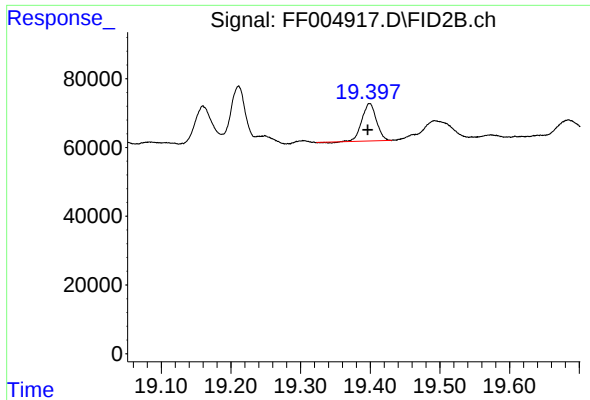

#15 N-TETRATRIACONTANE

R.T.: 19.399 min
Delta R.T.: 0.003 min
Response: 156436
Conc: 1.44 ug/ml

Instrument :
FID_F
ClientSampleId :
ERM-1RE

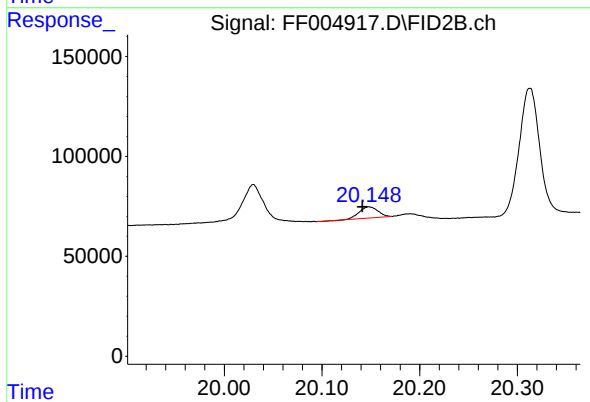

#16 N-HEXATRIACONTANE

R.T.: 20.148 min
Delta R.T.: 0.007 min
Response: 72444
Conc: 0.70 ug/ml