

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF070119\
 Data File : FF004919.D
 Signal(s) : FID2B.ch
 Acq On : 02 Jul 2019 12:04
 Operator : DD\AJ
 Sample : K3570-01 2X
 Misc :
 ALS Vial : 87 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :
 PW-2R

Integration File: autoint1.e
 Quant Time: Jul 02 14:43:10 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF062619.M
 Quant Title :
 QLast Update : Wed Jun 26 14:27:24 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.686	1057742	10.876 ug/ml
Target Compounds			
3) N-DODECANE	6.437	205346	1.618 ug/ml
4) N-TETRADECANE	8.197	207307	1.657 ug/ml
5) N-HEXADECANE	9.829	429076	3.475 ug/ml
7) N-EICOSANE	12.636f	456245	3.932 ug/ml
12) N-OCTACOSANE	16.874	145818	1.307 ug/ml
13) N-TRIACONTANE	17.768	211451	1.882 ug/ml
14) N-DOTRIACONTANE	18.611	201570	1.770 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF070119\
Data File : FF004919.D
Signal(s) : FID2B.ch
Acq On : 02 Jul 2019 12:04
Operator : DD\AJ
Sample : K3570-01 2X
Misc :
ALS Vial : 87 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
PW-2R

Integration File: autoint1.e
Quant Time: Jul 02 14:43:10 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF062619.M
Quant Title :
QLast Update : Wed Jun 26 14:27:24 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

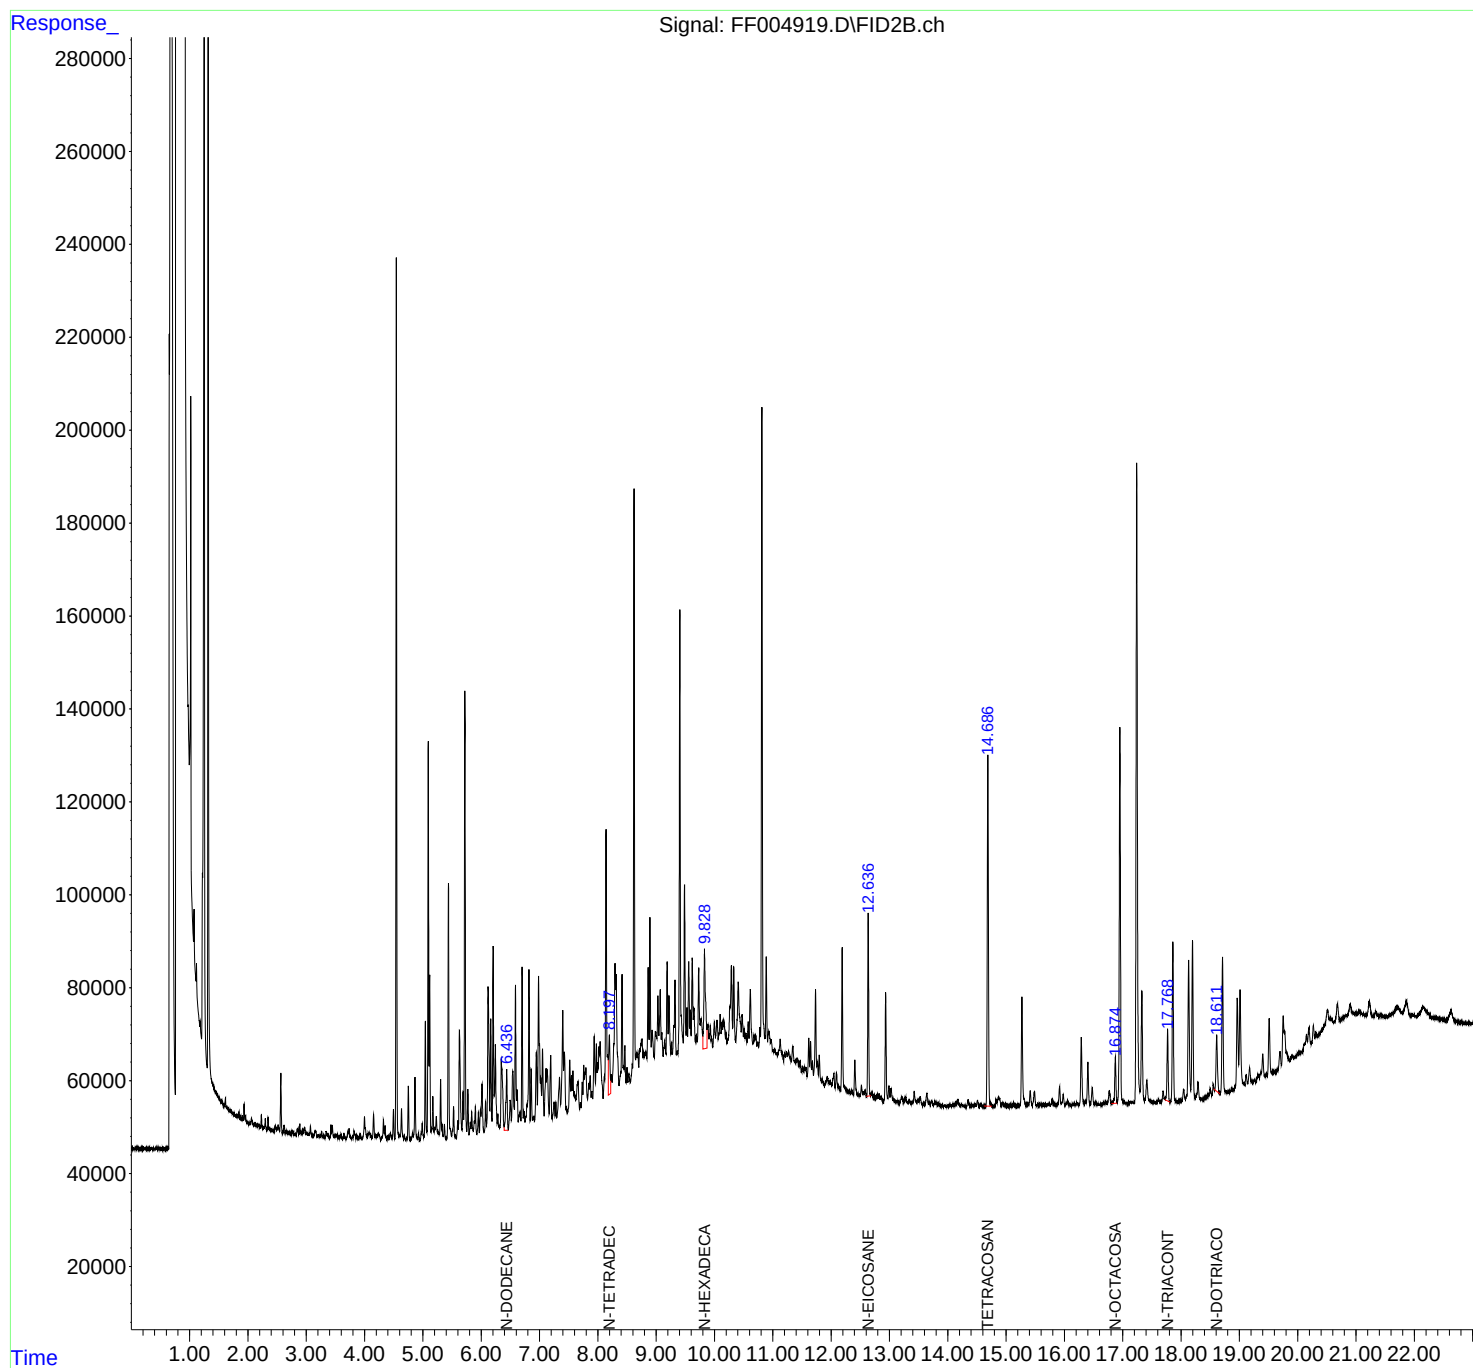


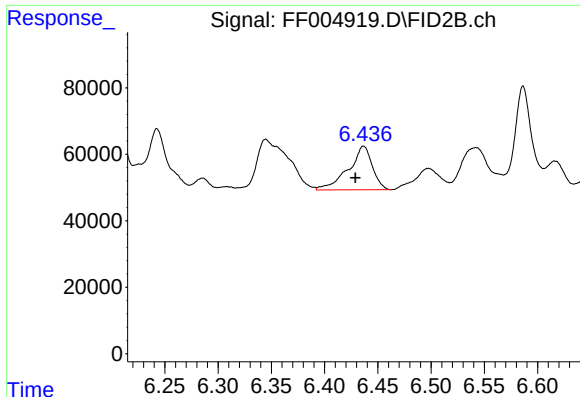

#3 N-DODECANE


R.T.: 6.437 min
Delta R.T.: 0.008 min
Response: 205346
Conc: 1.62 ug/ml

Instrument :
FID_F
ClientSampleId :
PW-2R

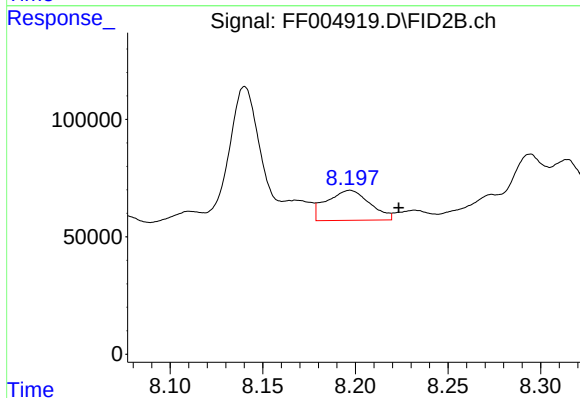


#4 N-TETRADECANE

R.T.: 8.197 min
Delta R.T.: -0.026 min
Response: 207307
Conc: 1.66 ug/ml

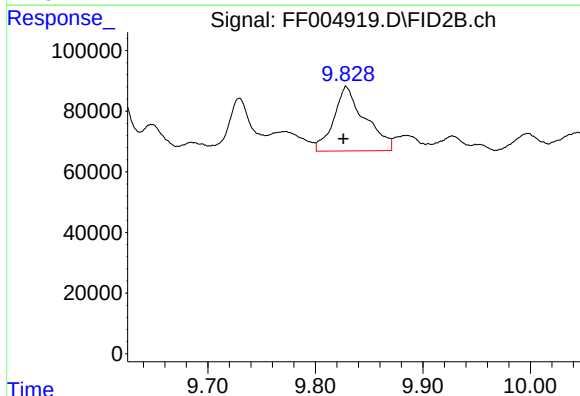


#5 N-HEXADECANE

R.T.: 9.829 min
Delta R.T.: 0.003 min
Response: 429076
Conc: 3.47 ug/ml

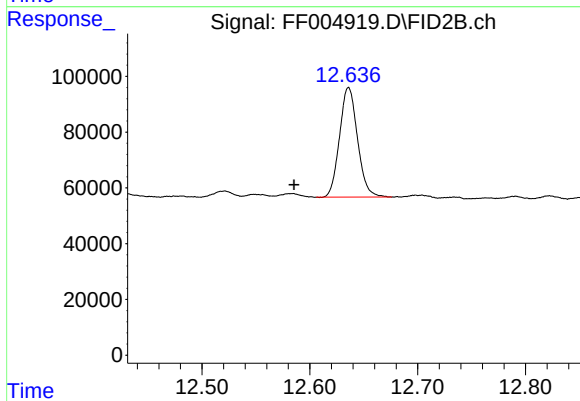

#7 N-EICOSANE


R.T.: 12.636 min
Delta R.T.: 0.050 min
Response: 456245
Conc: 3.93 ug/ml

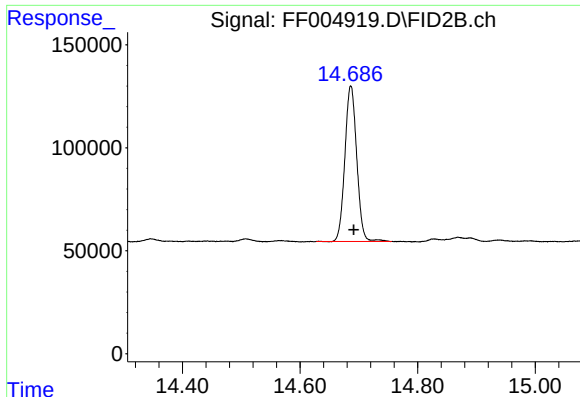

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.686 min
Delta R.T.: -0.005 min
Response: 1057742
Conc: 10.88 ug/ml

Instrument :
FID_F
ClientSampleId :
PW-2R

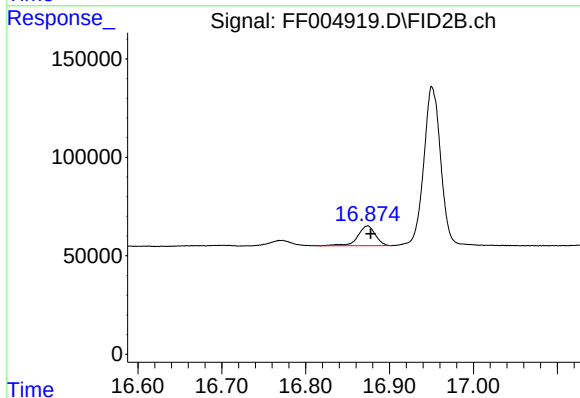


#12 N-OCTACOSANE

R.T.: 16.874 min
Delta R.T.: -0.004 min
Response: 145818
Conc: 1.31 ug/ml

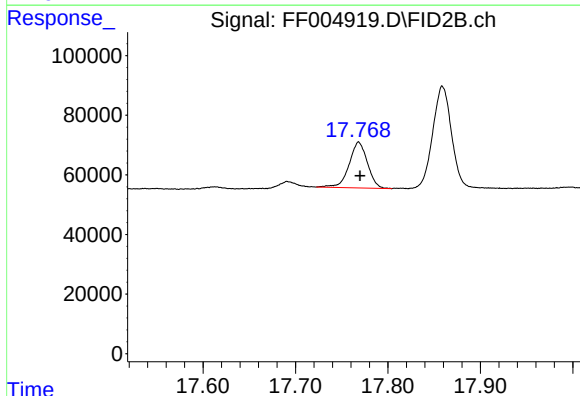

#13 N-TRIACONTANE

R.T.: 17.768 min
Delta R.T.: -0.001 min
Response: 211451
Conc: 1.88 ug/ml

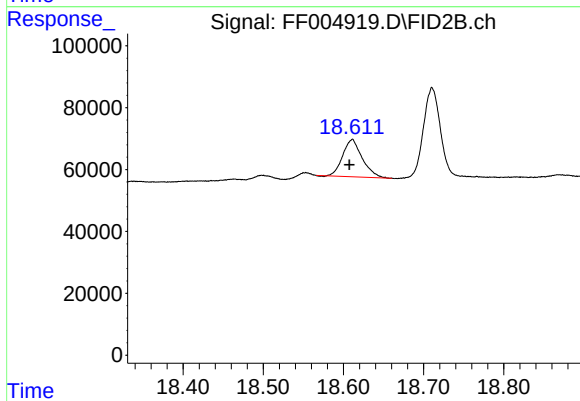

#14 N-DOTRIACONTANE

R.T.: 18.611 min
Delta R.T.: 0.004 min
Response: 201570
Conc: 1.77 ug/ml