

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF070119\
 Data File : FF004920.D
 Signal(s) : FID2B.ch
 Acq On : 02 Jul 2019 12:34
 Operator : DD\AJ
 Sample : K3570-02 2X
 Misc :
 ALS Vial : 88 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :
 ERM-16R

Integration File: autoint1.e
 Quant Time: Jul 02 14:43:15 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF062619.M
 Quant Title :
 QLast Update : Wed Jun 26 14:27:24 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.686	1066005	10.961 ug/ml
Target Compounds			
3) N-DODECANE	6.438	114058	0.899 ug/ml
4) N-TETRADECANE	8.195	125115	1.000 ug/ml
12) N-OCTACOSANE	16.872	168657	1.512 ug/ml
13) N-TRIACONTANE	17.767	266090	2.369 ug/ml
14) N-DOTRIACONTANE	18.607	219748	1.929 ug/ml
15) N-TETRATRIACONTANE	19.398	99264	0.915 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF070119\
Data File : FF004920.D
Signal(s) : FID2B.ch
Acq On : 02 Jul 2019 12:34
Operator : DD\AJ
Sample : K3570-02 2X
Misc :
ALS Vial : 88 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
ERM-16R

Integration File: autoint1.e
Quant Time: Jul 02 14:43:15 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF062619.M
Quant Title :
QLast Update : Wed Jun 26 14:27:24 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

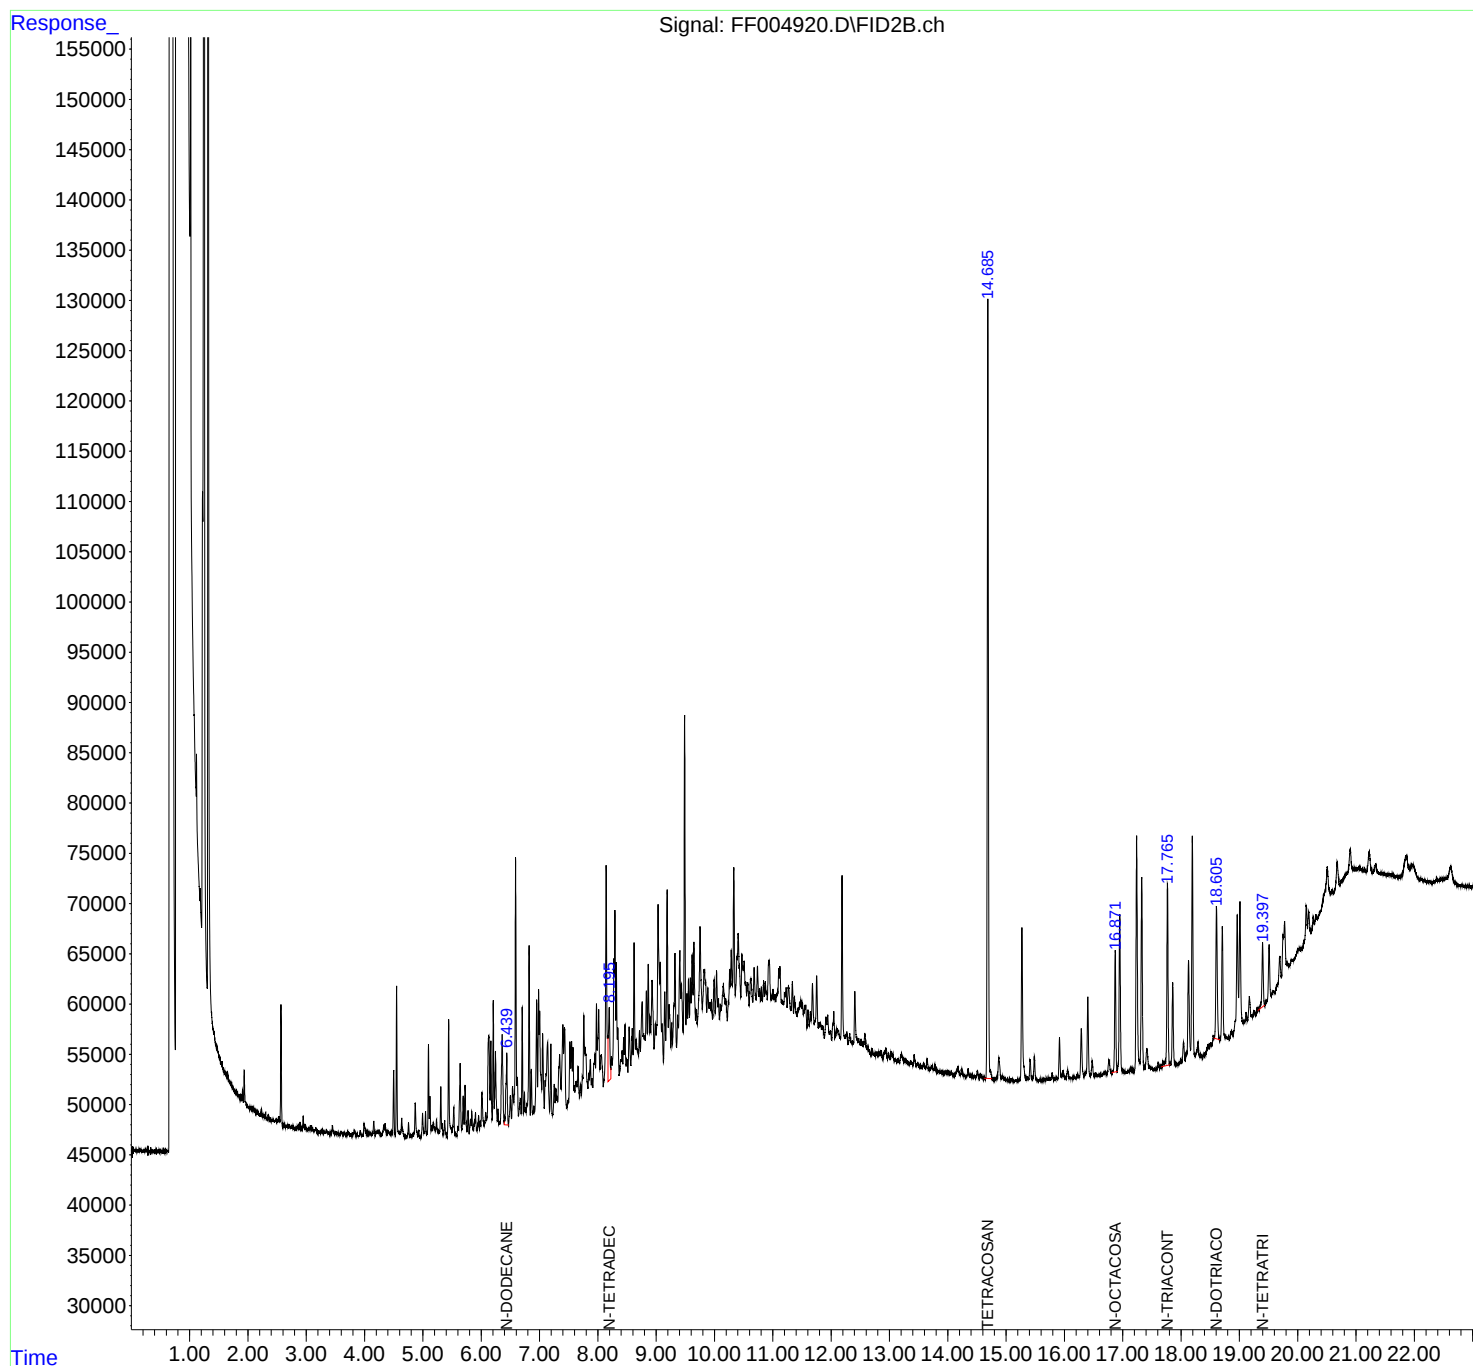


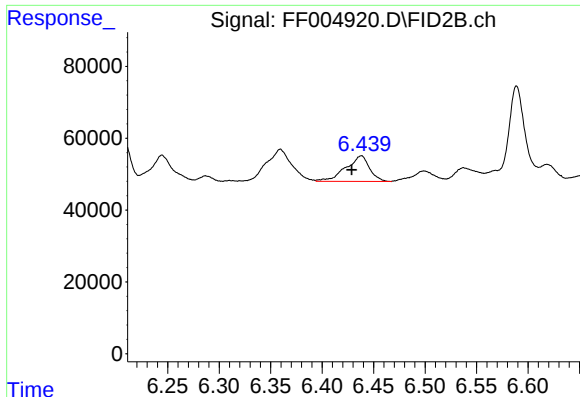

#3 N-DODECANE


R.T.: 6.438 min
Delta R.T.: 0.009 min
Response: 114058
Conc: 0.90 ug/ml

Instrument :
FID_F
ClientSampleId :
ERM-16R

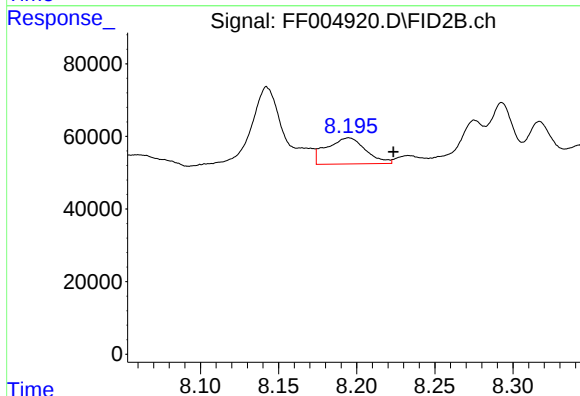


#4 N-TETRADECANE

R.T.: 8.195 min
Delta R.T.: -0.028 min
Response: 125115
Conc: 1.00 ug/ml

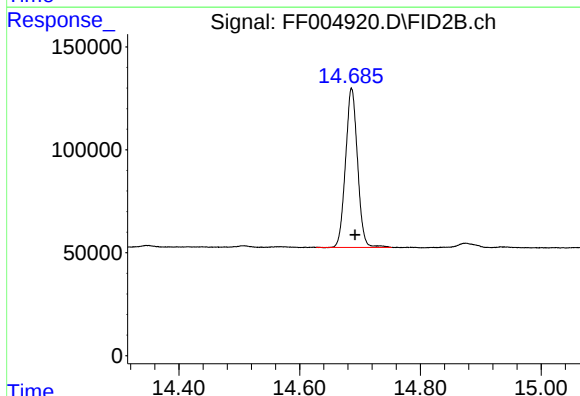


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.686 min
Delta R.T.: -0.005 min
Response: 1066005
Conc: 10.96 ug/ml

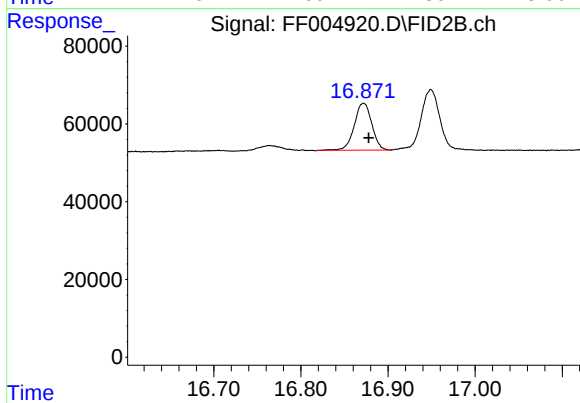

#12 N-OCTACOSANE


R.T.: 16.872 min
Delta R.T.: -0.006 min
Response: 168657
Conc: 1.51 ug/ml

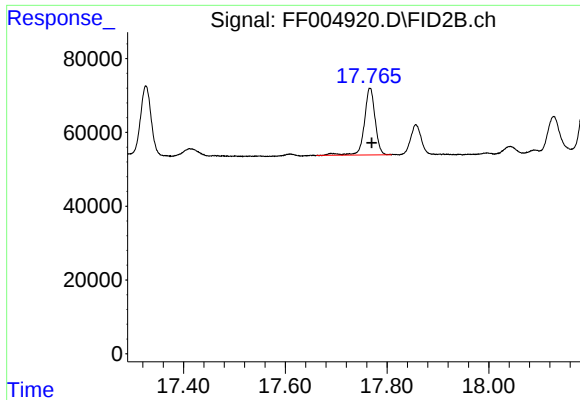

#13 N-TRIACONTANE


R.T.: 17.767 min
Delta R.T.: -0.003 min
Response: 266090
Conc: 2.37 ug/ml

Instrument :
FID_F
ClientSampleId :
ERM-16R

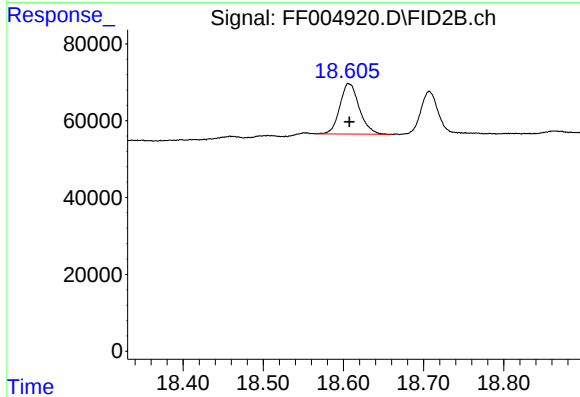

#14 N-DOTRIACONTANE

R.T.: 18.607 min
Delta R.T.: 0.000 min
Response: 219748
Conc: 1.93 ug/ml

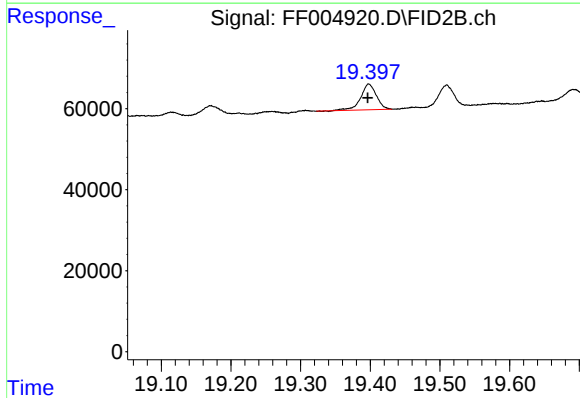

#15 N-TETRATRIACONTANE

R.T.: 19.398 min
Delta R.T.: 0.002 min
Response: 99264
Conc: 0.91 ug/ml