

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF070119\
 Data File : FF004922.D
 Signal(s) : FID2B.ch
 Acq On : 02 Jul 2019 13:33
 Operator : DD\AJ
 Sample : K3160-09 10X
 Misc :
 ALS Vial : 90 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :
 EO-01-062819-B

Integration File: autoint1.e
 Quant Time: Jul 02 14:43:25 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF062619.M
 Quant Title :
 QLast Update : Wed Jun 26 14:27:24 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.687	130028	1.337 ug/ml
Target Compounds			
4) N-TETRADECANE	8.216	237206	1.896 ug/ml
5) N-HEXADECANE	9.820	356600	2.888 ug/ml
6) N-OCTADECANE	11.265	372767	3.147 ug/ml
7) N-EICOSANE	12.579	302202	2.605 ug/ml
8) N-DOCOSANE	13.784	156773	1.393 ug/ml
10) N-TETRACOSANE	14.888	292685	2.629 ug/ml
11) N-HEXACOSANE	15.916	173206	1.566 ug/ml
12) N-OCTACOSANE	16.872	269436	2.416 ug/ml
13) N-TRIACONTANE	17.767	326859	2.910 ug/ml
14) N-DOTRIACONTANE	18.608	284800	2.501 ug/ml
15) N-TETRATRIACONTANE	19.398	240234	2.213 ug/ml
16) N-HEXATRIACONTANE	20.151	318308	3.074 ug/ml
17) N-OCTATRIACONTANE	20.903	165993	1.740 ug/ml
18) N-TETRACONTANE	21.832	159000	1.368 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF070119\
Data File : FF004922.D
Signal(s) : FID2B.ch
Acq On : 02 Jul 2019 13:33
Operator : DD\AJ
Sample : K3160-09 10X
Misc :
ALS Vial : 90 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
EO-01-062819-B

Integration File: autoint1.e
Quant Time: Jul 02 14:43:25 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF062619.M
Quant Title :
QLast Update : Wed Jun 26 14:27:24 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

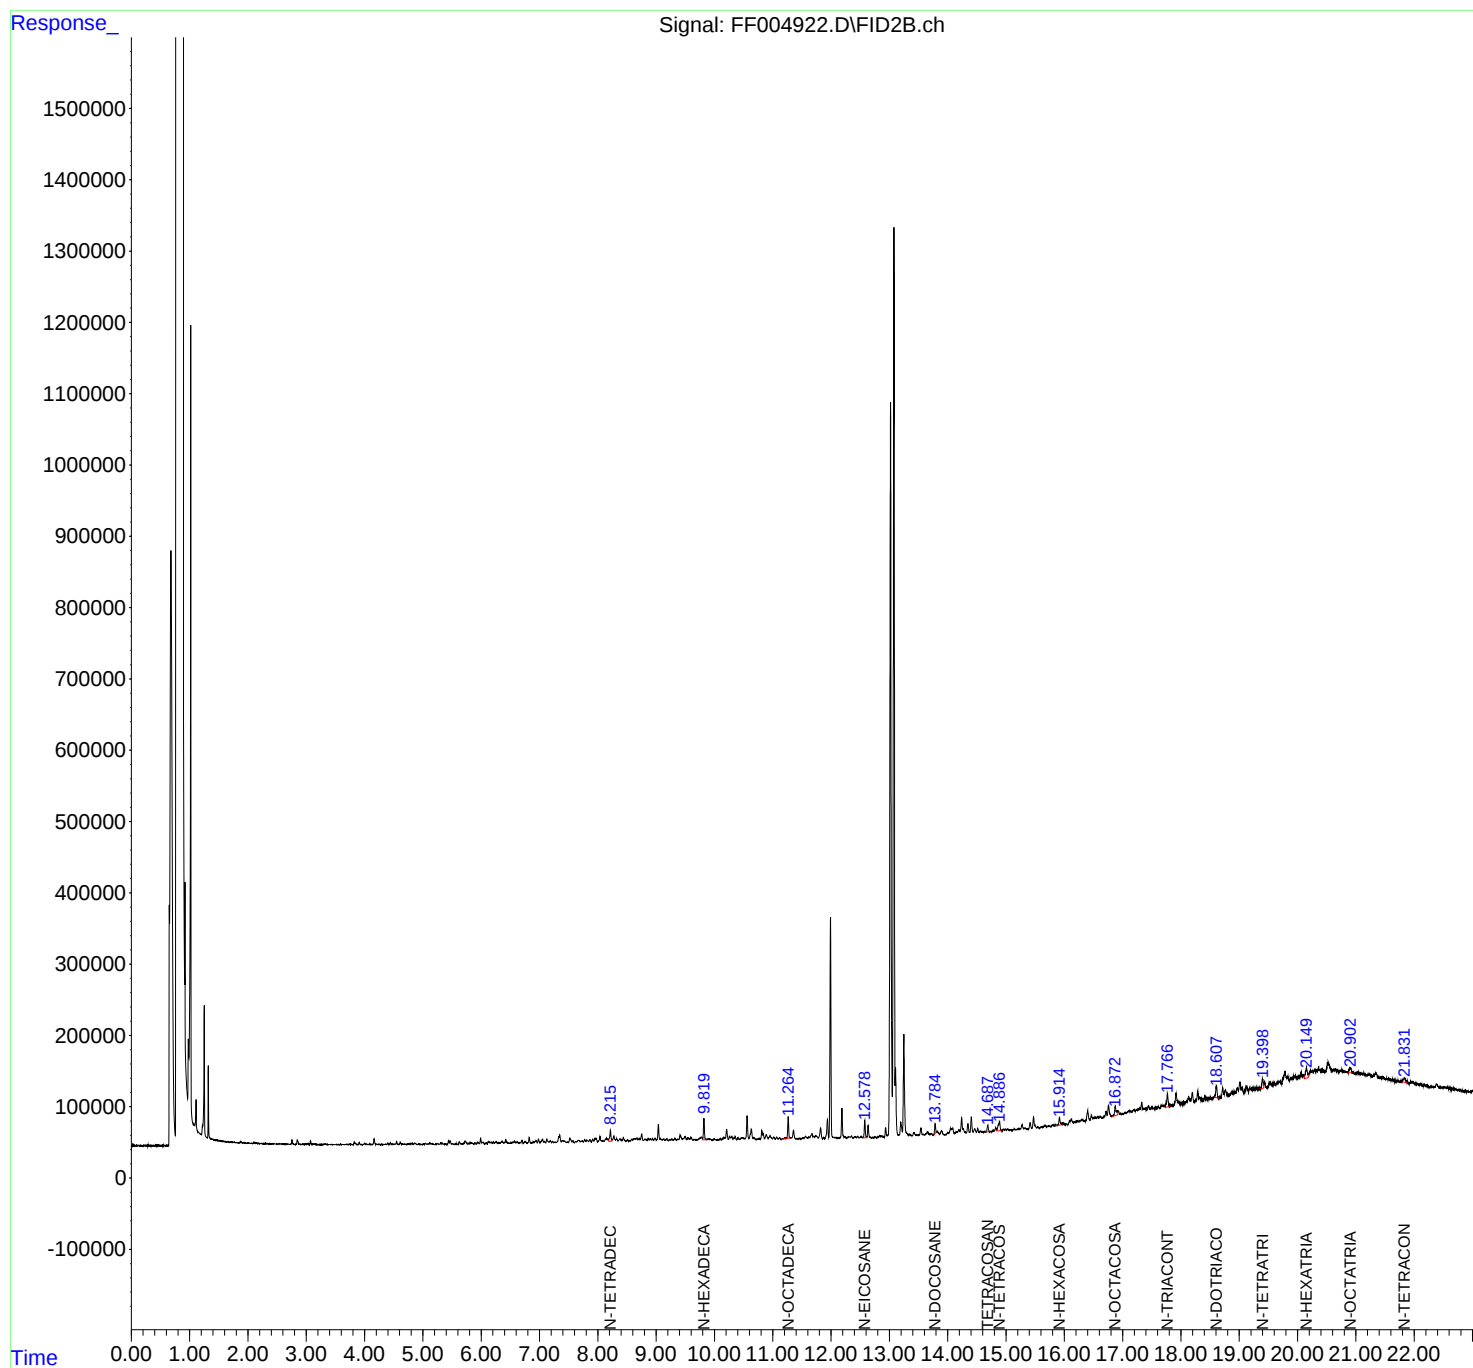


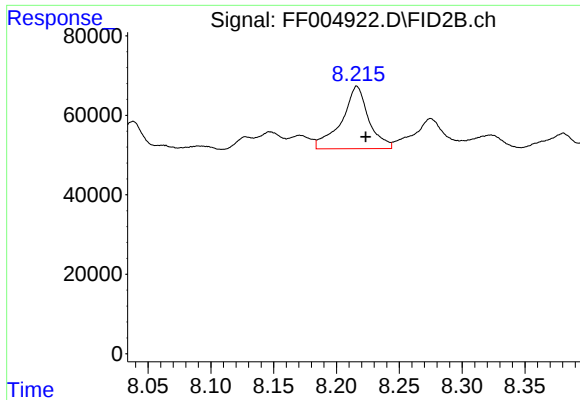

#4 N-TETRADECANE


R.T.: 8.216 min
Delta R.T.: -0.007 min
Response: 237206
Conc: 1.90 ug/ml

Instrument :
FID_F
ClientSampleId :
EO-01-062819-B

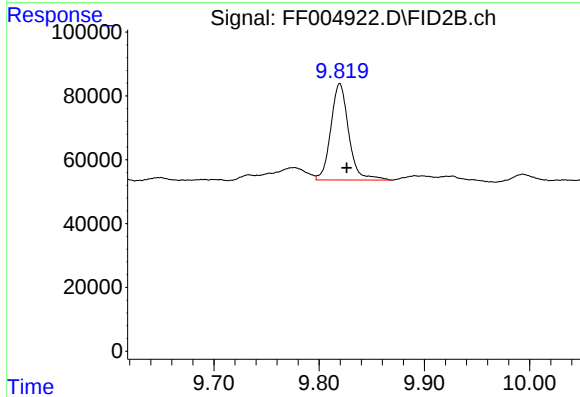


#5 N-HEXADECANE

R.T.: 9.820 min
Delta R.T.: -0.006 min
Response: 356600
Conc: 2.89 ug/ml

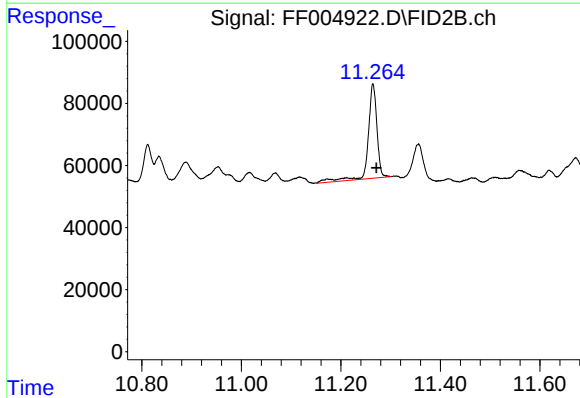


#6 N-OCTADECANE

R.T.: 11.265 min
Delta R.T.: -0.007 min
Response: 372767
Conc: 3.15 ug/ml

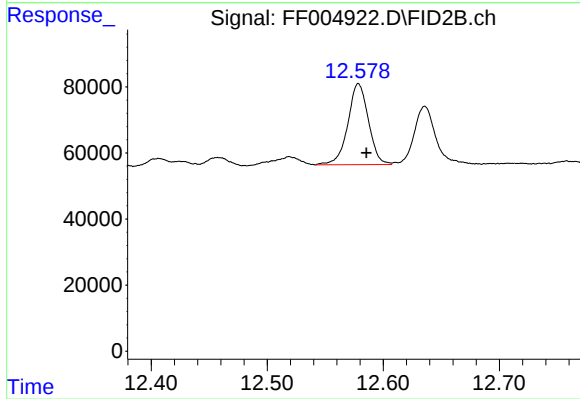

#7 N-EICOSANE


R.T.: 12.579 min
Delta R.T.: -0.007 min
Response: 302202
Conc: 2.60 ug/ml

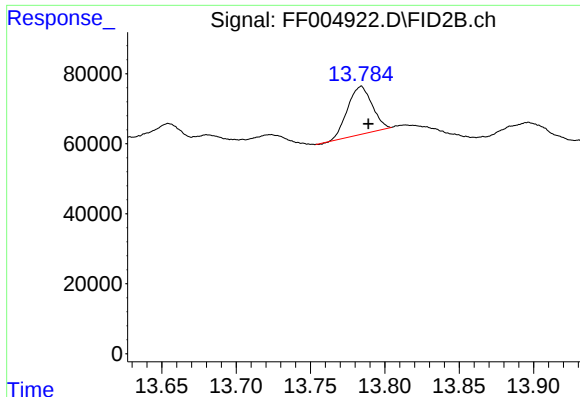

#8 N-DOCOSANE


R.T.: 13.784 min
Delta R.T.: -0.005 min
Response: 156773
Conc: 1.39 ug/ml

Instrument :
FID_F
ClientSampleId :
EO-01-062819-B

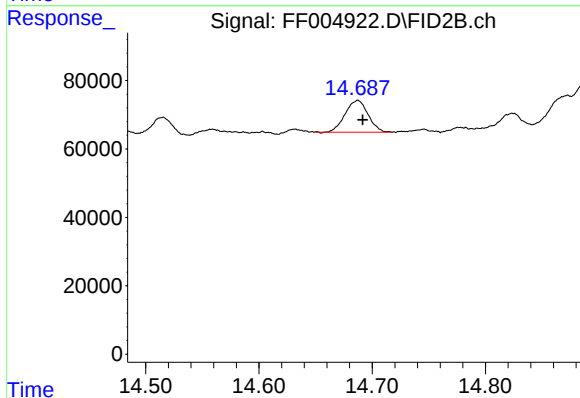


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.687 min
Delta R.T.: -0.004 min
Response: 130028
Conc: 1.34 ug/ml

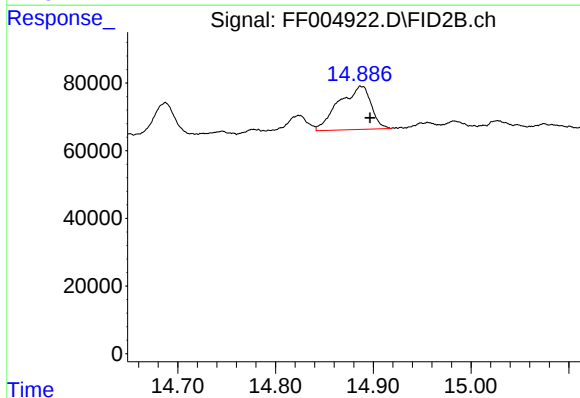


#10 N-TETRACOSANE

R.T.: 14.888 min
Delta R.T.: -0.009 min
Response: 292685
Conc: 2.63 ug/ml

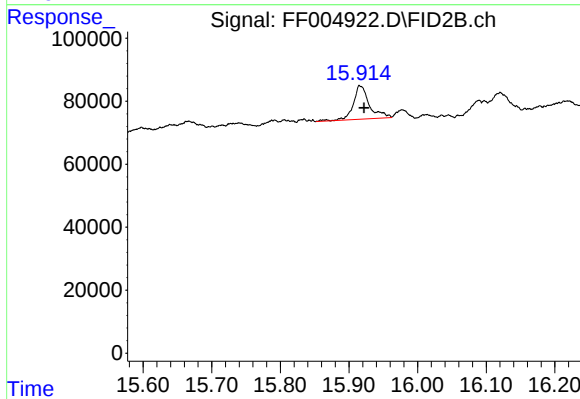

#11 N-HEXACOSANE


R.T.: 15.916 min
Delta R.T.: -0.006 min
Response: 173206
Conc: 1.57 ug/ml

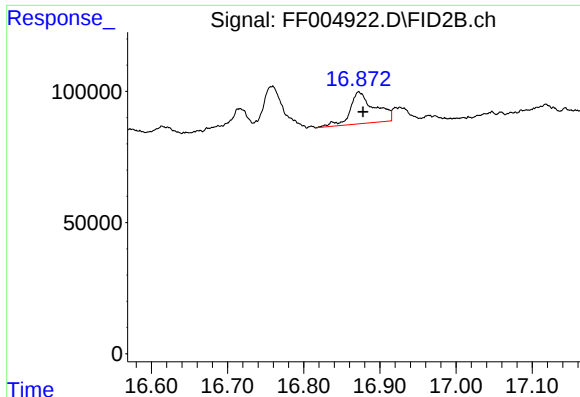

#12 N-OCTACOSANE


R.T.: 16.872 min
Delta R.T.: -0.006 min
Response: 269436
Conc: 2.42 ug/ml

Instrument :
FID_F
ClientSampleId :
EO-01-062819-B

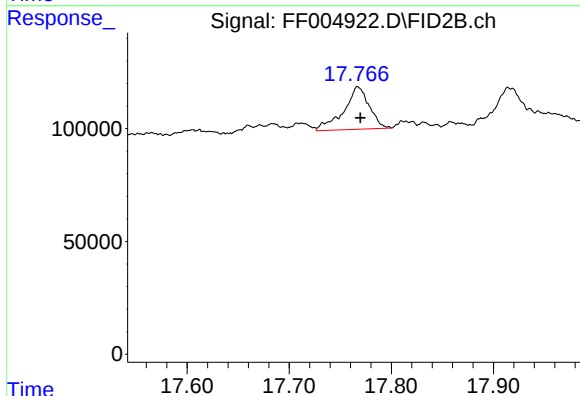


#13 N-TRIACONTANE

R.T.: 17.767 min
Delta R.T.: -0.003 min
Response: 326859
Conc: 2.91 ug/ml

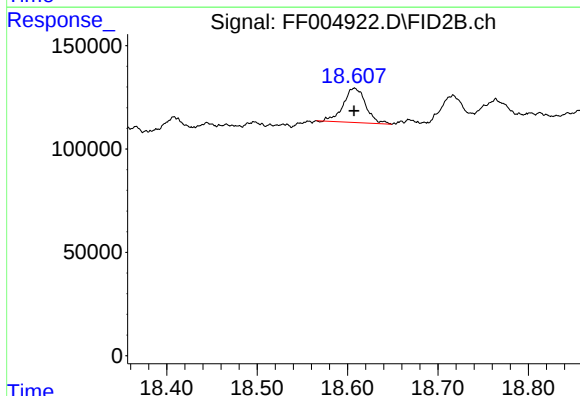


#14 N-DOTRIACONTANE

R.T.: 18.608 min
Delta R.T.: 0.000 min
Response: 284800
Conc: 2.50 ug/ml

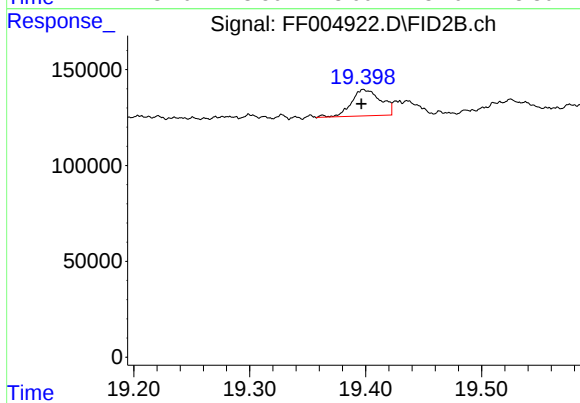

#15 N-TETRATRIACONTANE


R.T.: 19.398 min
Delta R.T.: 0.002 min
Response: 240234
Conc: 2.21 ug/ml

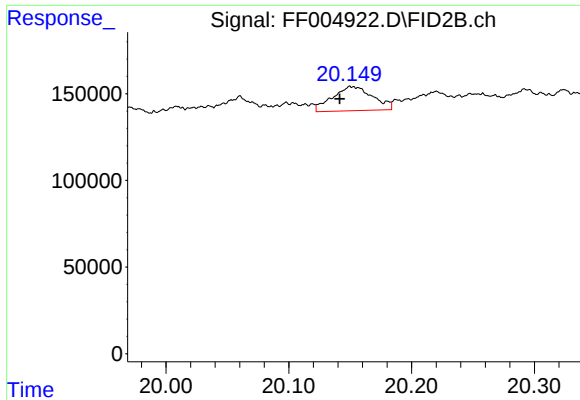

#16 N-HEXATRIACONTANE


R.T.: 20.151 min
Delta R.T.: 0.009 min
Response: 318308
Conc: 3.07 ug/ml

Instrument :
FID_F
ClientSampleId :
EO-01-062819-B

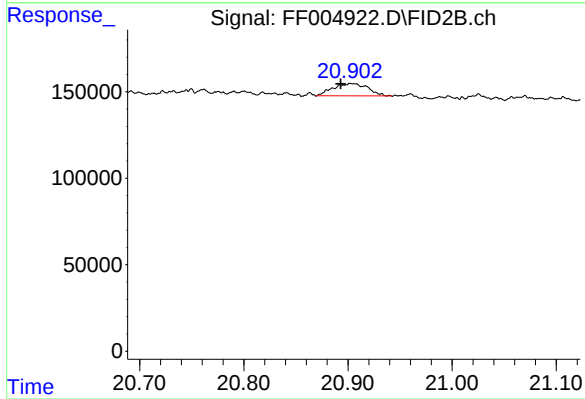

#17 N-OCTATRIACONTANE

R.T.: 20.903 min
Delta R.T.: 0.010 min
Response: 165993
Conc: 1.74 ug/ml

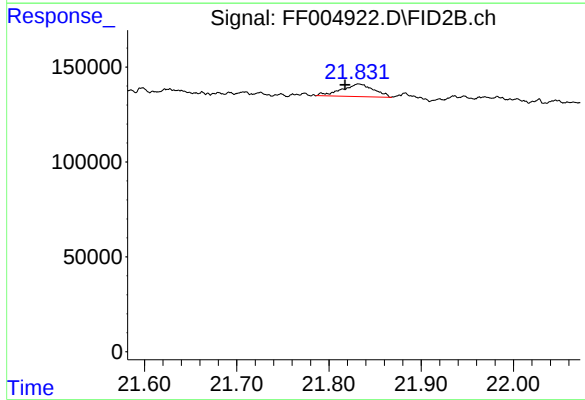

#18 N-TETRACONTANE

R.T.: 21.832 min
Delta R.T.: 0.015 min
Response: 159000
Conc: 1.37 ug/ml