

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_F\Data\FF070119\  
Data File : FF004882.D  
Signal(s) : FID2B.ch  
Acq On : 01 Jul 2019 10:29  
Operator : DD\AJ  
Sample : RT MARKER  
Misc :  
ALS Vial : 54 Sample Multiplier: 1

Instrument :  
FID\_F  
ClientSampleId :  
RT MARKER

Integration File: autoint1.e  
Quant Time: Jul 02 01:49:18 2019  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_F\Method\FF062619.M  
Quant Title :  
QLast Update : Wed Jun 26 14:27:24 2019  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1uL  
Signal Phase : Rxi-1ms  
Signal Info : 20mx0.18mmx0.18um

| Compound                    |              | R.T.   | Response | Conc Units   |
|-----------------------------|--------------|--------|----------|--------------|
| -----                       |              |        |          |              |
| System Monitoring Compounds |              |        |          |              |
| Target Compounds            |              |        |          |              |
| 3)                          | N-DODECANE   | 6.431  | 6127870  | 48.296 ug/ml |
| 12)                         | N-OCTACOSANE | 16.891 | 5955567  | 53.394 ug/ml |
| -----                       |              |        |          |              |

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_F\Data\FF070119\  
Data File : FF004882.D  
Signal(s) : FID2B.ch  
Acq On : 01 Jul 2019 10:29  
Operator : DD\AJ  
Sample : RT MARKER  
Misc :  
ALS Vial : 54 Sample Multiplier: 1

Instrument :  
FID\_F  
ClientSampleId :  
RT MARKER

Integration File: autoint1.e  
Quant Time: Jul 02 01:49:18 2019  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_F\Method\FF062619.M  
Quant Title :  
QLast Update : Wed Jun 26 14:27:24 2019  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1uL  
Signal Phase : Rxi-1ms  
Signal Info : 20mx0.18mmx0.18um

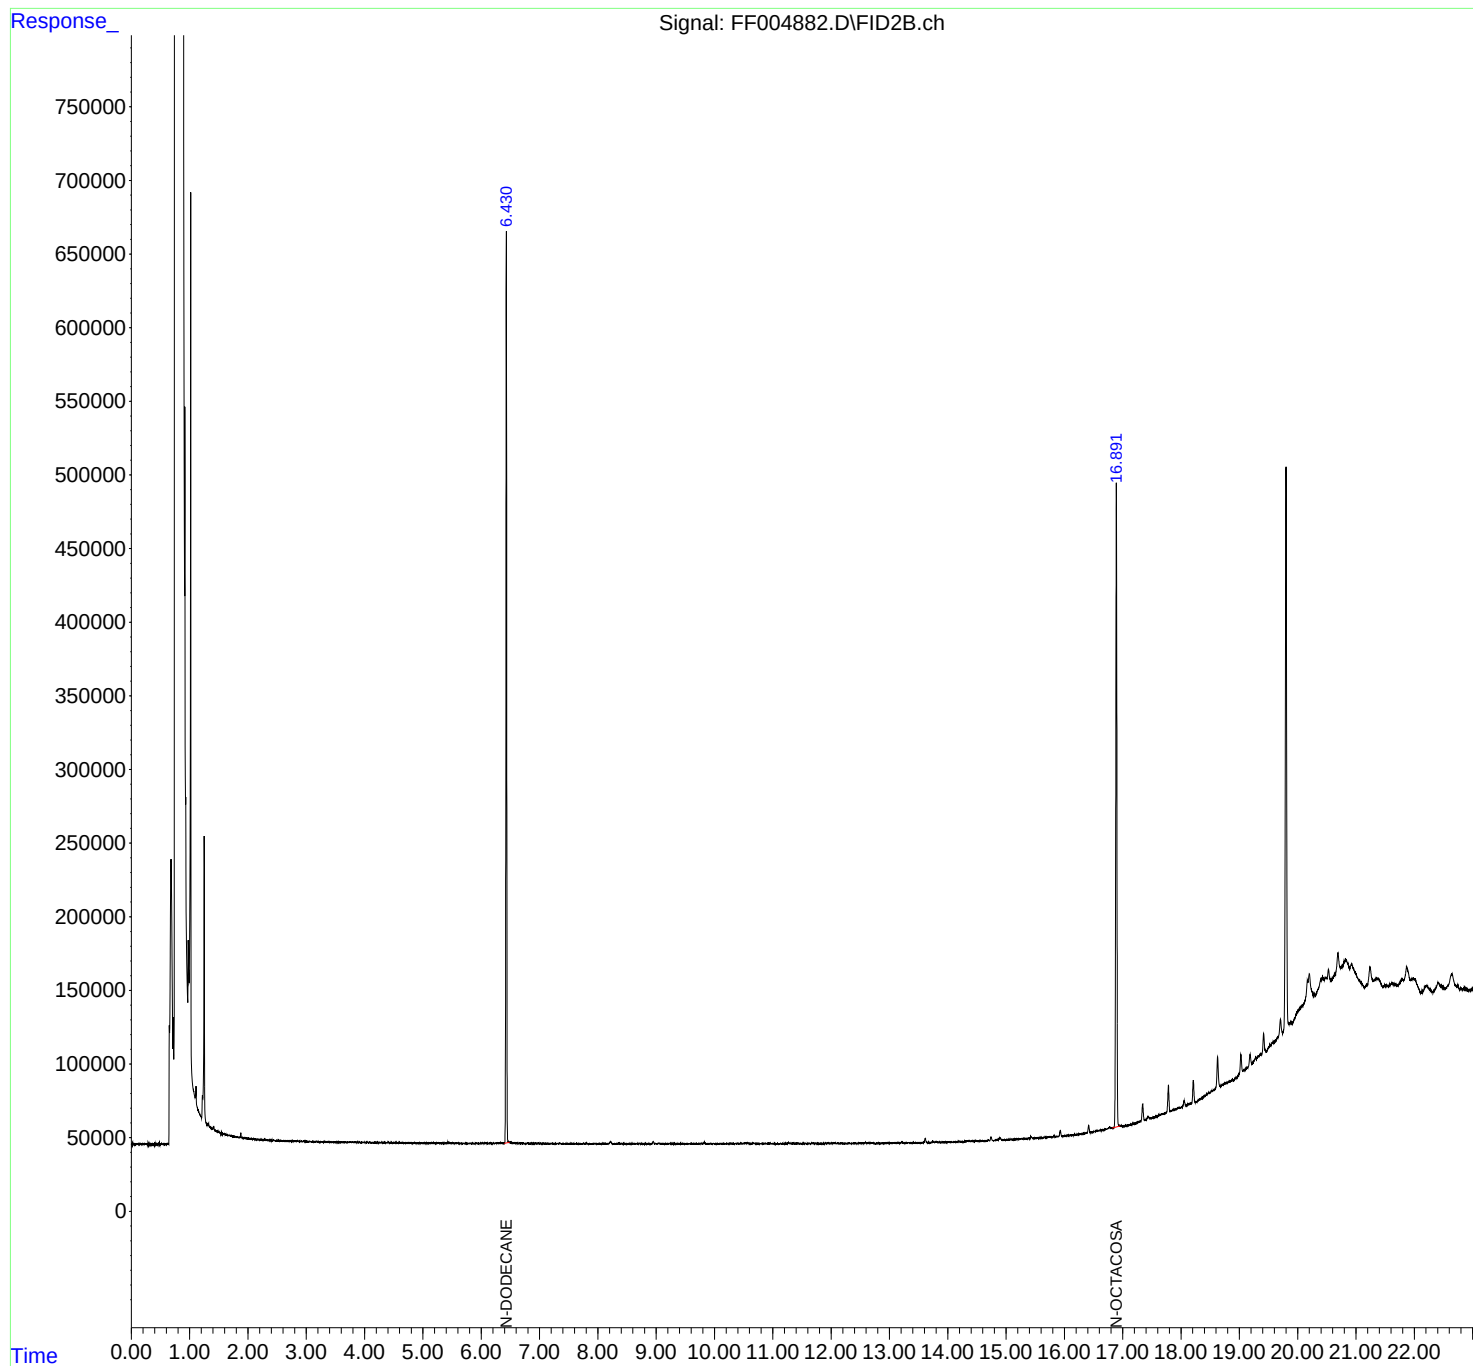


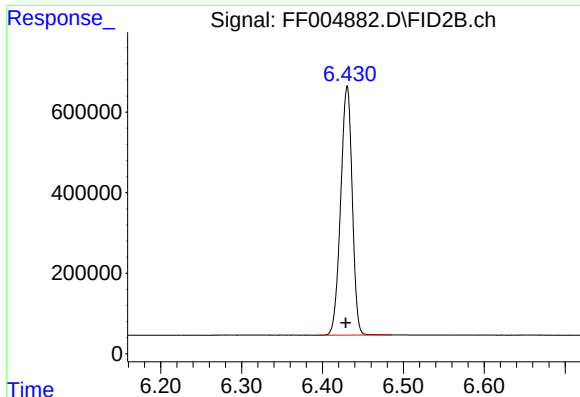

#3 N-DODECANE


R.T.: 6.431 min  
Delta R.T.: 0.002 min  
Response: 6127870  
Conc: 48.30 ug/ml

Instrument :  
FID\_F  
ClientSampleId :  
RT MARKER

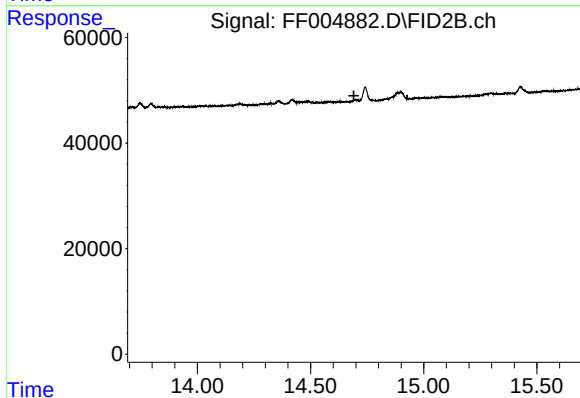

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min  
Exp R.T. : 14.692 min  
Response: 0  
Conc: N.D.

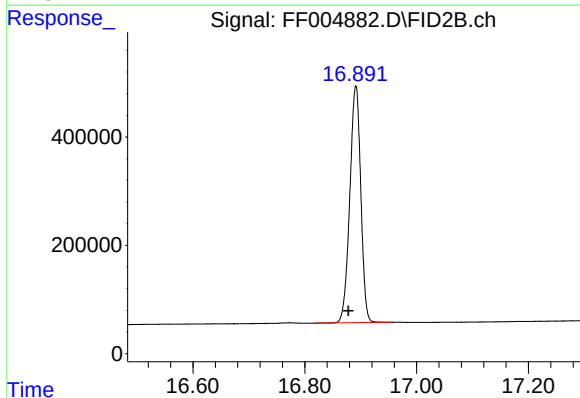

#12 N-OCTACOSANE

R.T.: 16.891 min  
Delta R.T.: 0.014 min  
Response: 5955567  
Conc: 53.39 ug/ml