

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF070119\
Data File : FF004907.D
Signal(s) : FID2B.ch
Acq On : 02 Jul 2019 03:00
Operator : DD\AJ
Sample : K3585-12
Misc :
ALS Vial : 77 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
RM-WATER-COMP

Manual Integrations
APPROVED

Ankita
7/2/2019 4:42:22 PM

Integration File: autoint1.e
Quant Time: Jul 02 08:18:24 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF062619.M
Quant Title :
QLast Update : Wed Jun 26 14:27:24 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.689	2390784	24.582 ug/mlm
Target Compounds			

(f)=RT Delta > 1/2 Window

(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF070119\
Data File : FF004907.D
Signal(s) : FID2B.ch
Acq On : 02 Jul 2019 03:00
Operator : DD\AJ
Sample : K3585-12
Misc :
ALS Vial : 77 Sample Multiplier: 1


Instrument :
FID_F
ClientSampleId :
RM-WATER-COMP


Manual Integrations
APPROVED

Ankita
7/2/2019 4:42:22 PM

Integration File: autoint1.e
Quant Time: Jul 02 08:18:24 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF062619.M
Quant Title :
QLast Update : Wed Jun 26 14:27:24 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

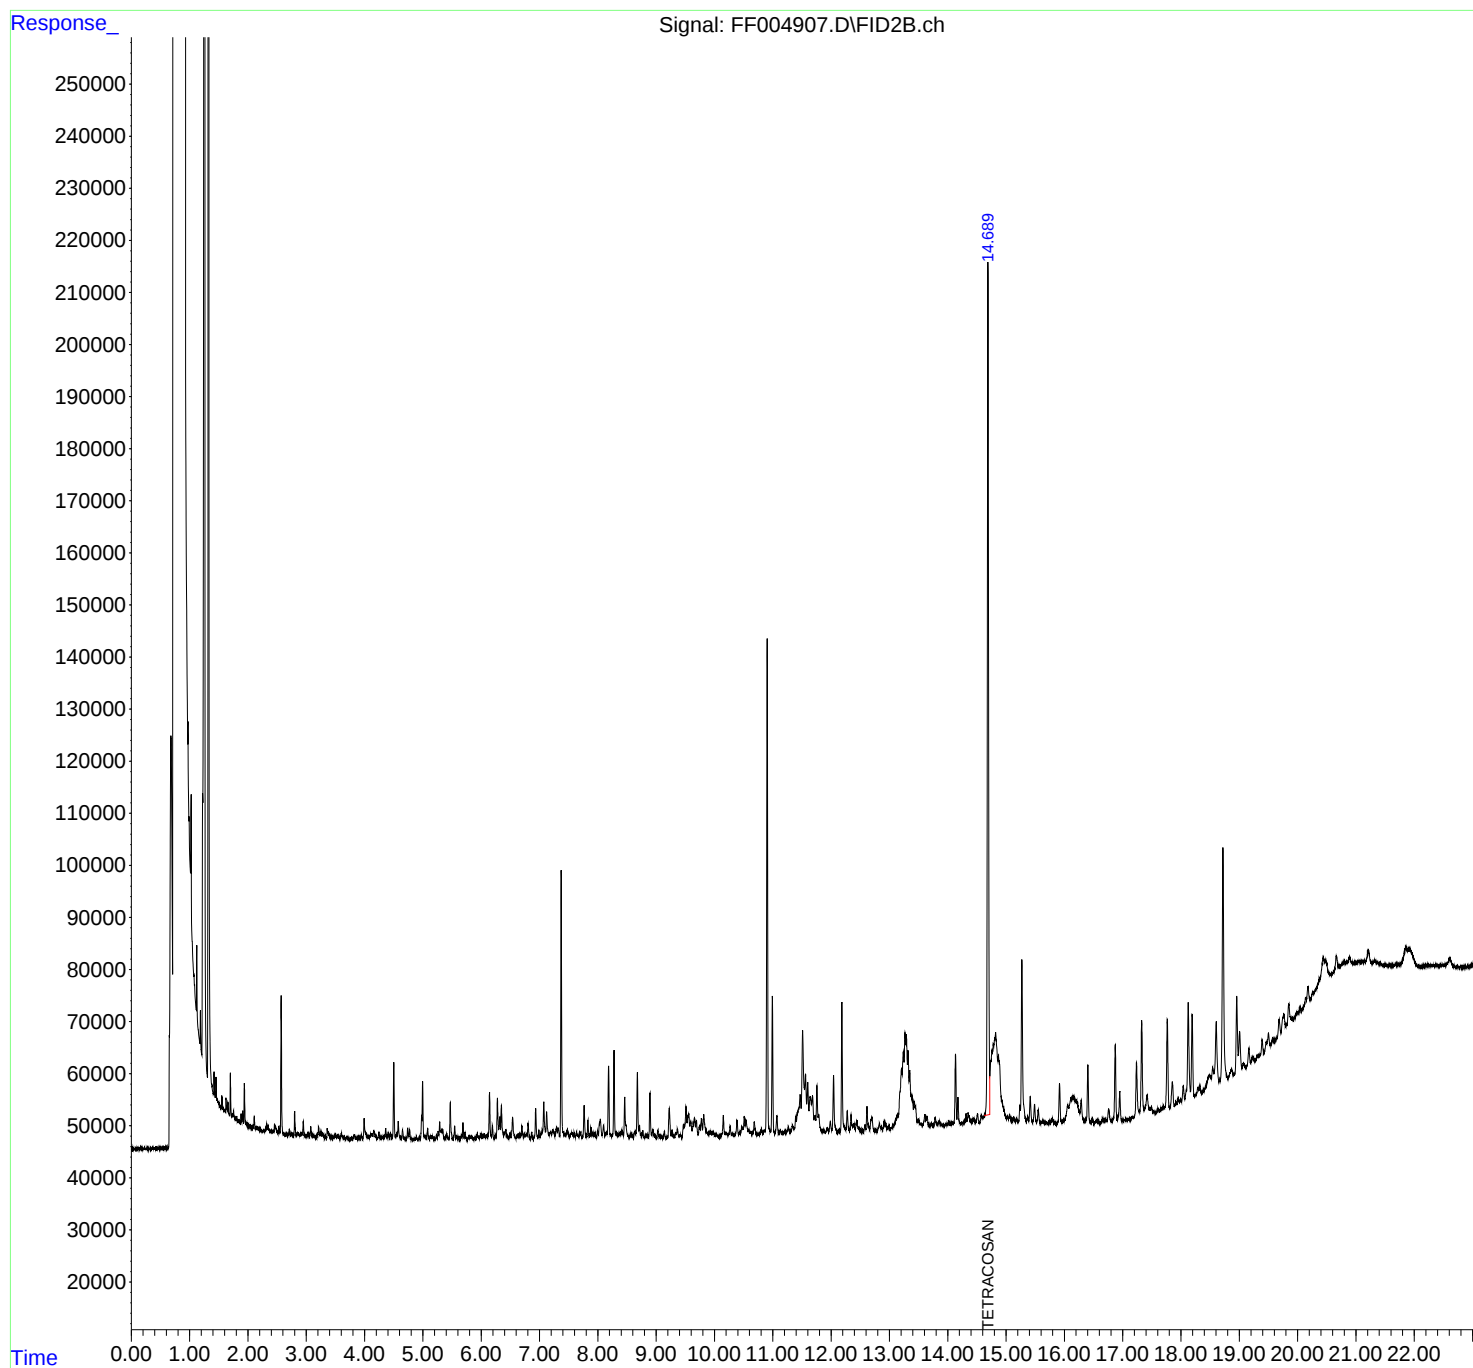

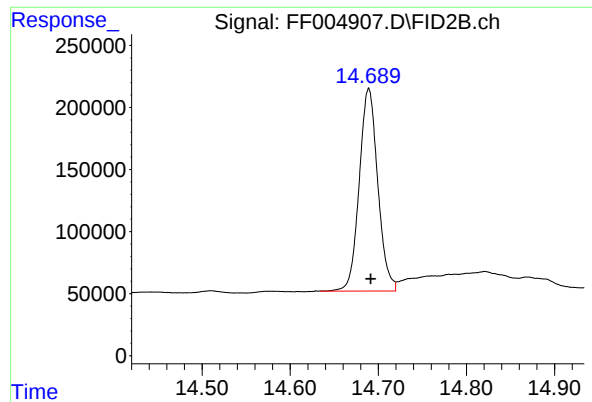

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.689 min
Delta R.T.: -0.003 min
Response: 2390784
Conc: 24.58 ug/ml m

Instrument :
FID_F
ClientSampleId :
RM-WATER-COMP

Manual Integrations
APPROVED

Ankita
7/2/2019 4:42:22 PM