

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF070119\
 Data File : FF004913.D
 Signal(s) : FID2B.ch
 Acq On : 02 Jul 2019 05:57
 Operator : DD\AJ
 Sample : 50 PPM TRPH STD
 Misc :
 ALS Vial : 53 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :
 50 PPM TRPH STD

Integration File: autoint1.e
 Quant Time: Jul 02 08:19:15 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF062619.M
 Quant Title :
 QLast Update : Wed Jun 26 14:27:24 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.690	5187265	53.335 ug/ml
Target Compounds			
2) N-DECANE	4.403	6392946	50.625 ug/ml
3) N-DODECANE	6.427	6446902	50.810 ug/ml
4) N-TETRADECANE	8.221	6374810	50.946 ug/ml
5) N-HEXADECANE	9.824	6321672	51.197 ug/ml
6) N-OCTADECANE	11.269	6142440	51.848 ug/ml
7) N-EICOSANE	12.583	6072752	52.340 ug/ml
8) N-DOCOSANE	13.786	5949802	52.880 ug/ml
10) N-TETRACOSANE	14.895	5942330	53.383 ug/ml
11) N-HEXACOSANE	15.921	5963447	53.916 ug/ml
12) N-OCTACOSANE	16.876	6034899	54.106 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF070119\
Data File : FF004913.D
Signal(s) : FID2B.ch
Acq On : 02 Jul 2019 05:57
Operator : DD\AJ
Sample : 50 PPM TRPH STD
Misc :
ALS Vial : 53 Sample Multiplier: 1

Instrument :
FID_F
ClientSampled :
50 PPM TRPH STD

Integration File: autoint1.e
Quant Time: Jul 02 08:19:15 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF062619.M
Quant Title :
QLast Update : Wed Jun 26 14:27:24 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

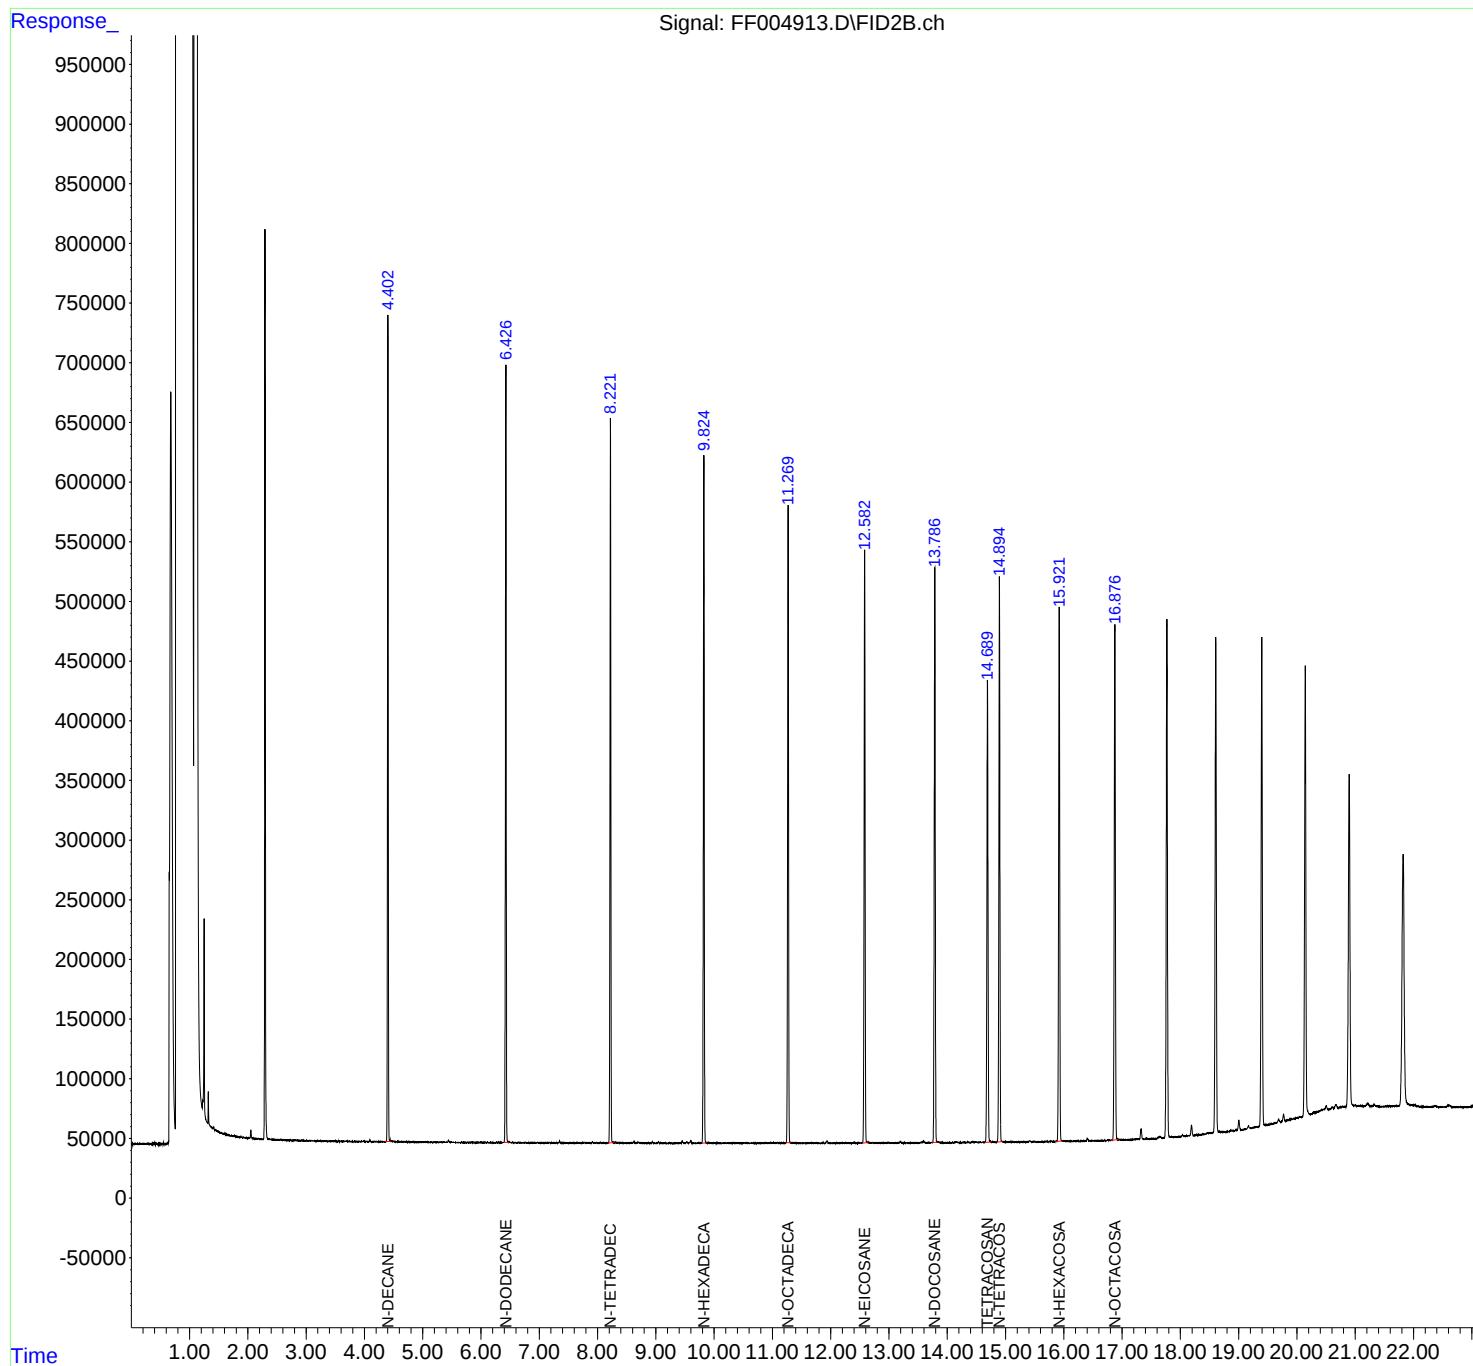


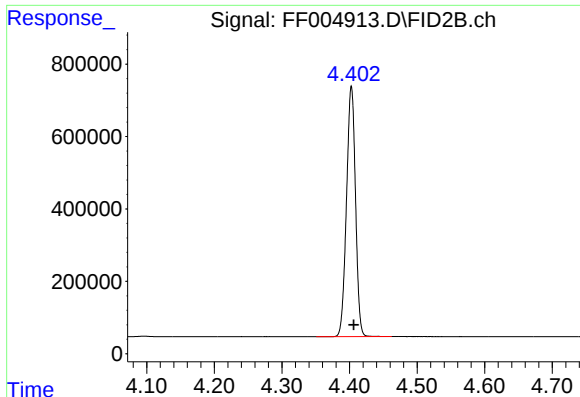

#2 N-DECANE


R.T.: 4.403 min
Delta R.T.: -0.003 min
Response: 6392946
Conc: 50.62 ug/ml

Instrument :
FID_F
ClientSampleId :
50 PPM TRPH STD

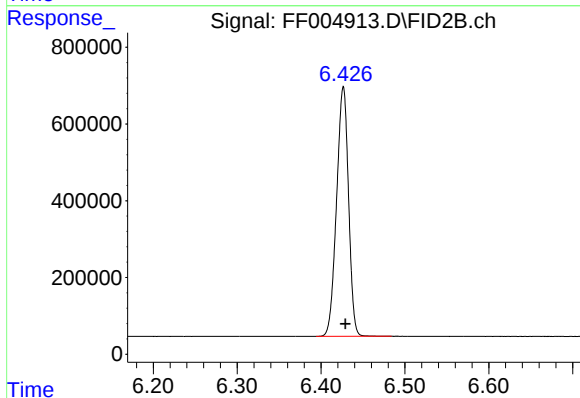


#3 N-DODECANE

R.T.: 6.427 min
Delta R.T.: -0.002 min
Response: 6446902
Conc: 50.81 ug/ml

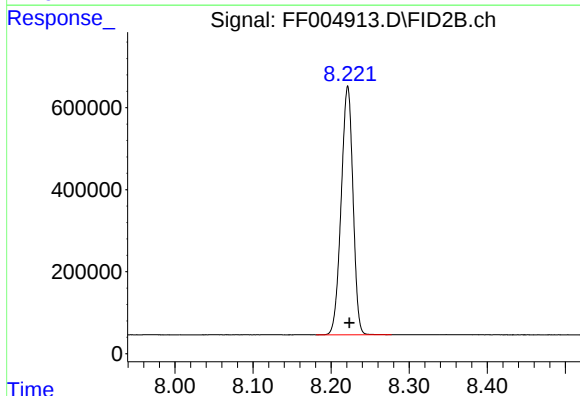


#4 N-TETRADECANE

R.T.: 8.221 min
Delta R.T.: -0.002 min
Response: 6374810
Conc: 50.95 ug/ml

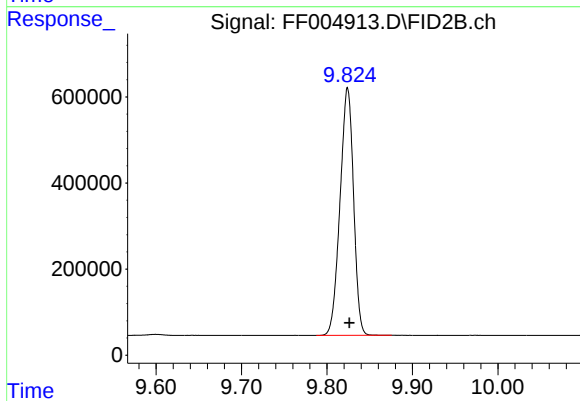

#5 N-HEXADECANE


R.T.: 9.824 min
Delta R.T.: -0.002 min
Response: 6321672
Conc: 51.20 ug/ml

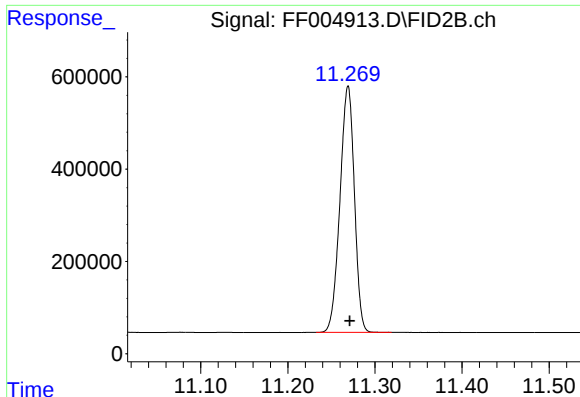

#6 N-OCTADECANE


R.T.: 11.269 min
Delta R.T.: -0.002 min
Response: 6142440
Conc: 51.85 ug/ml

Instrument :
FID_F
ClientSampleId :
50 PPM TRPH STD

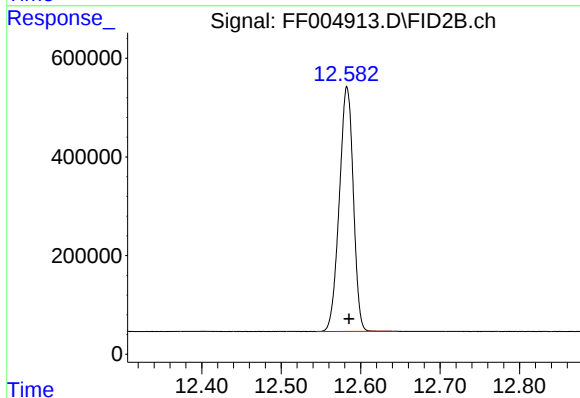


#7 N-EICOSANE

R.T.: 12.583 min
Delta R.T.: -0.003 min
Response: 6072752
Conc: 52.34 ug/ml

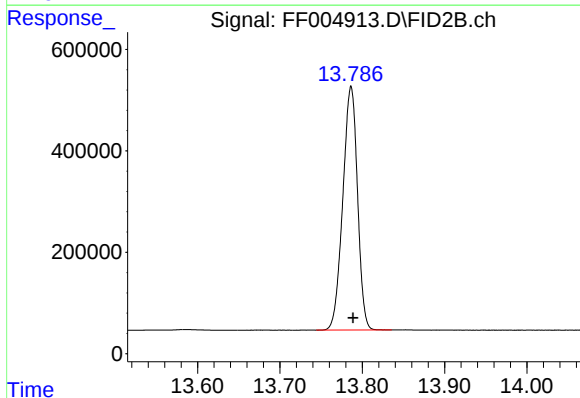


#8 N-DOCOSANE

R.T.: 13.786 min
Delta R.T.: -0.002 min
Response: 5949802
Conc: 52.88 ug/ml

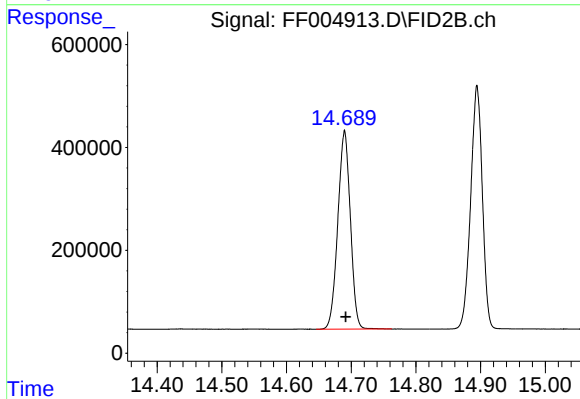

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.690 min
Delta R.T.: -0.002 min
Response: 5187265
Conc: 53.33 ug/ml

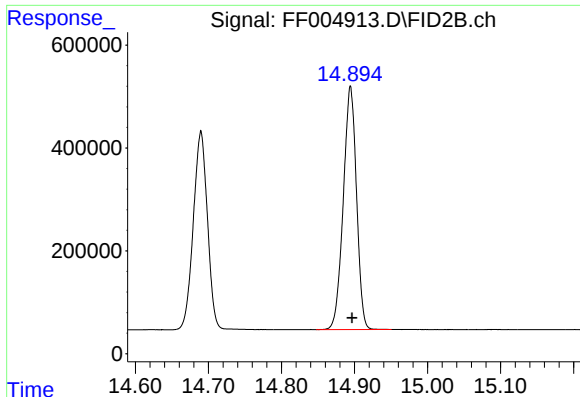

#10 N-TETRACOSANE


R.T.: 14.895 min
Delta R.T.: -0.002 min
Response: 5942330
Conc: 53.38 ug/ml

Instrument :
FID_F
ClientSampleId :
50 PPM TRPH STD

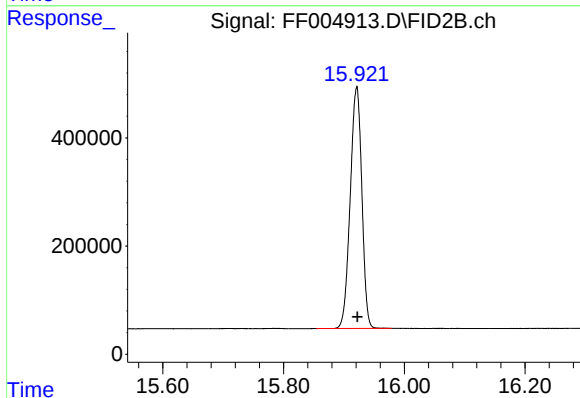

#11 N-HEXACOSANE

R.T.: 15.921 min
Delta R.T.: 0.000 min
Response: 5963447
Conc: 53.92 ug/ml

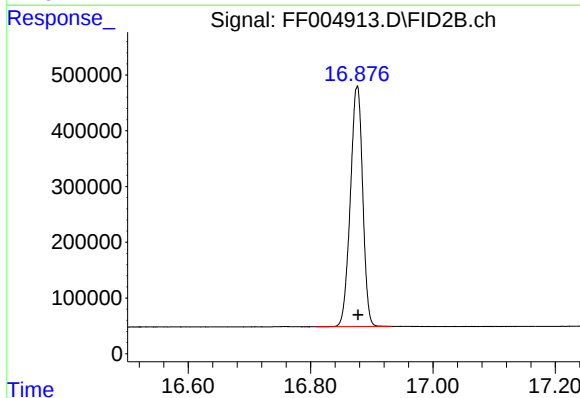

#12 N-OCTACOSANE

R.T.: 16.876 min
Delta R.T.: -0.002 min
Response: 6034899
Conc: 54.11 ug/ml