

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF070119\
 Data File : FF004915.D
 Signal(s) : FID2B.ch
 Acq On : 02 Jul 2019 10:03
 Operator : DD\AJ
 Sample : PB121008BS
 Misc :
 ALS Vial : 83 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :
 PB121008BS

Integration File: autoint1.e
 Quant Time: Jul 02 14:42:49 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF062619.M
 Quant Title :
 QLast Update : Wed Jun 26 14:27:24 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.687	2017066	20.739 ug/ml
Target Compounds			
2) N-DECANE	4.401	2508343	19.863 ug/ml
3) N-DODECANE	6.423	2518839	19.852 ug/ml
4) N-TETRADECANE	8.217	2491970	19.915 ug/ml
5) N-HEXADECANE	9.820	2465622	19.968 ug/ml
6) N-OCTADECANE	11.265	2394749	20.214 ug/ml
7) N-EICOSANE	12.580	2365472	20.388 ug/ml
8) N-DOCOSANE	13.783	2325288	20.666 ug/ml
10) N-TETRACOSANE	14.892	2327402	20.908 ug/ml
11) N-HEXACOSANE	15.918	2318218	20.959 ug/ml
12) N-OCTACOSANE	16.872	2347962	21.051 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF070119\
Data File : FF004915.D
Signal(s) : FID2B.ch
Acq On : 02 Jul 2019 10:03
Operator : DD\AJ
Sample : PB121008BS
Misc :
ALS Vial : 83 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
PB121008BS

Integration File: autoint1.e
Quant Time: Jul 02 14:42:49 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF062619.M
Quant Title :
QLast Update : Wed Jun 26 14:27:24 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

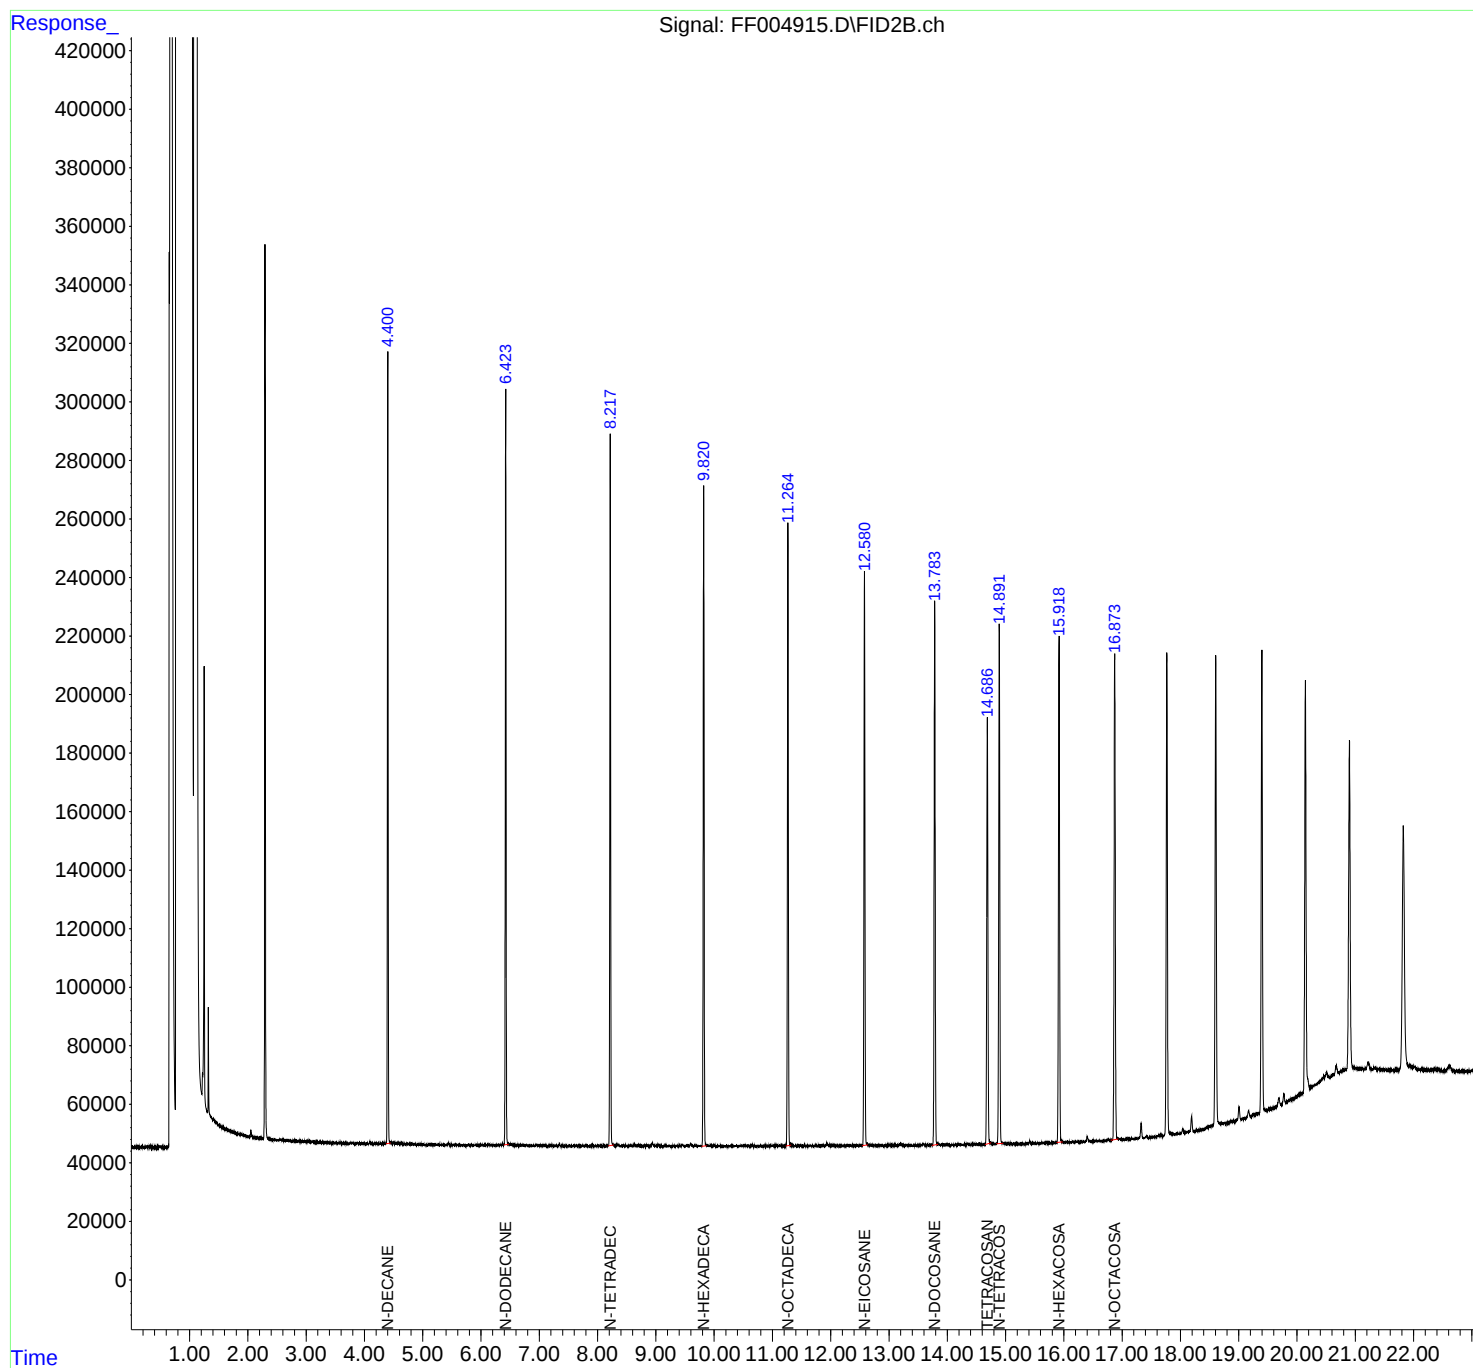


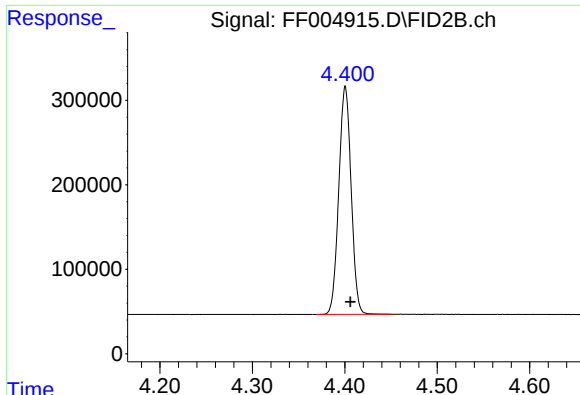

#2 N-DECANE


R.T.: 4.401 min
Delta R.T.: -0.006 min
Response: 2508343
Conc: 19.86 ug/ml

Instrument :
FID_F
ClientSampleId :
PB121008BS

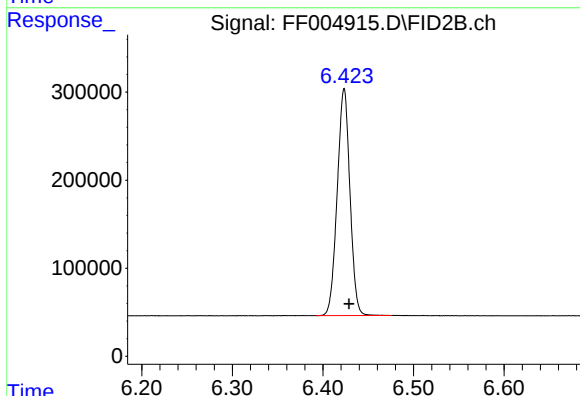


#3 N-DODECANE

R.T.: 6.423 min
Delta R.T.: -0.005 min
Response: 2518839
Conc: 19.85 ug/ml

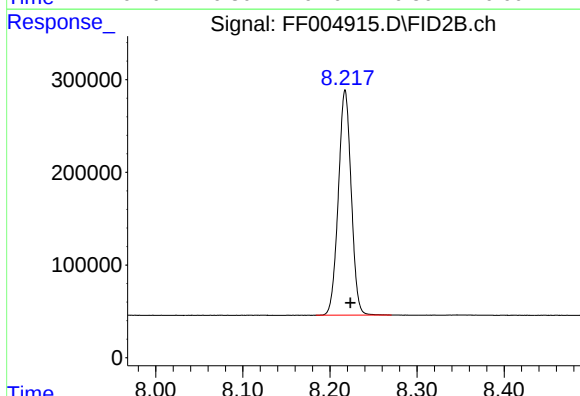


#4 N-TETRADECANE

R.T.: 8.217 min
Delta R.T.: -0.006 min
Response: 2491970
Conc: 19.92 ug/ml

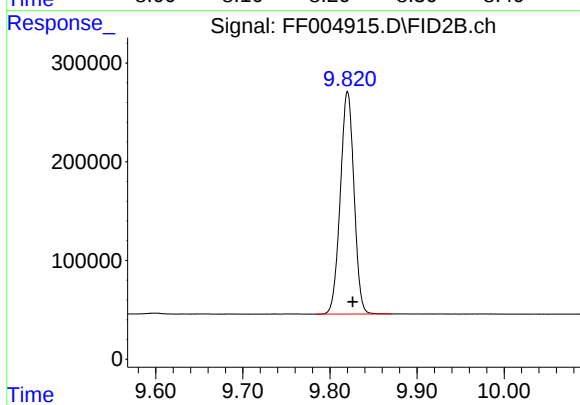

#5 N-HEXADECANE


R.T.: 9.820 min
Delta R.T.: -0.006 min
Response: 2465622
Conc: 19.97 ug/ml

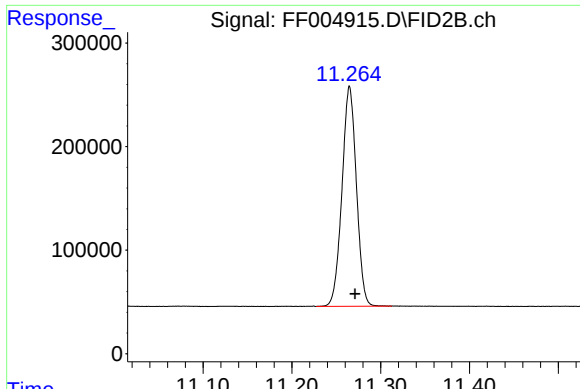

#6 N-OCTADECANE


R.T.: 11.265 min
Delta R.T.: -0.006 min
Response: 2394749
Conc: 20.21 ug/ml

Instrument :
FID_F
ClientSampleId :
PB121008BS

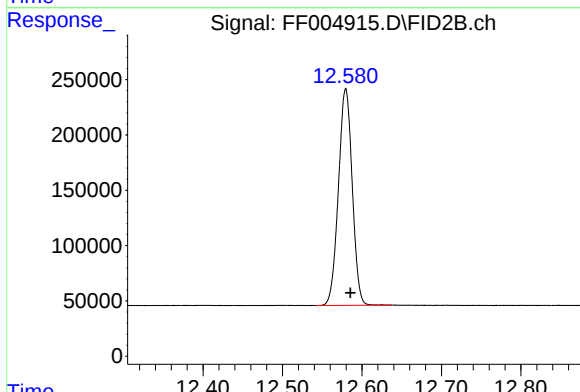


#7 N-EICOSANE

R.T.: 12.580 min
Delta R.T.: -0.006 min
Response: 2365472
Conc: 20.39 ug/ml

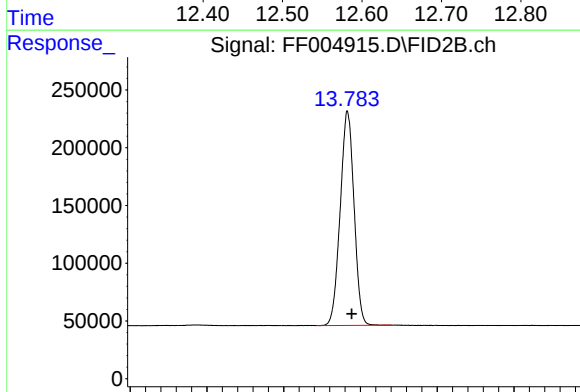


#8 N-DOCOSANE

R.T.: 13.783 min
Delta R.T.: -0.006 min
Response: 2325288
Conc: 20.67 ug/ml

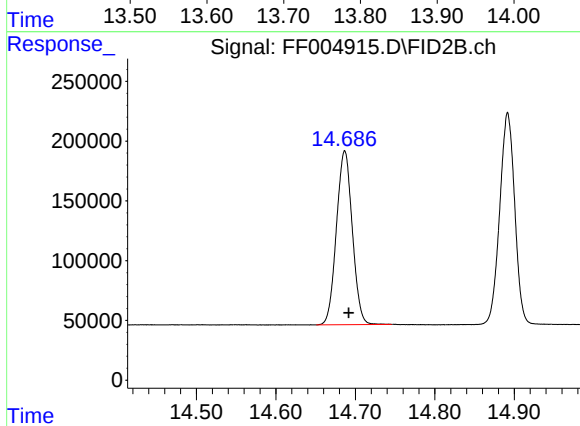

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.687 min
Delta R.T.: -0.005 min
Response: 2017066
Conc: 20.74 ug/ml

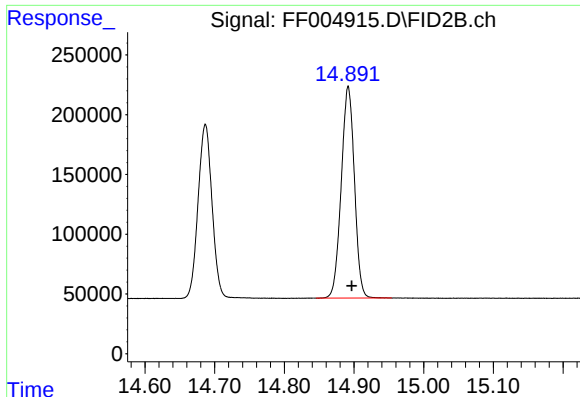

#10 N-TETRACOSANE


R.T.: 14.892 min
Delta R.T.: -0.005 min
Response: 2327402
Conc: 20.91 ug/ml

Instrument :
FID_F
ClientSampleId :
PB121008BS

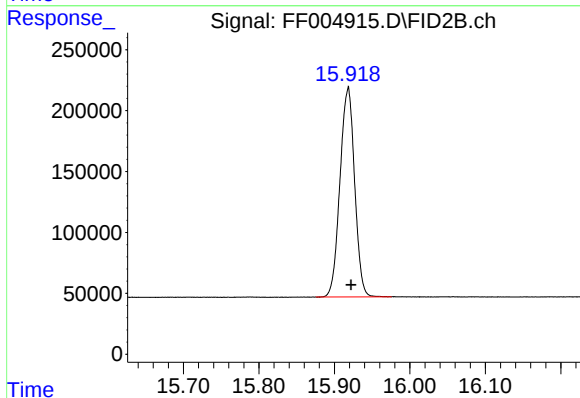

#11 N-HEXACOSANE

R.T.: 15.918 min
Delta R.T.: -0.004 min
Response: 2318218
Conc: 20.96 ug/ml

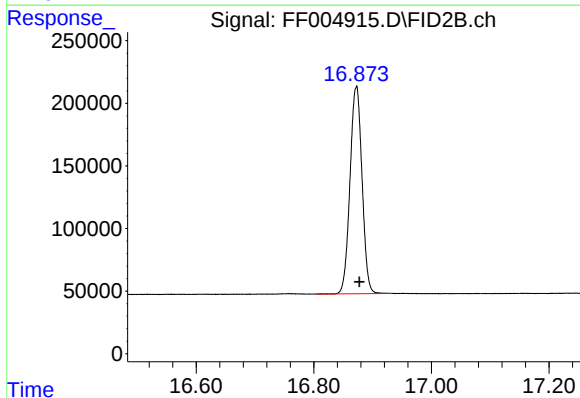

#12 N-OCTACOSANE

R.T.: 16.872 min
Delta R.T.: -0.005 min
Response: 2347962
Conc: 21.05 ug/ml