

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF070119\
Data File : FF004923.D
Signal(s) : FID2B.ch
Acq On : 02 Jul 2019 14:02
Operator : DD\AJ
Sample : K3160-11 10X
Misc :
ALS Vial : 91 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
EO-01-062819-C

Integration File: autoint1.e
Quant Time: Jul 02 14:43:31 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF062619.M
Quant Title :
QLast Update : Wed Jun 26 14:27:24 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.687	162963	1.676 ug/ml
Target Compounds			

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF070119\
Data File : FF004923.D
Signal(s) : FID2B.ch
Acq On : 02 Jul 2019 14:02
Operator : DD\AJ
Sample : K3160-11 10X
Misc :
ALS Vial : 91 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
EO-01-062819-C

Integration File: autoint1.e
Quant Time: Jul 02 14:43:31 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF062619.M
Quant Title :
QLast Update : Wed Jun 26 14:27:24 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

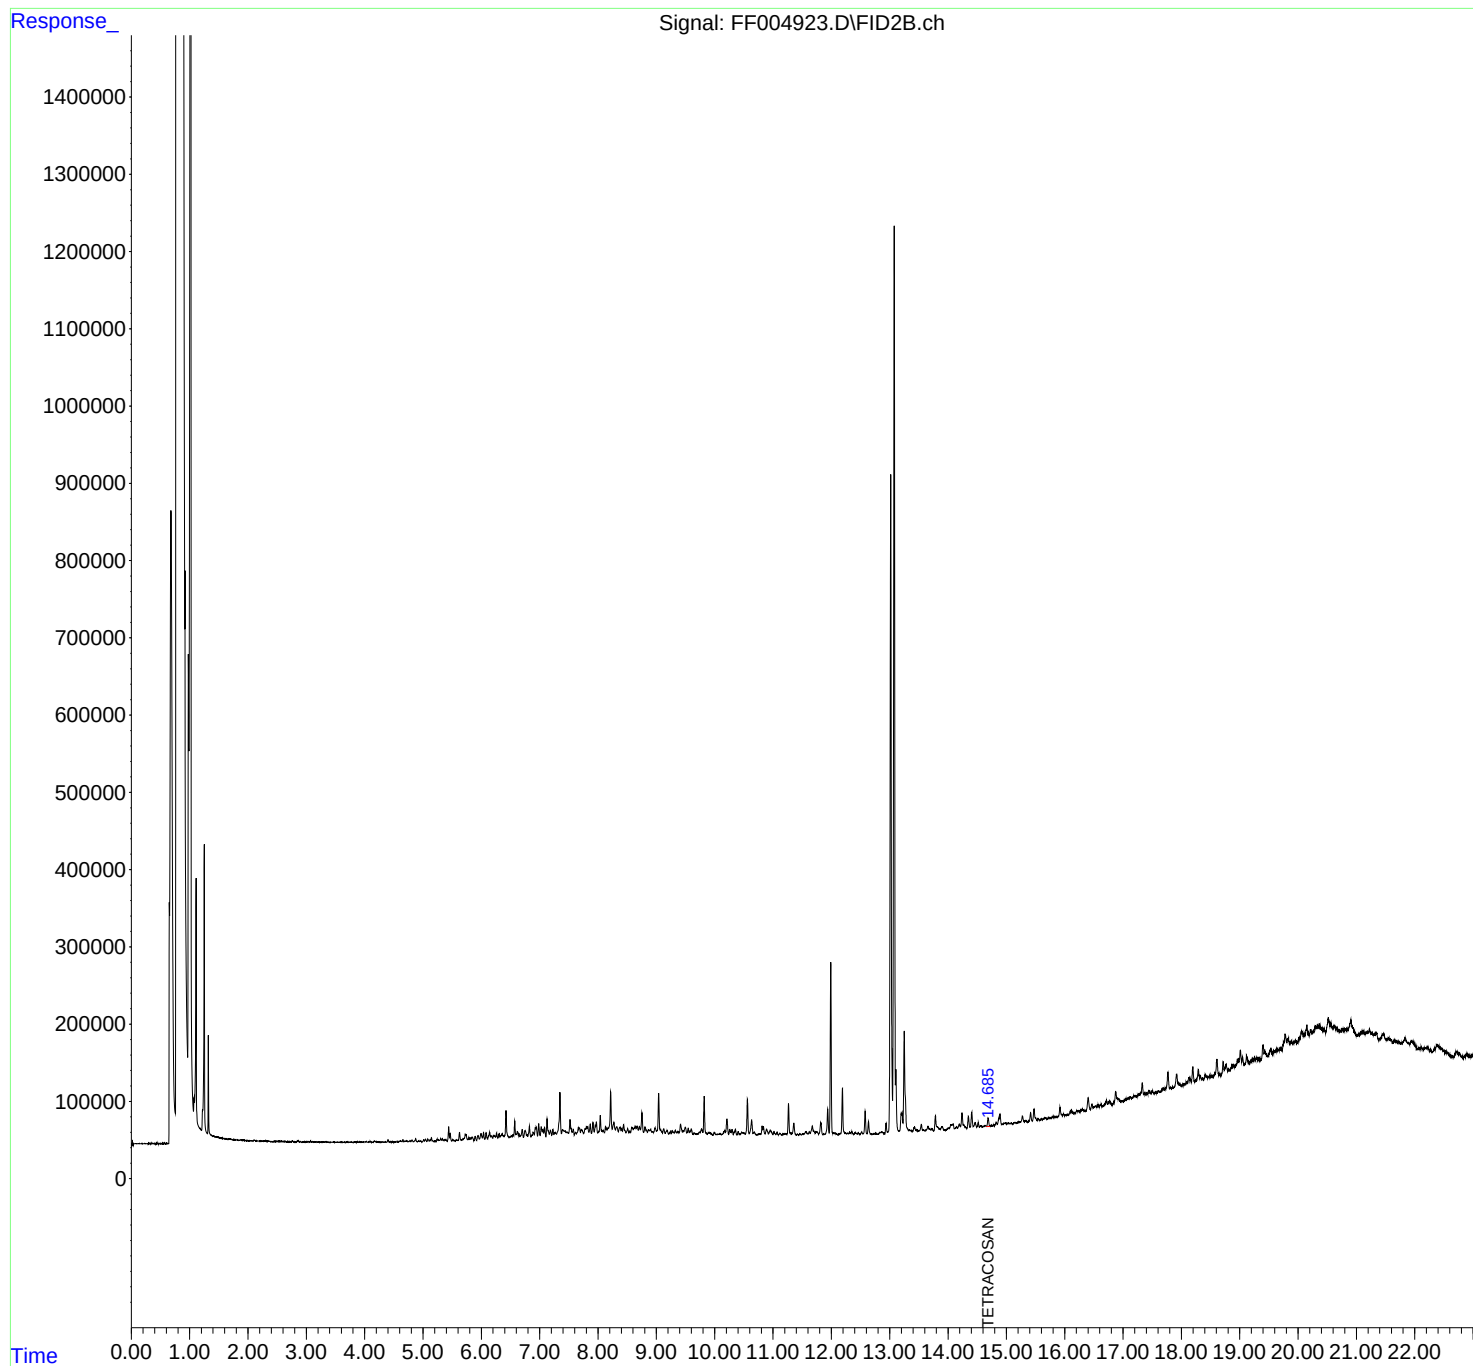

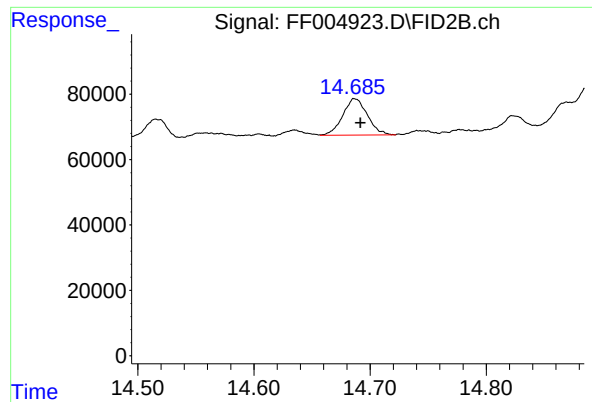

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.687 min
Delta R.T.: -0.005 min
Response: 162963
Conc: 1.68 ug/ml

Instrument :
FID_F
ClientSampleId :
EO-01-062819-C