

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF070122\
Data File : FF010947.D
Signal(s) : FID2B.ch
Acq On : 01 Jul 2022 08:50
Operator : AJ\MA
Sample : MECL2
Misc :
ALS Vial : 51 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Jul 02 02:56:48 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF063022.M
Quant Title :
QLast Update : Fri Jul 01 01:40:42 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
Target Compounds				
14)	N-DOTRIACONTANE	18.724	334996	3.121 ug/ml
16)	N-HEXATRIACONTANE	20.271	419976	4.884 ug/ml
18)	N-TETRACONTANE	21.797	686545	8.057 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF070122\
Data File : FF010947.D
Signal(s) : FID2B.ch
Acq On : 01 Jul 2022 08:50
Operator : AJ\MA
Sample : MECL2
Misc :
ALS Vial : 51 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Jul 02 02:56:48 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF063022.M
Quant Title :
QLast Update : Fri Jul 01 01:40:42 2022
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

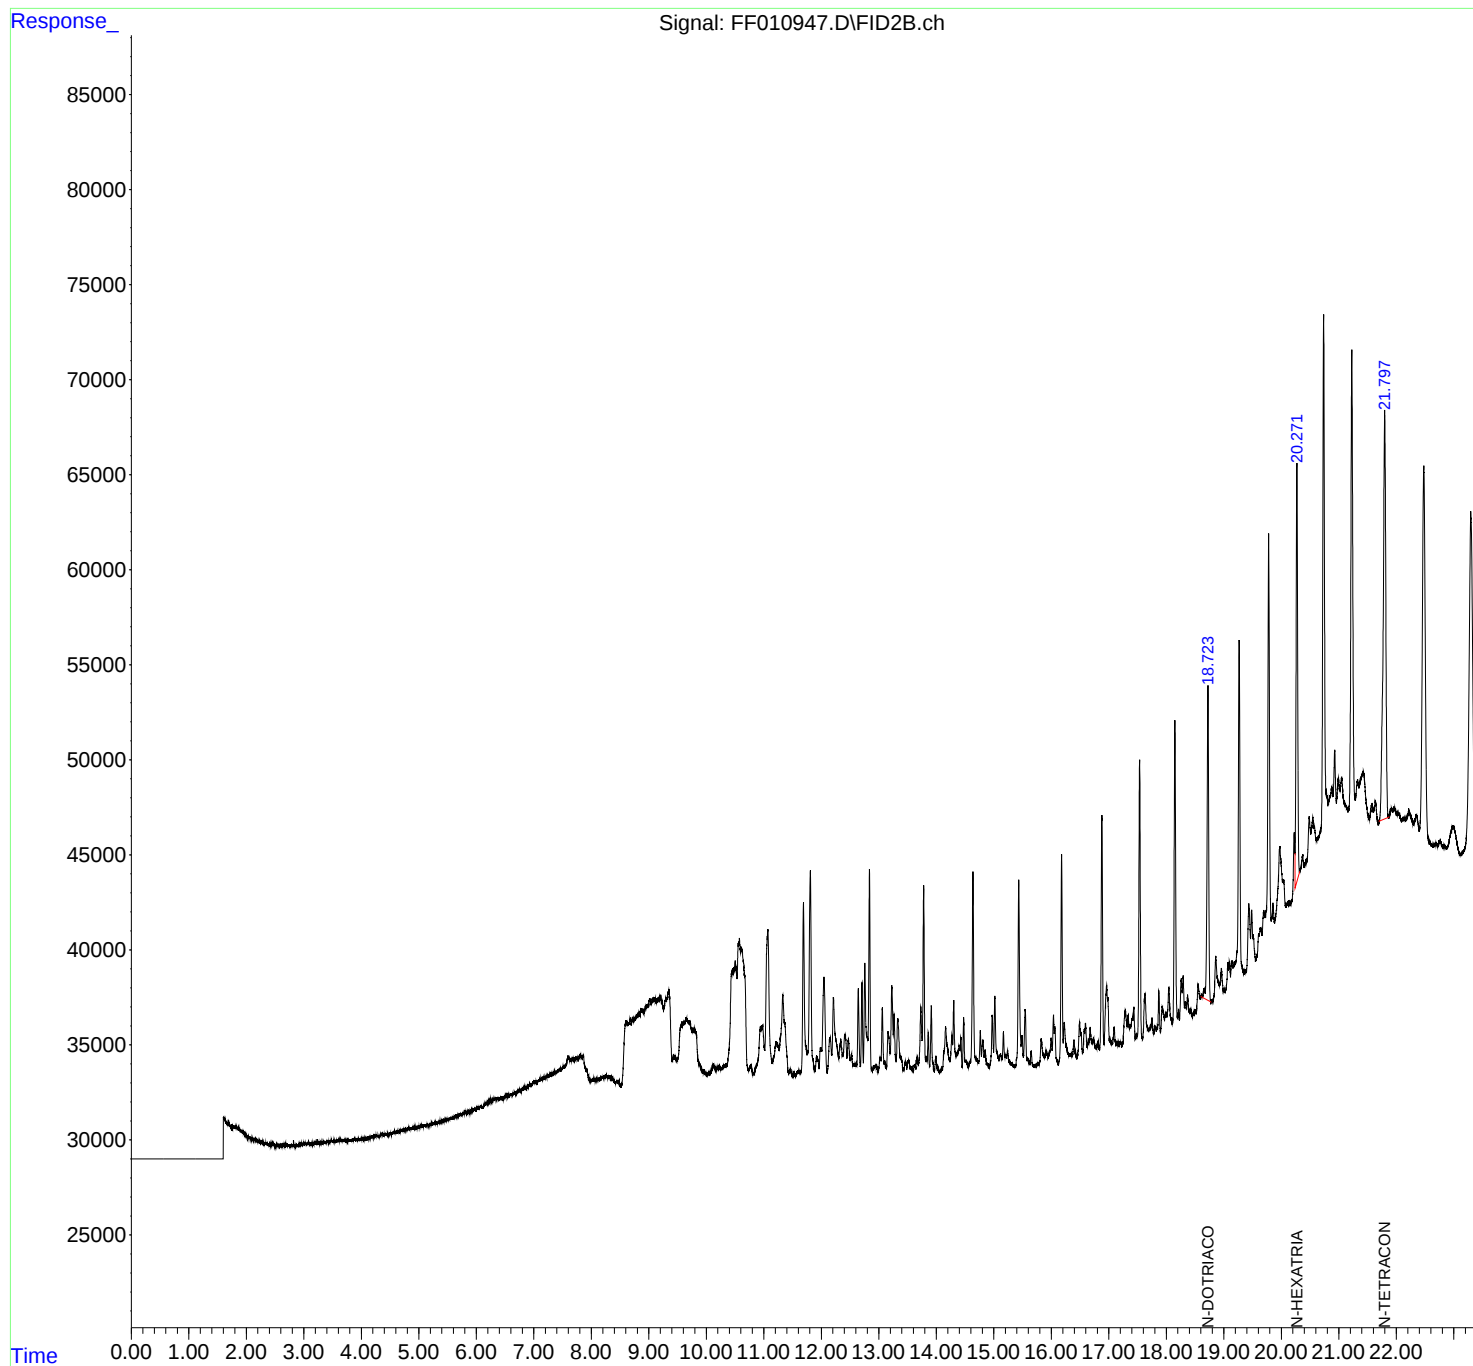

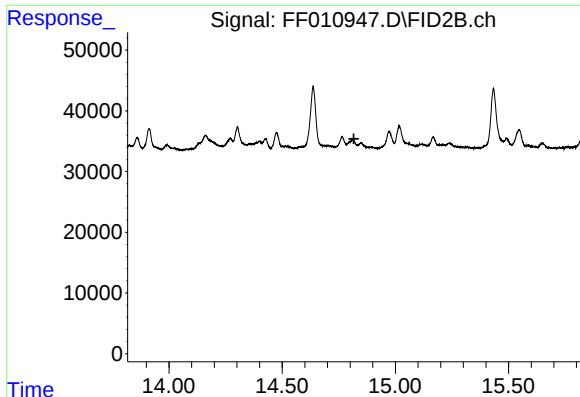


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T.: 14.817 min
Response: 0
Conc: N.D.

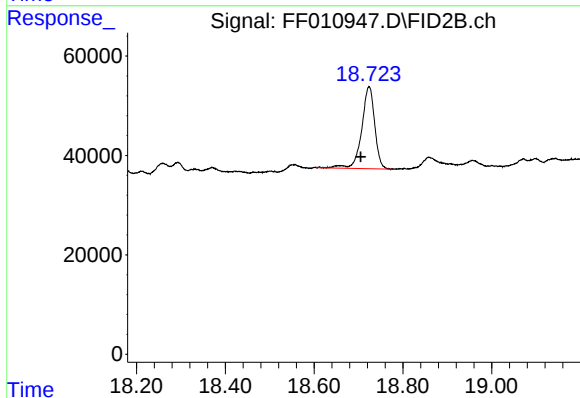


#14 N-DOTRIACONTANE

R.T.: 18.724 min
Delta R.T.: 0.019 min
Response: 334996
Conc: 3.12 ug/ml

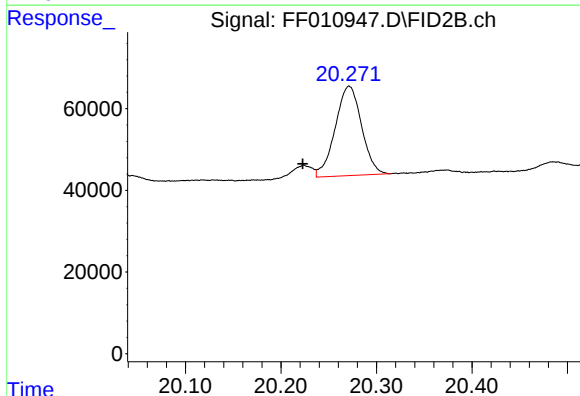

#16 N-HEXATRIACONTANE

R.T.: 20.271 min
Delta R.T.: 0.049 min
Response: 419976
Conc: 4.88 ug/ml

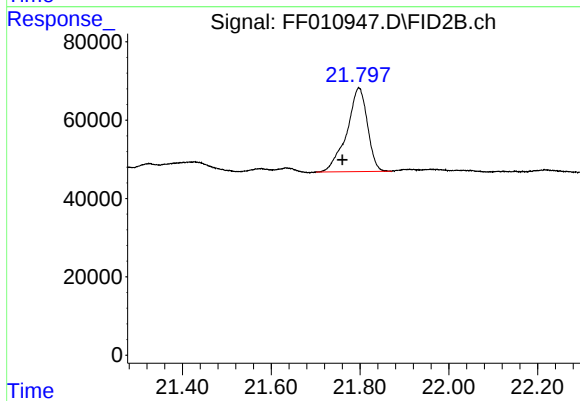

#18 N-TETRACONTANE

R.T.: 21.797 min
Delta R.T.: 0.037 min
Response: 686545
Conc: 8.06 ug/ml