

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF070218\
 Data File : FF001186.D
 Signal(s) : FID2B.ch
 Acq On : 02 Jul 2018 12:12
 Operator : UA\AJ
 Sample : 50 TRPH STD
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Jul 02 13:21:39 2018
 Quant Method : Z:\PESTPCBSRV\HPCHEM1\FID_F\Method\FF070218.M
 Quant Title :
 QLast Update : Mon Jul 02 13:21:18 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.467	5445286	50.000 ug/ml
Target Compounds			
1) N-OCTANE	2.151	6395853	50.000 ug/ml
2) N-DECANE	4.231	6384721	50.000 ug/ml
3) N-DODECANE	6.244	6410029	50.000 ug/ml
4) N-TETRADECANE	8.033	6407367	50.000 ug/ml
5) N-HEXADECANE	9.628	6377709	50.000 ug/ml
6) N-OCTADECANE	11.066	6378618	50.000 ug/ml
7) N-EICOSANE	12.374	6308454	50.000 ug/ml
8) N-DOCOSANE	13.569	6244561	50.000 ug/ml
10) N-TETRACOSANE	14.671	6175262	50.000 ug/ml
11) N-HEXACOSANE	15.689	6132806	50.000 ug/ml
12) N-OCTACOSANE	16.637	6083057	50.000 ug/ml
13) N-TRIACONTANE	17.523	6041941	50.000 ug/ml
14) N-DOTRIACONTANE	18.353	5906352	50.000 ug/ml
15) N-TETRATRIACONTANE	19.137	5889257	50.000 ug/ml
16) N-HEXATRIACONTANE	19.877	5698314	50.000 ug/ml
17) N-OCTATRIACONTANE	20.589	5163515	50.000 ug/ml
18) N-TETRACONTANE	21.421	5155397	50.000 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF070218\
Data File : FF001186.D
Signal(s) : FID2B.ch
Acq On : 02 Jul 2018 12:12
Operator : UA\AJ
Sample : 50 TRPH STD
Misc :
ALS Vial : 4 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Jul 02 13:21:39 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\FID_F\Method\FF070218.M
Quant Title :
QLast Update : Mon Jul 02 13:21:18 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

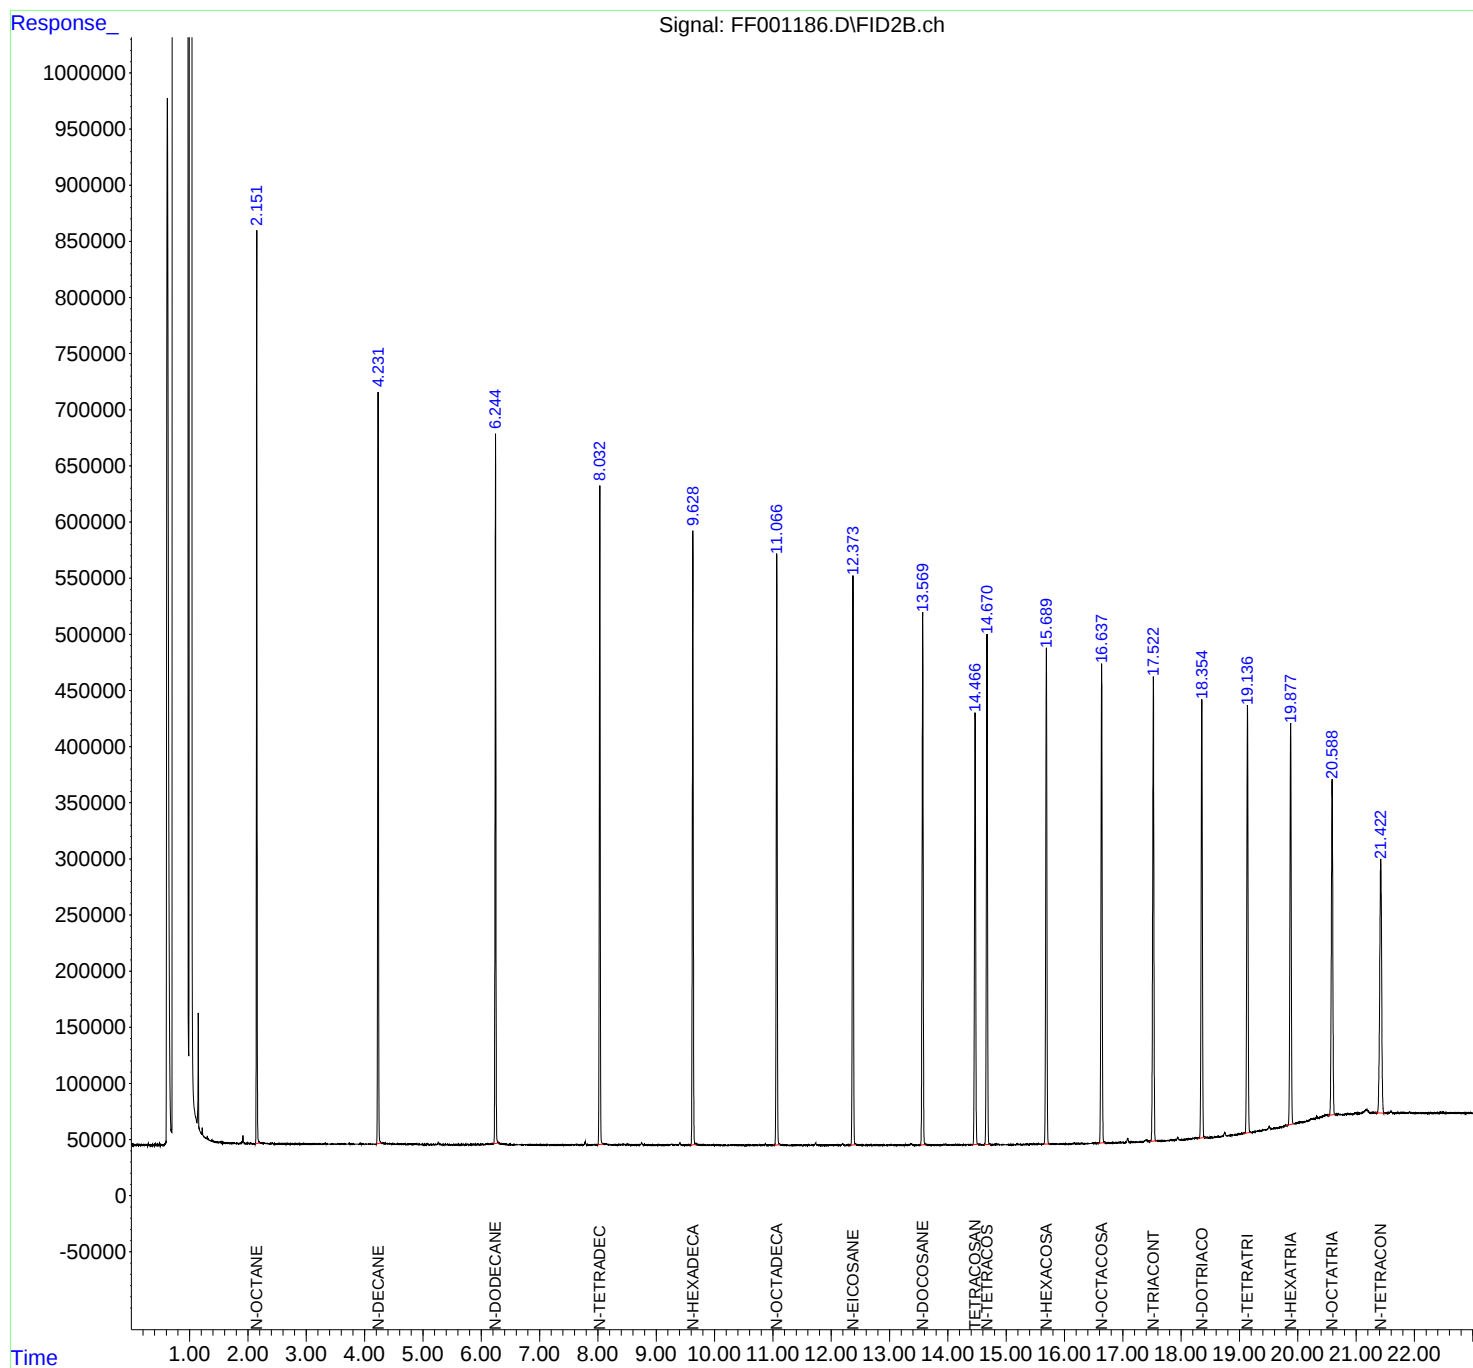

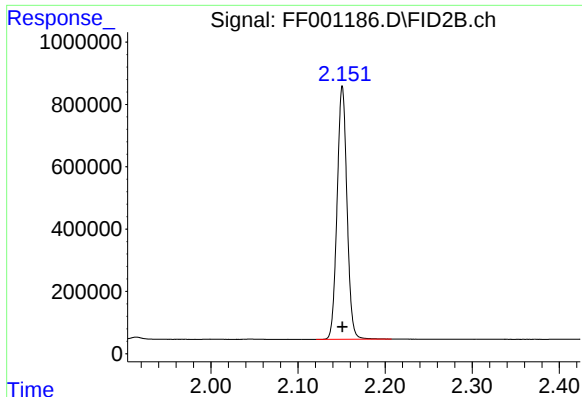


#1 N-OCTANE

R.T.: 2.151 min
Delta R.T.: 0.000 min
Response: 6395853
Conc: 50.00 ug/ml

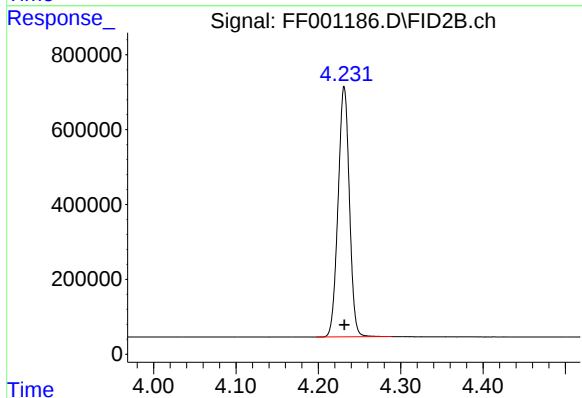


#2 N-DECANE

R.T.: 4.231 min
Delta R.T.: 0.000 min
Response: 6384721
Conc: 50.00 ug/ml

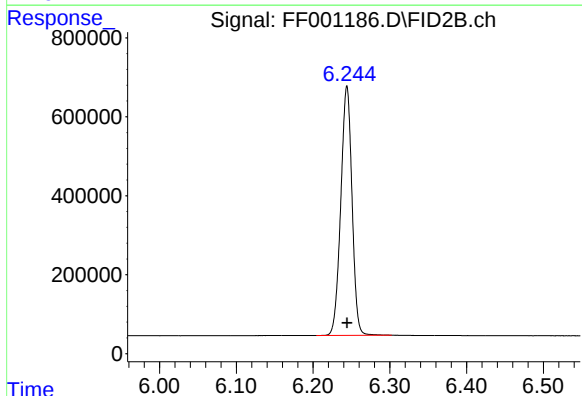


#3 N-DODECANE

R.T.: 6.244 min
Delta R.T.: 0.000 min
Response: 6410029
Conc: 50.00 ug/ml

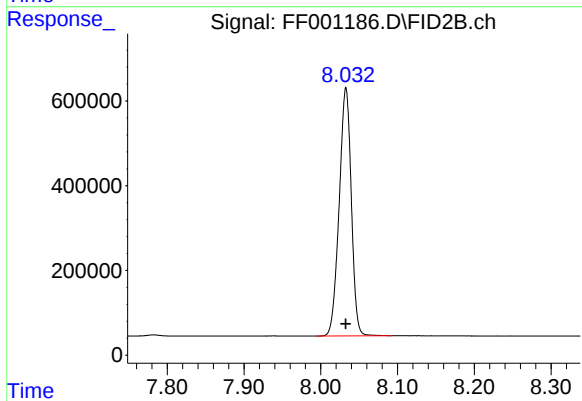


#4 N-TETRADECANE

R.T.: 8.033 min
Delta R.T.: 0.000 min
Response: 6407367
Conc: 50.00 ug/ml

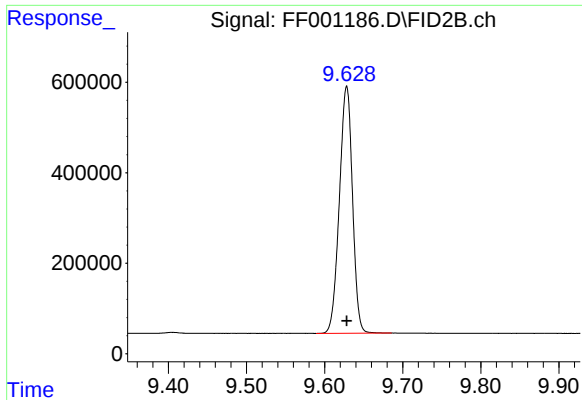


#5 N-HEXADECANE

R.T.: 9.628 min
Delta R.T.: 0.000 min
Response: 6377709
Conc: 50.00 ug/ml

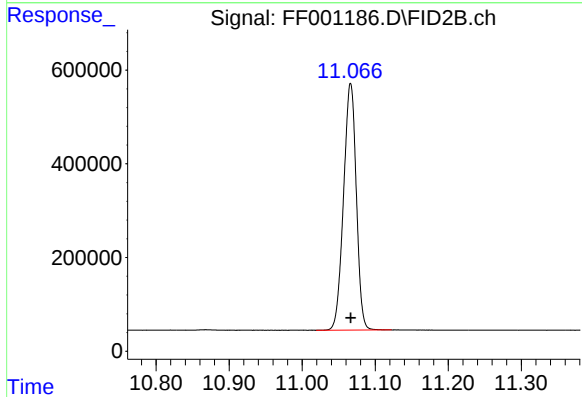


#6 N-OCTADECANE

R.T.: 11.066 min
Delta R.T.: 0.000 min
Response: 6378618
Conc: 50.00 ug/ml

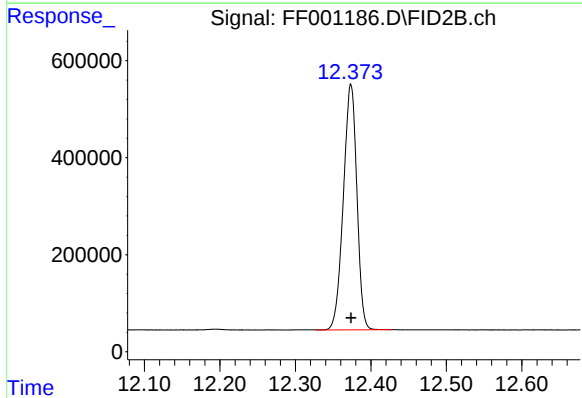


#7 N-EICOSANE

R.T.: 12.374 min
Delta R.T.: 0.000 min
Response: 6308454
Conc: 50.00 ug/ml

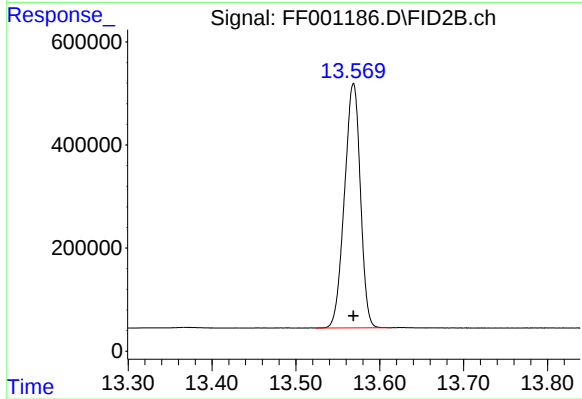


#8 N-DOCOSANE

R.T.: 13.569 min
Delta R.T.: 0.000 min
Response: 6244561
Conc: 50.00 ug/ml

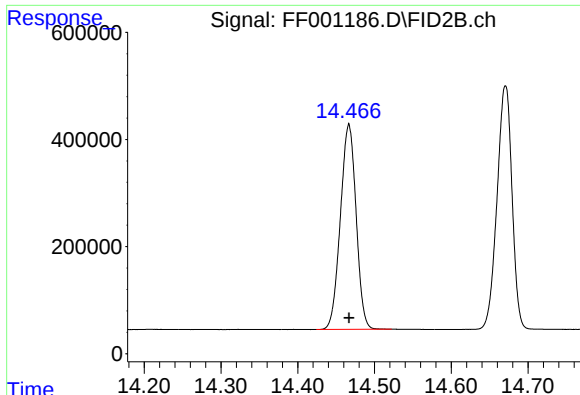


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.467 min
Delta R.T.: 0.000 min
Response: 5445286
Conc: 50.00 ug/ml

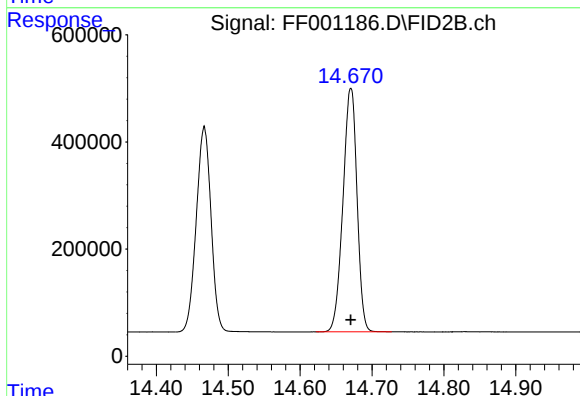


#10 N-TETRACOSANE

R.T.: 14.671 min
Delta R.T.: 0.000 min
Response: 6175262
Conc: 50.00 ug/ml

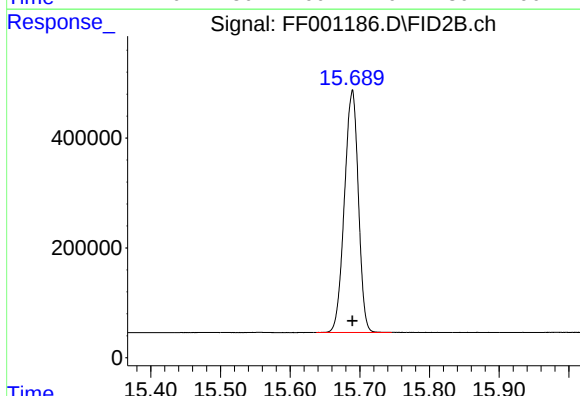


#11 N-HEXACOSANE

R.T.: 15.689 min
Delta R.T.: 0.000 min
Response: 6132806
Conc: 50.00 ug/ml

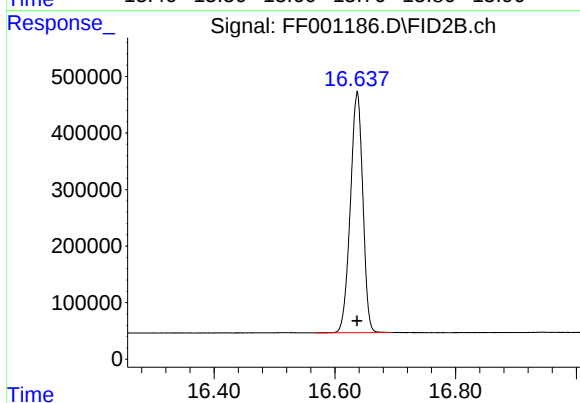


#12 N-OCTACOSANE

R.T.: 16.637 min
Delta R.T.: 0.000 min
Response: 6083057
Conc: 50.00 ug/ml

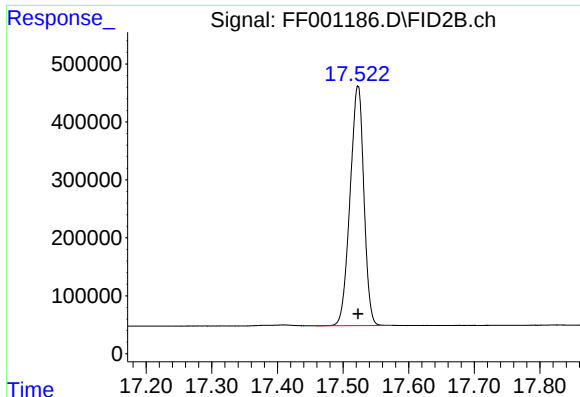


#13 N-TRIACONTANE

R.T.: 17.523 min
Delta R.T.: 0.000 min
Response: 6041941
Conc: 50.00 ug/ml

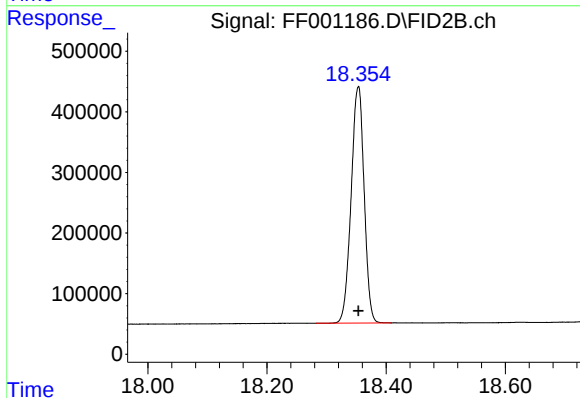


#14 N-DOTRIACONTANE

R.T.: 18.353 min
Delta R.T.: 0.000 min
Response: 5906352
Conc: 50.00 ug/ml

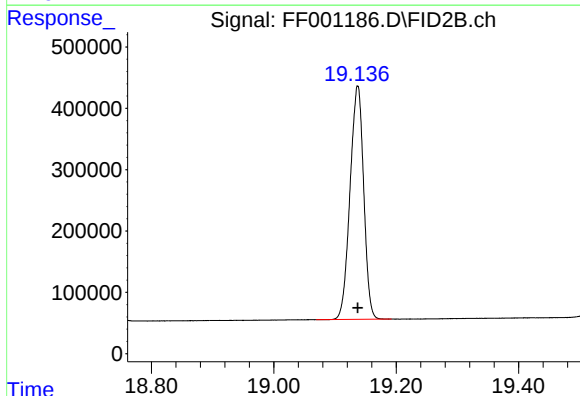


#15 N-TETRATRIACONTANE

R.T.: 19.137 min
Delta R.T.: 0.000 min
Response: 5889257
Conc: 50.00 ug/ml

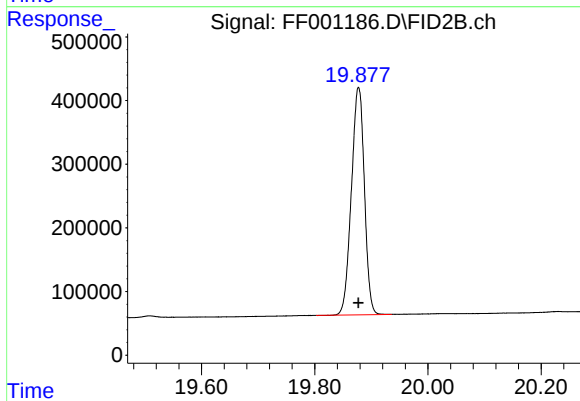


#16 N-HEXATRIACONTANE

R.T.: 19.877 min
Delta R.T.: 0.000 min
Response: 5698314
Conc: 50.00 ug/ml

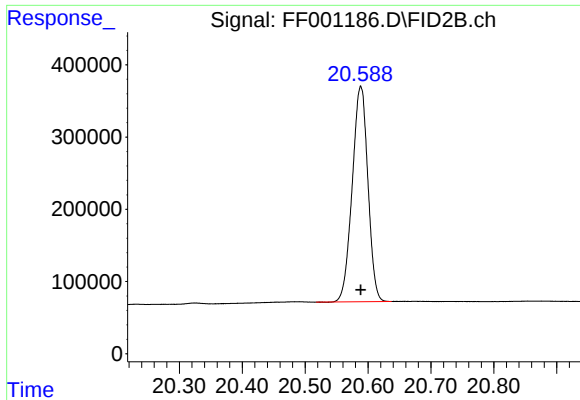

#17 N-OCTATRIACONTANE

R.T.: 20.589 min
Delta R.T.: 0.000 min
Response: 5163515
Conc: 50.00 ug/ml

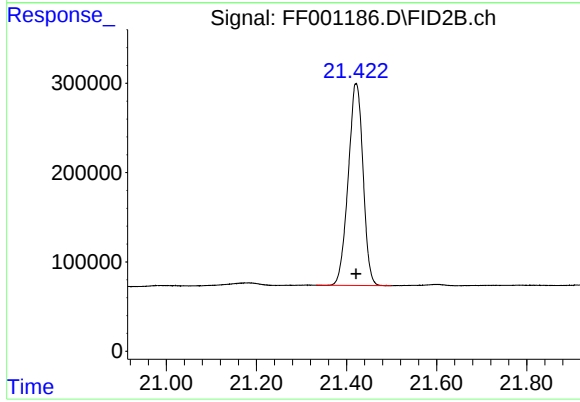

#18 N-TETRACONTANE

R.T.: 21.421 min
Delta R.T.: 0.000 min
Response: 5155397
Conc: 50.00 ug/ml