

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF070219\
Data File : FF004927.D
Signal(s) : FID2B.ch
Acq On : 02 Jul 2019 16:39
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jul 03 00:57:01 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF062619.M
Quant Title :
QLast Update : Wed Jun 26 14:27:24 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.689	2166405	22.275 ug/ml
Target Compounds			
16) N-HEXATRIACONTANE	20.189	97147	0.938 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF070219\
Data File : FF004927.D
Signal(s) : FID2B.ch
Acq On : 02 Jul 2019 16:39
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jul 03 00:57:01 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF062619.M
Quant Title :
QLast Update : Wed Jun 26 14:27:24 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

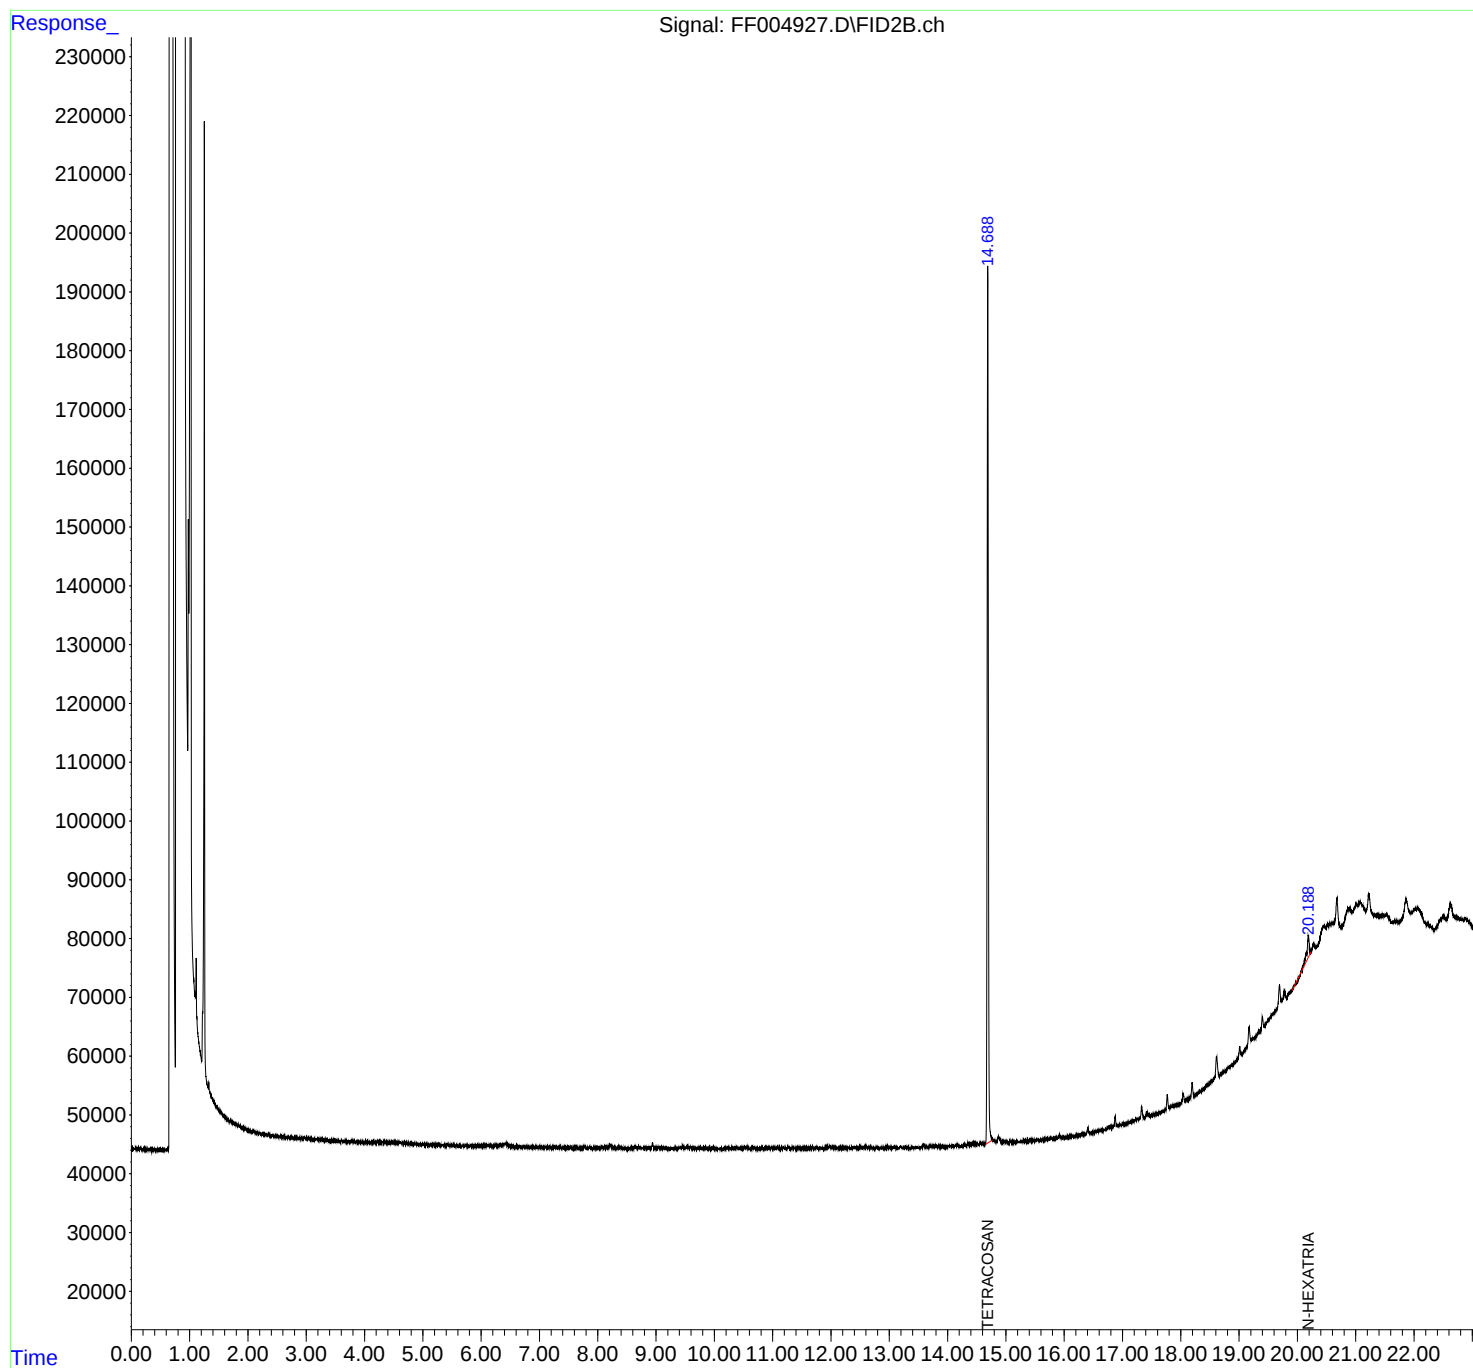


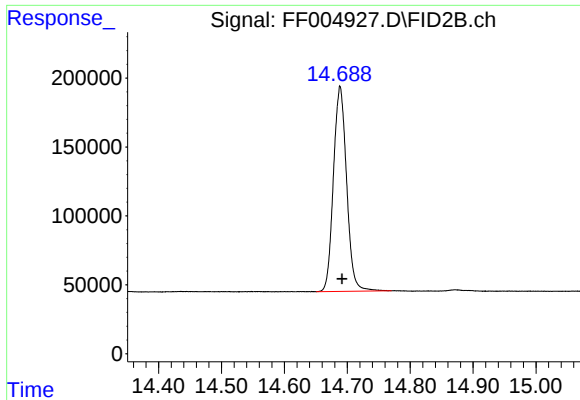

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.689 min
Delta R.T.: -0.003 min
Response: 2166405
Conc: 22.27 ug/ml

Instrument :
FID_F
ClientSampleId :

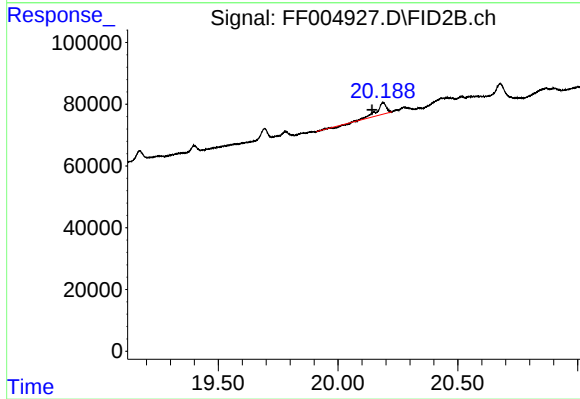

#16 N-HEXATRIACONTANE

R.T.: 20.189 min
Delta R.T.: 0.047 min
Response: 97147
Conc: 0.94 ug/ml