

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF070219\
Data File : FF004929.D
Signal(s) : FID2B.ch
Acq On : 02 Jul 2019 17:38
Operator : DD\AJ
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
RT MARKER

Integration File: autoint1.e
Quant Time: Jul 03 00:57:43 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF062619.M
Quant Title :
QLast Update : Wed Jun 26 14:27:24 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds

3)	N-DODECANE	6.425	6700522	52.809 ug/ml
12)	N-OCTACOSANE	16.876	6443696	57.771 ug/ml
13)	N-TRIACONTANE	17.766	415536	3.699 ug/ml
14)	N-DOTRIACONTANE	18.604	459381	4.033 ug/ml
15)	N-TETRATRIACONTANE	19.395	353175	3.254 ug/ml
16)	N-HEXATRIACONTANE	20.144	153504	1.482 ug/ml
17)	N-OCTATRIACONTANE	20.896	146206	1.533 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF070219\
Data File : FF004929.D
Signal(s) : FID2B.ch
Acq On : 02 Jul 2019 17:38
Operator : DD\AJ
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
RT MARKER

Integration File: autoint1.e
Quant Time: Jul 03 00:57:43 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF062619.M
Quant Title :
QLast Update : Wed Jun 26 14:27:24 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

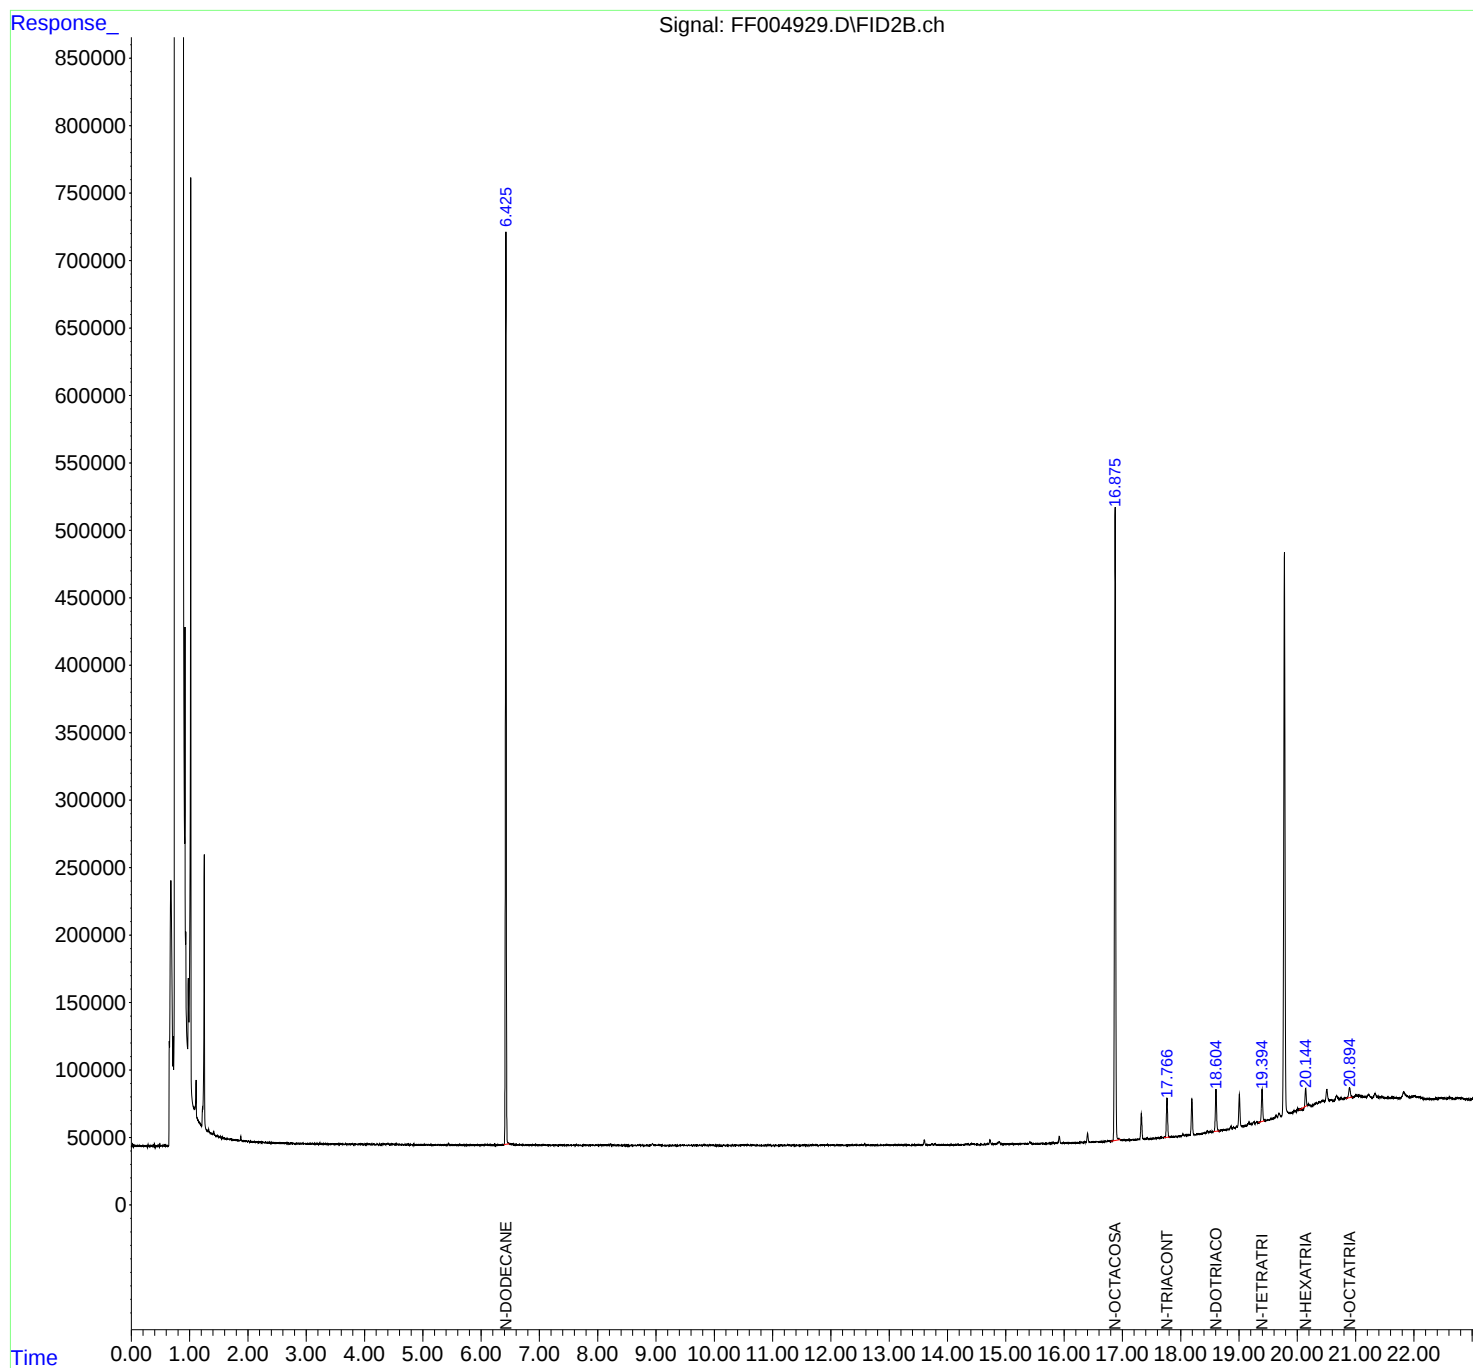


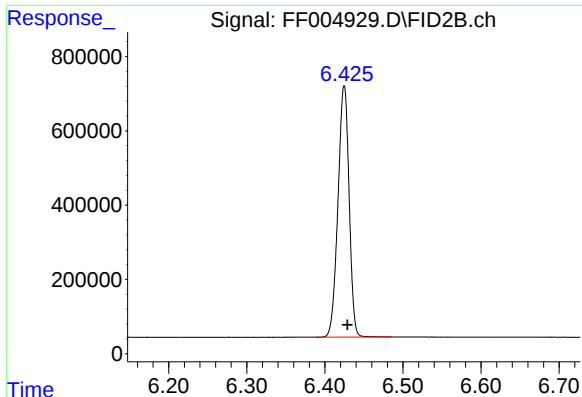

#3 N-DODECANE


R.T.: 6.425 min
Delta R.T.: -0.004 min
Response: 6700522
Conc: 52.81 ug/ml

Instrument :
FID_F
ClientSampleId :
RT MARKER

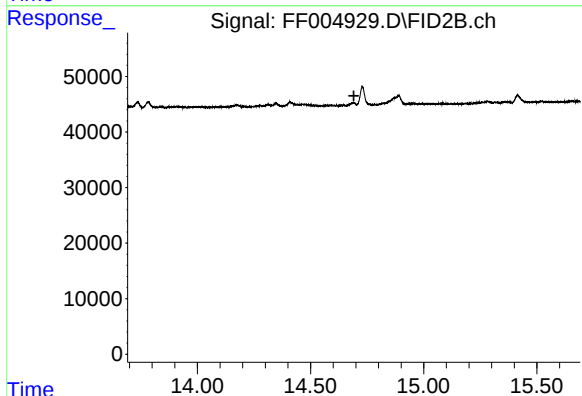


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.692 min
Response: 0
Conc: N.D.

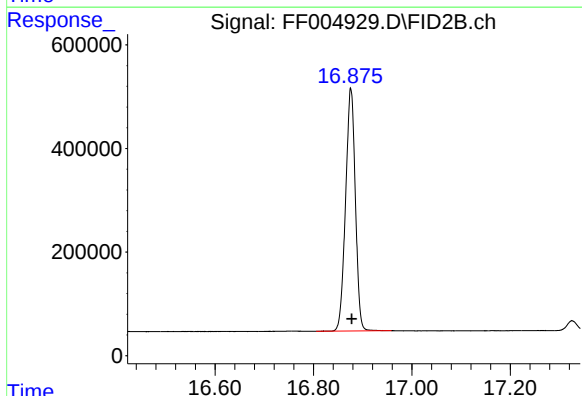


#12 N-OCTACOSANE

R.T.: 16.876 min
Delta R.T.: -0.002 min
Response: 6443696
Conc: 57.77 ug/ml

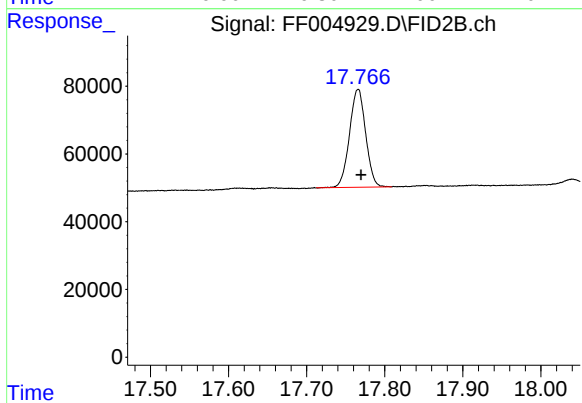

#13 N-TRIACONTANE


R.T.: 17.766 min
Delta R.T.: -0.004 min
Response: 415536
Conc: 3.70 ug/ml

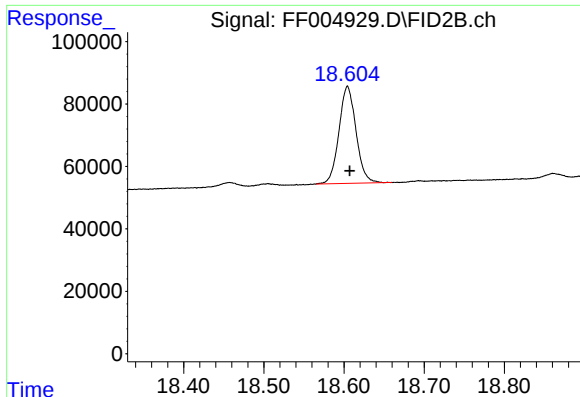

#14 N-DOTRIACONTANE


R.T.: 18.604 min
Delta R.T.: -0.003 min
Response: 459381
Conc: 4.03 ug/ml

Instrument :
FID_F
ClientSampleId :
RT MARKER

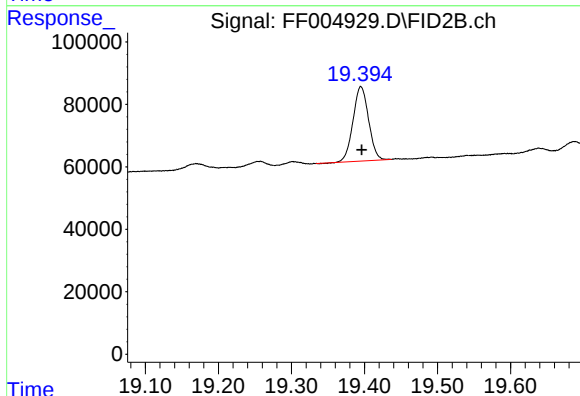


#15 N-TETRATRIACONTANE

R.T.: 19.395 min
Delta R.T.: -0.001 min
Response: 353175
Conc: 3.25 ug/ml

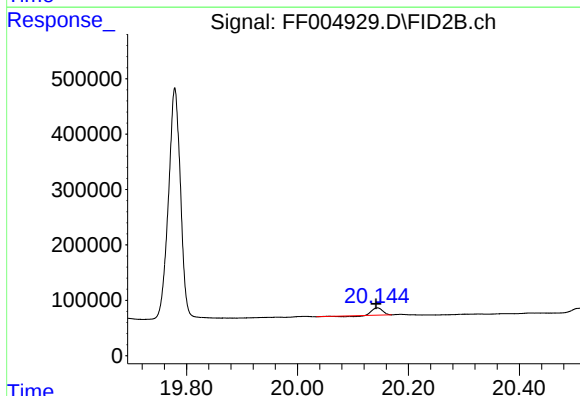

#16 N-HEXATRIACONTANE

R.T.: 20.144 min
Delta R.T.: 0.003 min
Response: 153504
Conc: 1.48 ug/ml

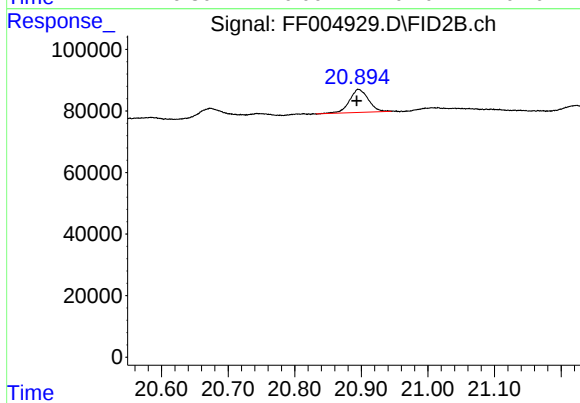

#17 N-OCTATRIACONTANE

R.T.: 20.896 min
Delta R.T.: 0.003 min
Response: 146206
Conc: 1.53 ug/ml