

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF070219\
 Data File : FF004931.D
 Signal(s) : FID2B.ch
 Acq On : 02 Jul 2019 18:38
 Operator : DD\AJ
 Sample : K3160-11 20X
 Misc :
 ALS Vial : 56 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :
 EO-01-062819-C

Integration File: autoint1.e
 Quant Time: Jul 03 00:58:30 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF062619.M
 Quant Title :
 QLast Update : Wed Jun 26 14:27:24 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
3) N-DODECANE	6.422	208273	1.641 ug/ml
4) N-TETRADECANE	8.217	301503	2.410 ug/ml
5) N-HEXADECANE	9.820	271015	2.195 ug/ml
6) N-OCTADECANE	11.265	226101	1.909 ug/ml
7) N-EICOSANE	12.579	174604	1.505 ug/ml
8) N-DOCOSANE	13.783	102735	0.913 ug/ml
10) N-TETRACOSANE	14.888	149725	1.345 ug/ml
12) N-OCTACOSANE	16.873	94279	0.845 ug/ml
13) N-TRIACONTANE	17.765	271984	2.421 ug/ml
14) N-DOTRIACONTANE	18.604	225068	1.976 ug/ml
15) N-TETRATRIACONTANE	19.396	135524	1.249 ug/ml
16) N-HEXATRIACONTANE	20.142	258069	2.492 ug/ml
17) N-OCTATRIACONTANE	20.899	211791	2.221 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF070219\
Data File : FF004931.D
Signal(s) : FID2B.ch
Acq On : 02 Jul 2019 18:38
Operator : DD\AJ
Sample : K3160-11 20X
Misc :
ALS Vial : 56 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
EO-01-062819-C

Integration File: autoint1.e
Quant Time: Jul 03 00:58:30 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF062619.M
Quant Title :
QLast Update : Wed Jun 26 14:27:24 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

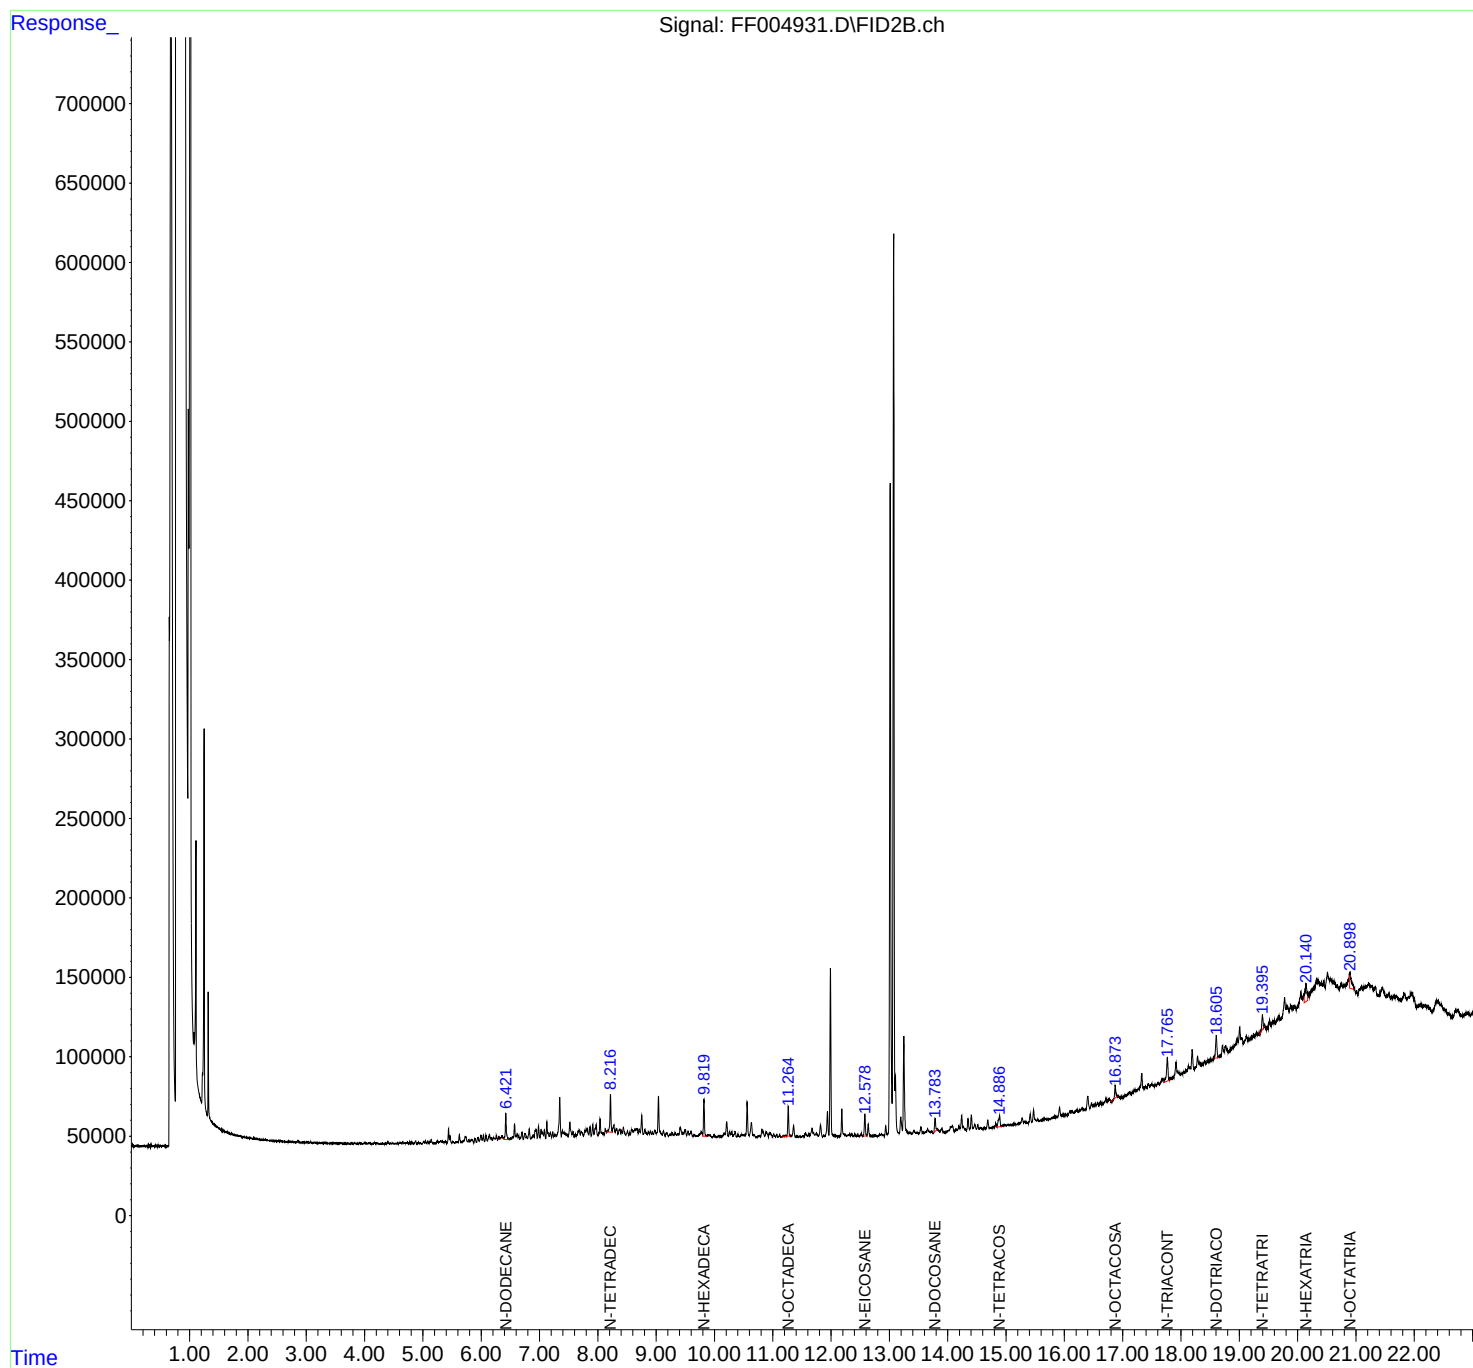


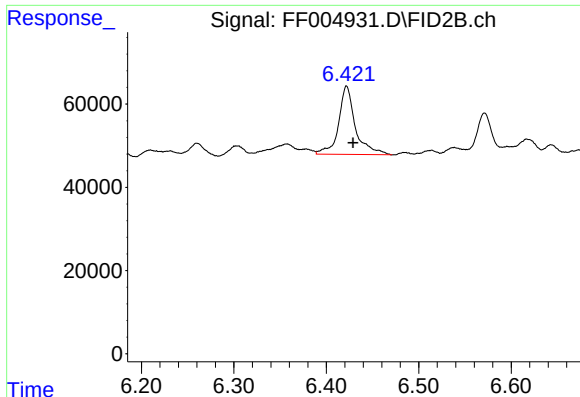

#3 N-DODECANE


R.T.: 6.422 min
Delta R.T.: -0.007 min
Response: 208273
Conc: 1.64 ug/ml

Instrument :
FID_F
ClientSampleId :
EO-01-062819-C

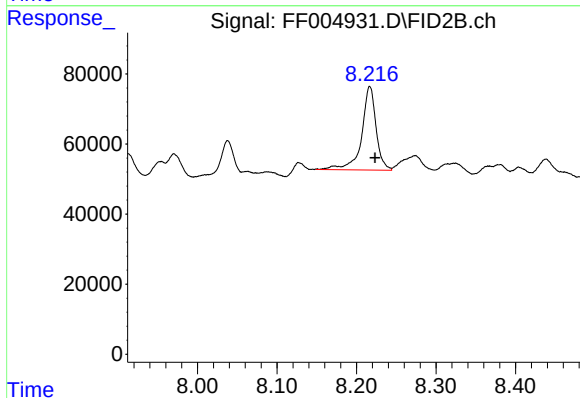


#4 N-TETRADECANE

R.T.: 8.217 min
Delta R.T.: -0.007 min
Response: 301503
Conc: 2.41 ug/ml

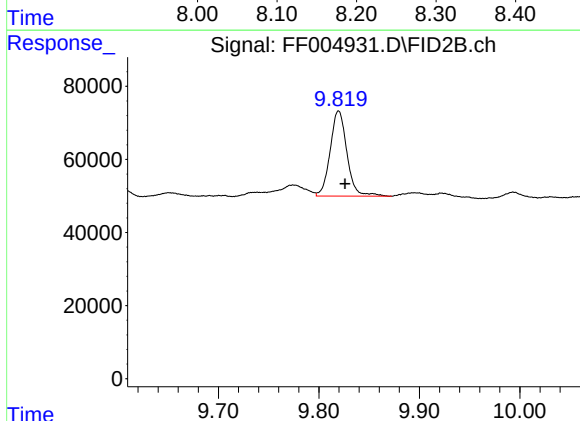


#5 N-HEXADECANE

R.T.: 9.820 min
Delta R.T.: -0.006 min
Response: 271015
Conc: 2.19 ug/ml

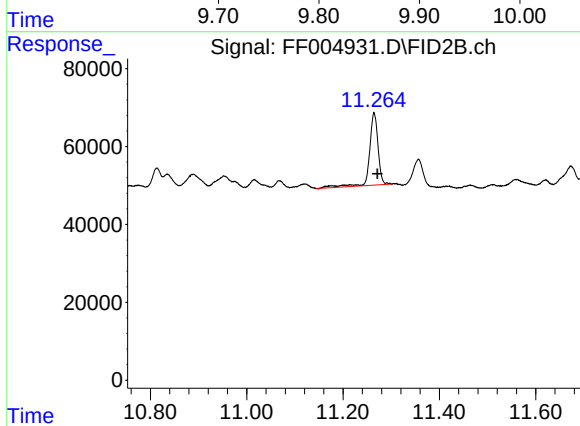

#6 N-OCTADECANE


R.T.: 11.265 min
Delta R.T.: -0.007 min
Response: 226101
Conc: 1.91 ug/ml

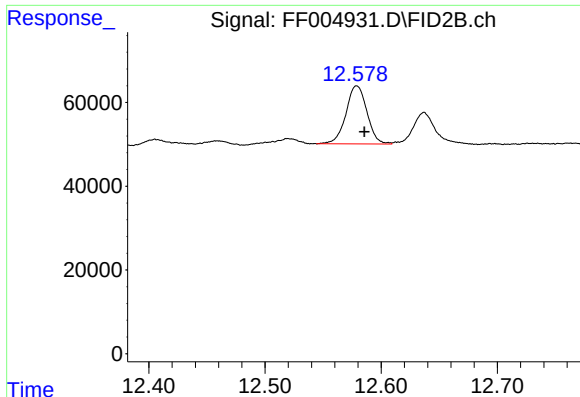

#7 N-EICOSANE


R.T.: 12.579 min
Delta R.T.: -0.006 min
Response: 174604
Conc: 1.50 ug/ml

Instrument :
FID_F
ClientSampleId :
EO-01-062819-C

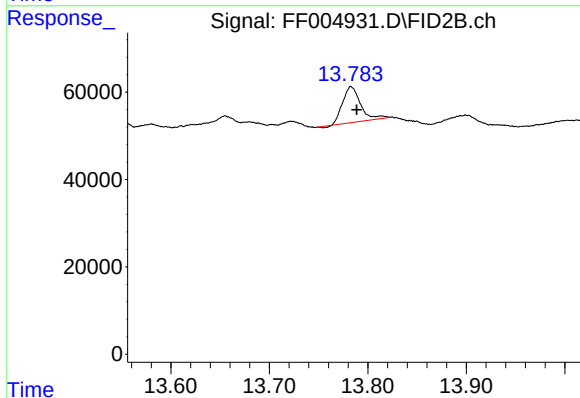


#8 N-DOCOSANE

R.T.: 13.783 min
Delta R.T.: -0.006 min
Response: 102735
Conc: 0.91 ug/ml

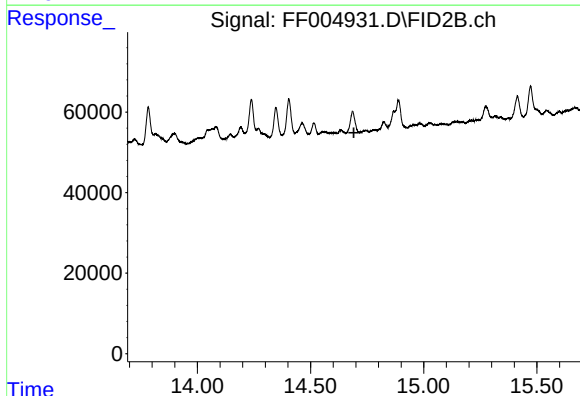


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.692 min
Response: 0
Conc: N.D.

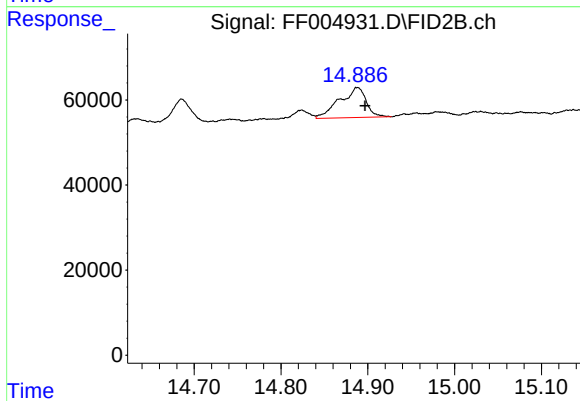

#10 N-TETRACOSANE


R.T.: 14.888 min
Delta R.T.: -0.009 min
Response: 149725
Conc: 1.35 ug/ml

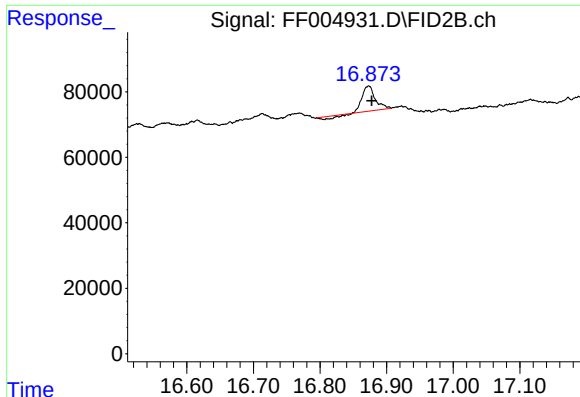

#12 N-OCTACOSANE


R.T.: 16.873 min
Delta R.T.: -0.005 min
Response: 94279
Conc: 0.85 ug/ml

Instrument :
FID_F
ClientSampleId :
EO-01-062819-C

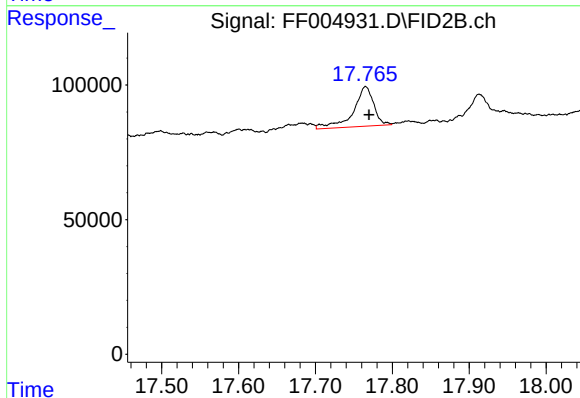


#13 N-TRIACONTANE

R.T.: 17.765 min
Delta R.T.: -0.005 min
Response: 271984
Conc: 2.42 ug/ml

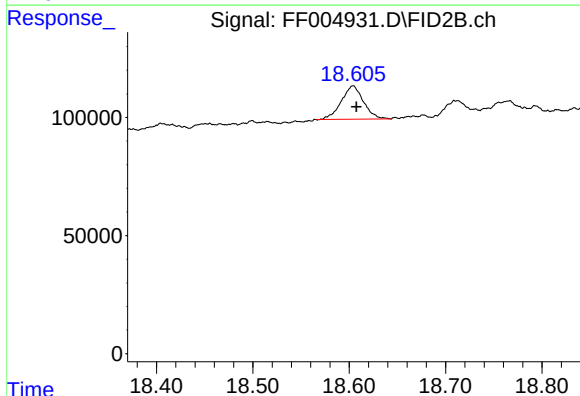


#14 N-DOTRIACONTANE

R.T.: 18.604 min
Delta R.T.: -0.003 min
Response: 225068
Conc: 1.98 ug/ml

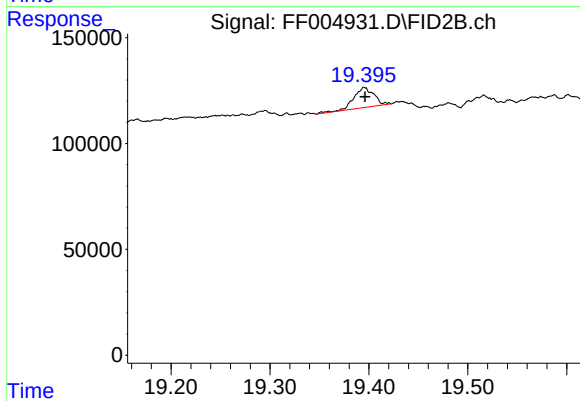

#15 N-TETRATRIACONTANE


R.T.: 19.396 min
Delta R.T.: 0.000 min
Response: 135524
Conc: 1.25 ug/ml

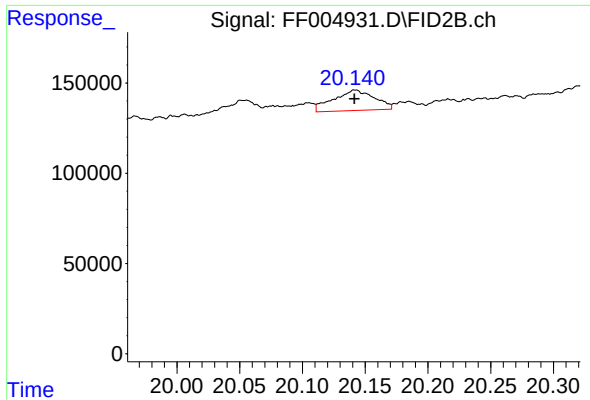

#16 N-HEXATRIACONTANE

R.T.: 20.142 min
Delta R.T.: 0.000 min
Response: 258069
Conc: 2.49 ug/ml

Instrument :
FID_F
ClientSampleId :
EO-01-062819-C

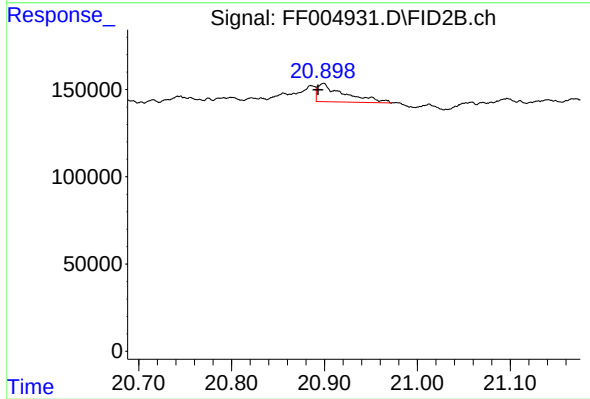

#17 N-OCTATRIACONTANE

R.T.: 20.899 min
Delta R.T.: 0.006 min
Response: 211791
Conc: 2.22 ug/ml