

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF070219\
 Data File : FF004933.D
 Signal(s) : FID2B.ch
 Acq On : 02 Jul 2019 19:37
 Operator : DD\AJ
 Sample : K3555-02
 Misc :
 ALS Vial : 58 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jul 03 00:59:06 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF062619.M
 Quant Title :
 QLast Update : Wed Jun 26 14:27:24 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.689	1444389	14.851 ug/ml
Target Compounds			
4) N-TETRADECANE	8.276f	488125	3.901 ug/ml
11) N-HEXACOSANE	15.920	140560	1.271 ug/ml
12) N-OCTACOSANE	16.875	341699	3.063 ug/ml
13) N-TRIACONTANE	17.768	435492	3.877 ug/ml
14) N-DOTRIACONTANE	18.608	281084	2.468 ug/ml
15) N-TETRATRIACONTANE	19.397	151936	1.400 ug/ml
16) N-HEXATRIACONTANE	20.141	173536	1.676 ug/ml
17) N-OCTATRIACONTANE	20.900	130322	1.366 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF070219\
Data File : FF004933.D
Signal(s) : FID2B.ch
Acq On : 02 Jul 2019 19:37
Operator : DD\AJ
Sample : K3555-02
Misc :
ALS Vial : 58 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jul 03 00:59:06 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF062619.M
Quant Title :
QLast Update : Wed Jun 26 14:27:24 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

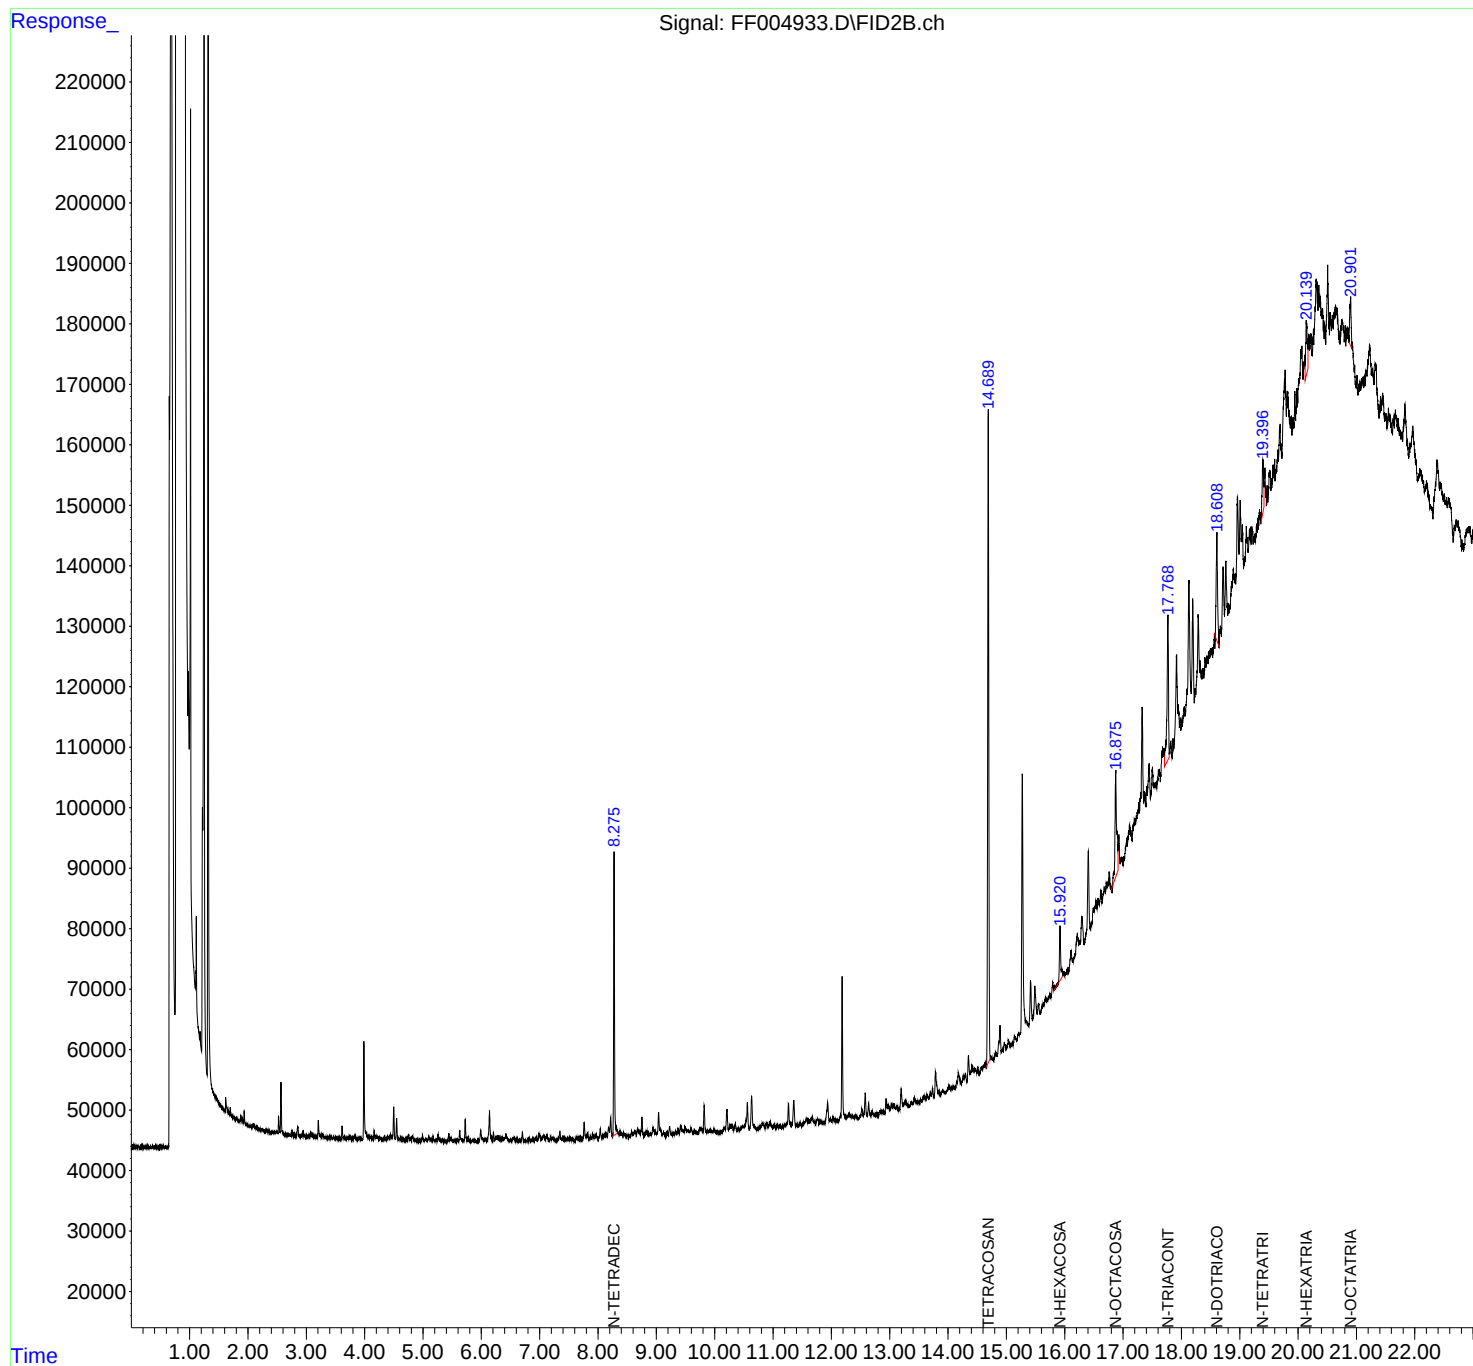


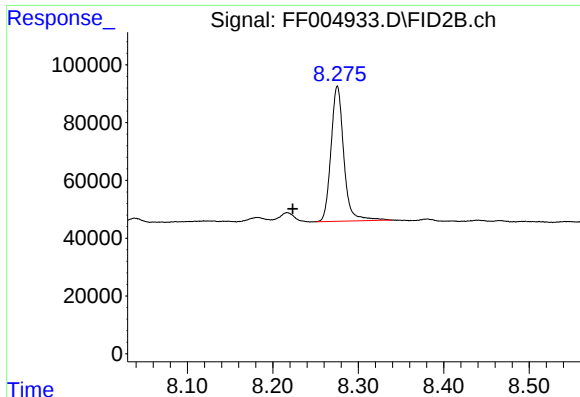

#4 N-TETRADECANE


R.T.: 8.276 min
Delta R.T.: 0.052 min
Response: 488125
Conc: 3.90 ug/ml

Instrument :
FID_F
ClientSampleId :

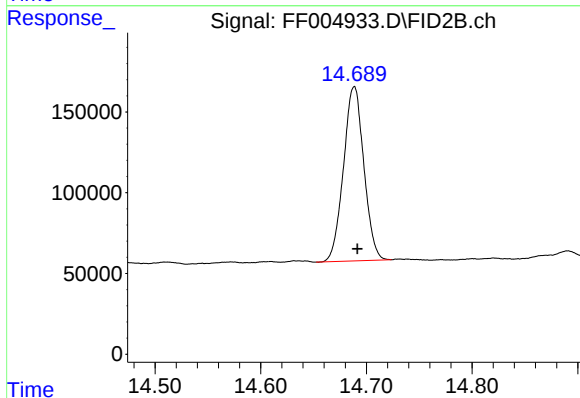


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.689 min
Delta R.T.: -0.003 min
Response: 1444389
Conc: 14.85 ug/ml

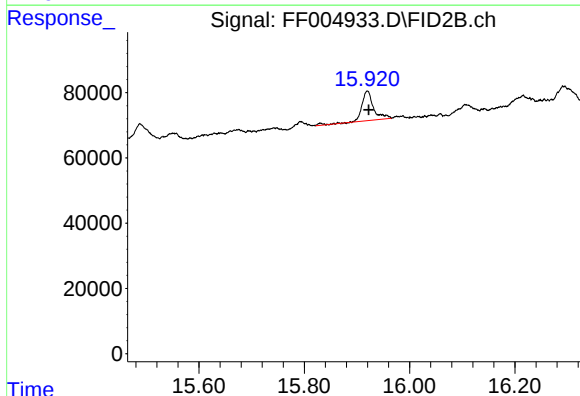


#11 N-HEXACOSANE

R.T.: 15.920 min
Delta R.T.: -0.002 min
Response: 140560
Conc: 1.27 ug/ml

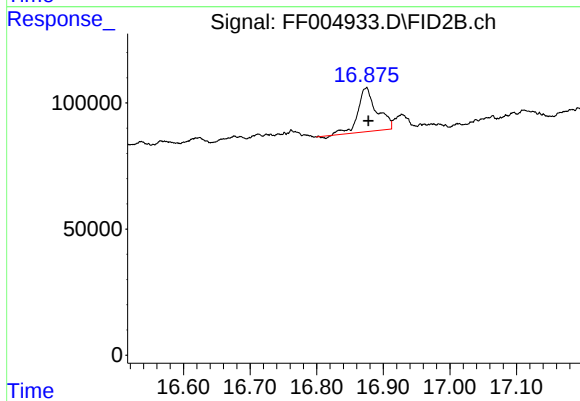

#12 N-OCTACOSANE


R.T.: 16.875 min
Delta R.T.: -0.003 min
Response: 341699
Conc: 3.06 ug/ml

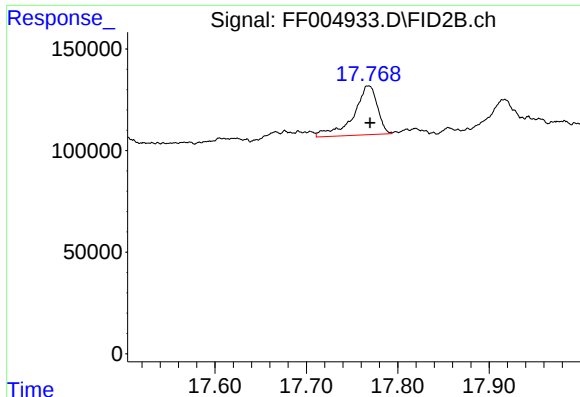

#13 N-TRIACONTANE


R.T.: 17.768 min
Delta R.T.: -0.002 min
Response: 435492
Conc: 3.88 ug/ml

Instrument :
FID_F
ClientSampleId :

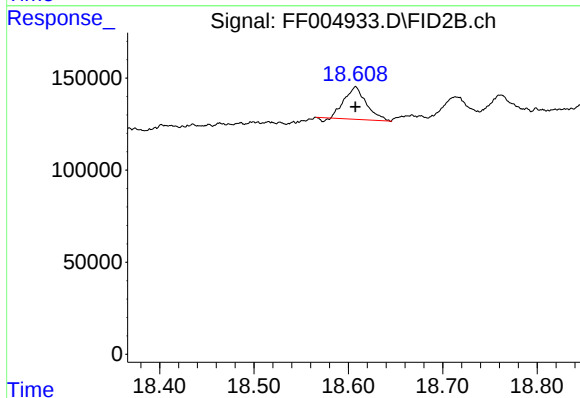


#14 N-DOTRIACONTANE

R.T.: 18.608 min
Delta R.T.: 0.000 min
Response: 281084
Conc: 2.47 ug/ml

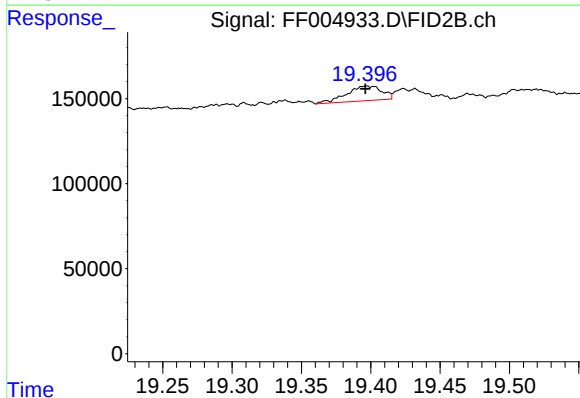


#15 N-TETRATRIACONTANE

R.T.: 19.397 min
Delta R.T.: 0.000 min
Response: 151936
Conc: 1.40 ug/ml

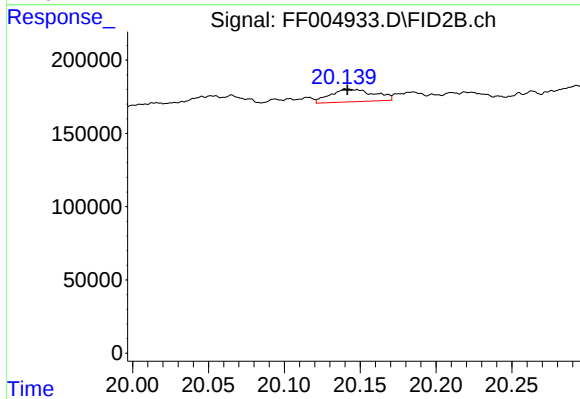

#16 N-HEXATRIACONTANE

R.T.: 20.141 min
Delta R.T.: 0.000 min
Response: 173536
Conc: 1.68 ug/ml

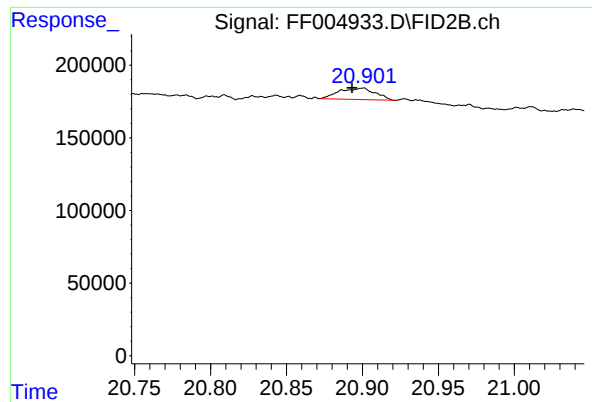

#17 N-OCTATRIACONTANE

R.T.: 20.900 min
Delta R.T.: 0.007 min
Response: 130322
Conc: 1.37 ug/ml

Instrument :
FID_F
ClientSampleId :