

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF070219\
 Data File : FF004935.D
 Signal(s) : FID2B.ch
 Acq On : 02 Jul 2019 20:36
 Operator : DD\AJ
 Sample : K3555-06
 Misc :
 ALS Vial : 60 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :
 SAMPLE-18

Integration File: autoint1.e
 Quant Time: Jul 03 00:59:29 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF062619.M
 Quant Title :
 QLast Update : Wed Jun 26 14:27:24 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.689	2225676	22.884 ug/ml
Target Compounds			
4) N-TETRADECANE	8.276f	623912	4.986 ug/ml
11) N-HEXACOSANE	15.918	110751	1.001 ug/ml
12) N-OCTACOSANE	16.872	196678	1.763 ug/ml
13) N-TRIACONTANE	17.765	271328	2.415 ug/ml
14) N-DOTRIACONTANE	18.605	216802	1.904 ug/ml
16) N-HEXATRIACONTANE	20.186	436224	4.213 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF070219\
Data File : FF004935.D
Signal(s) : FID2B.ch
Acq On : 02 Jul 2019 20:36
Operator : DD\AJ
Sample : K3555-06
Misc :
ALS Vial : 60 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
SAMPLE-18

Integration File: autoint1.e
Quant Time: Jul 03 00:59:29 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF062619.M
Quant Title :
QLast Update : Wed Jun 26 14:27:24 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

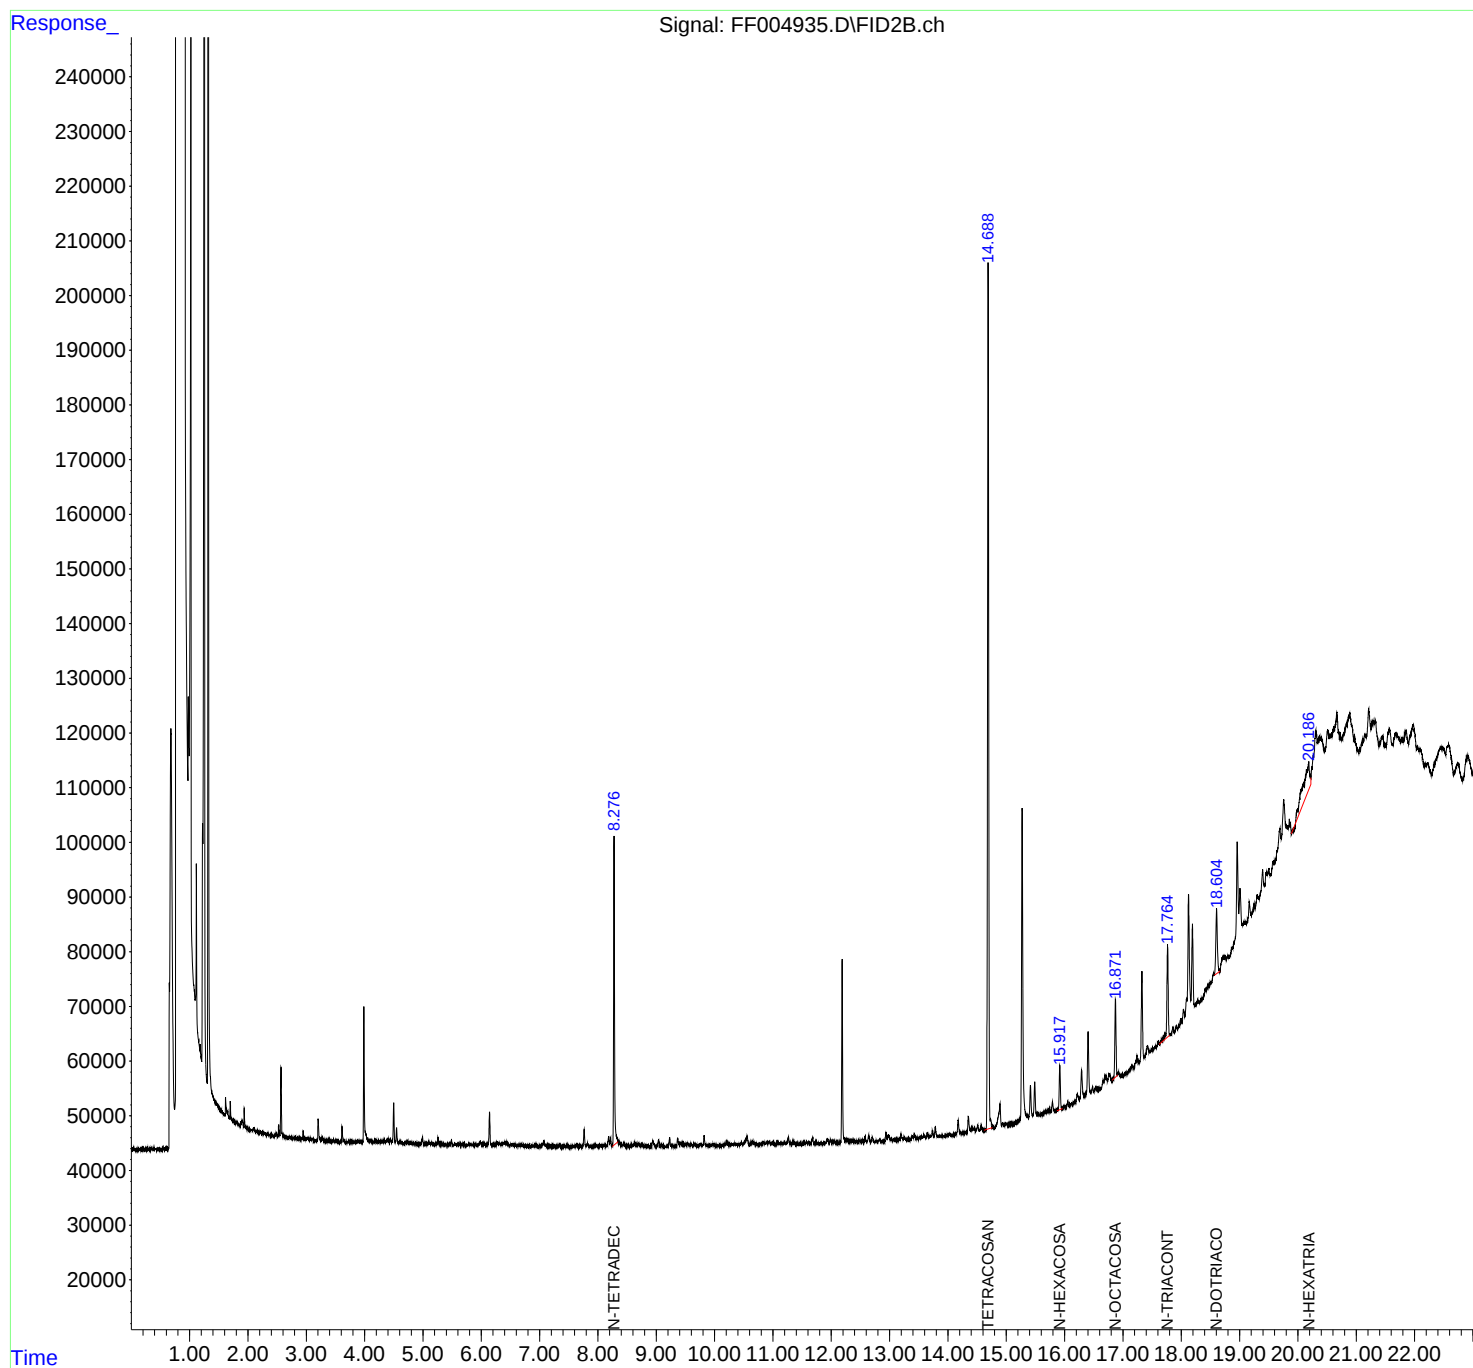


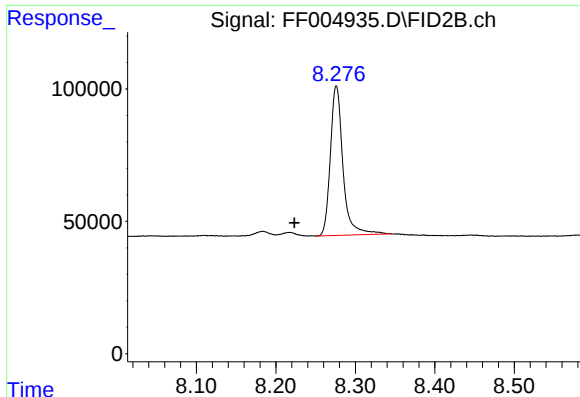

#4 N-TETRADECANE


R.T.: 8.276 min
Delta R.T.: 0.053 min
Response: 623912
Conc: 4.99 ug/ml

Instrument :
FID_F
ClientSampleId :
SAMPLE-18

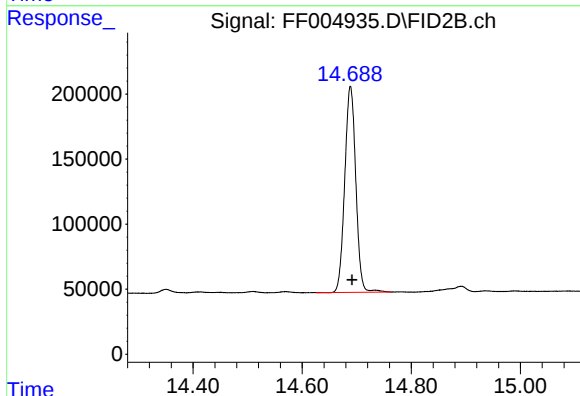


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.689 min
Delta R.T.: -0.003 min
Response: 2225676
Conc: 22.88 ug/ml

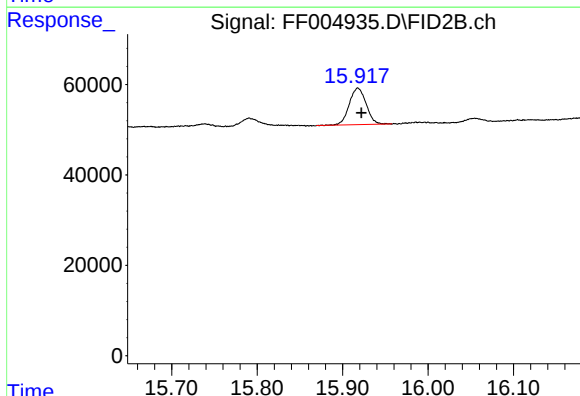


#11 N-HEXACOSANE

R.T.: 15.918 min
Delta R.T.: -0.004 min
Response: 110751
Conc: 1.00 ug/ml

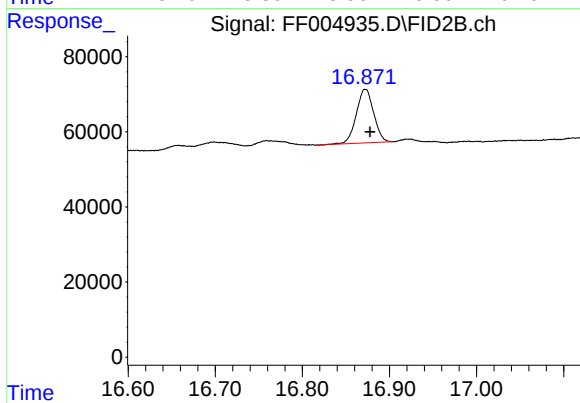

#12 N-OCTACOSANE


R.T.: 16.872 min
Delta R.T.: -0.005 min
Response: 196678
Conc: 1.76 ug/ml

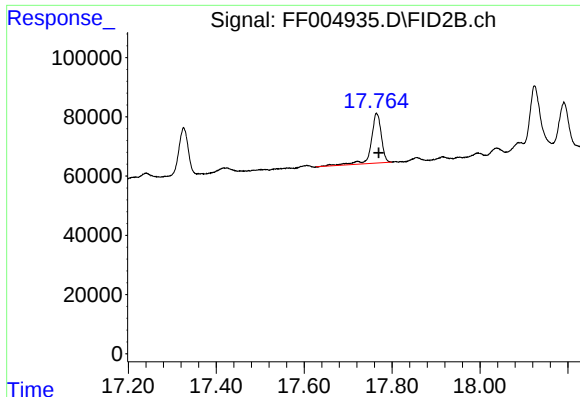

#13 N-TRIACONTANE


R.T.: 17.765 min
Delta R.T.: -0.005 min
Response: 271328
Conc: 2.42 ug/ml

Instrument :
FID_F
ClientSampleId :
SAMPLE-18

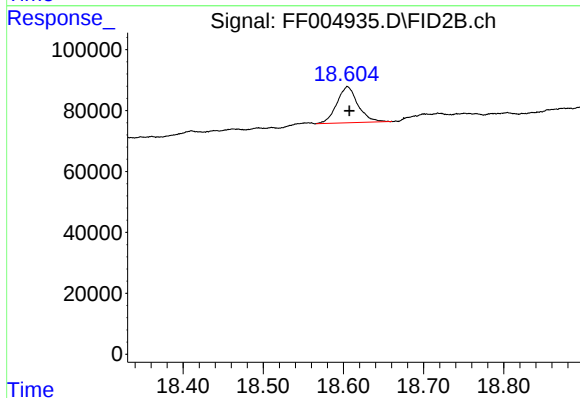

#14 N-DOTRIACONTANE

R.T.: 18.605 min
Delta R.T.: -0.002 min
Response: 216802
Conc: 1.90 ug/ml

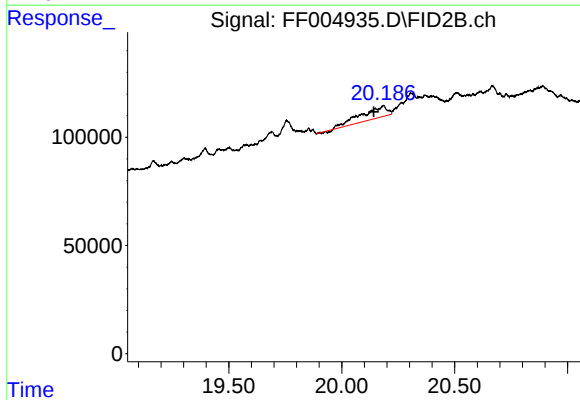

#16 N-HEXATRIACONTANE

R.T.: 20.186 min
Delta R.T.: 0.044 min
Response: 436224
Conc: 4.21 ug/ml