

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF070219\
 Data File : FF004936.D
 Signal(s) : FID2B.ch
 Acq On : 02 Jul 2019 21:05
 Operator : DD\AJ
 Sample : K3555-07
 Misc :
 ALS Vial : 61 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :
 SAMPLE-18A

Integration File: autoint1.e
 Quant Time: Jul 03 00:59:39 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF062619.M
 Quant Title :
 QLast Update : Wed Jun 26 14:27:24 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.688	1172316	12.054 ug/ml
Target Compounds			
4) N-TETRADECANE	8.276f	356257	2.847 ug/ml
12) N-OCTACOSANE	16.874	118635	1.064 ug/ml
13) N-TRIACONTANE	17.765	149362	1.330 ug/ml
14) N-DOTRIACONTANE	18.602	124941	1.097 ug/ml
16) N-HEXATRIACONTANE	20.177	340800	3.291 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF070219\
Data File : FF004936.D
Signal(s) : FID2B.ch
Acq On : 02 Jul 2019 21:05
Operator : DD\AJ
Sample : K3555-07
Misc :
ALS Vial : 61 Sample Multiplier: 1

Instrument :
FID_F
ClientSampled :
SAMPLE-18A

Integration File: autoint1.e
Quant Time: Jul 03 00:59:39 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF062619.M
Quant Title :
QLast Update : Wed Jun 26 14:27:24 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

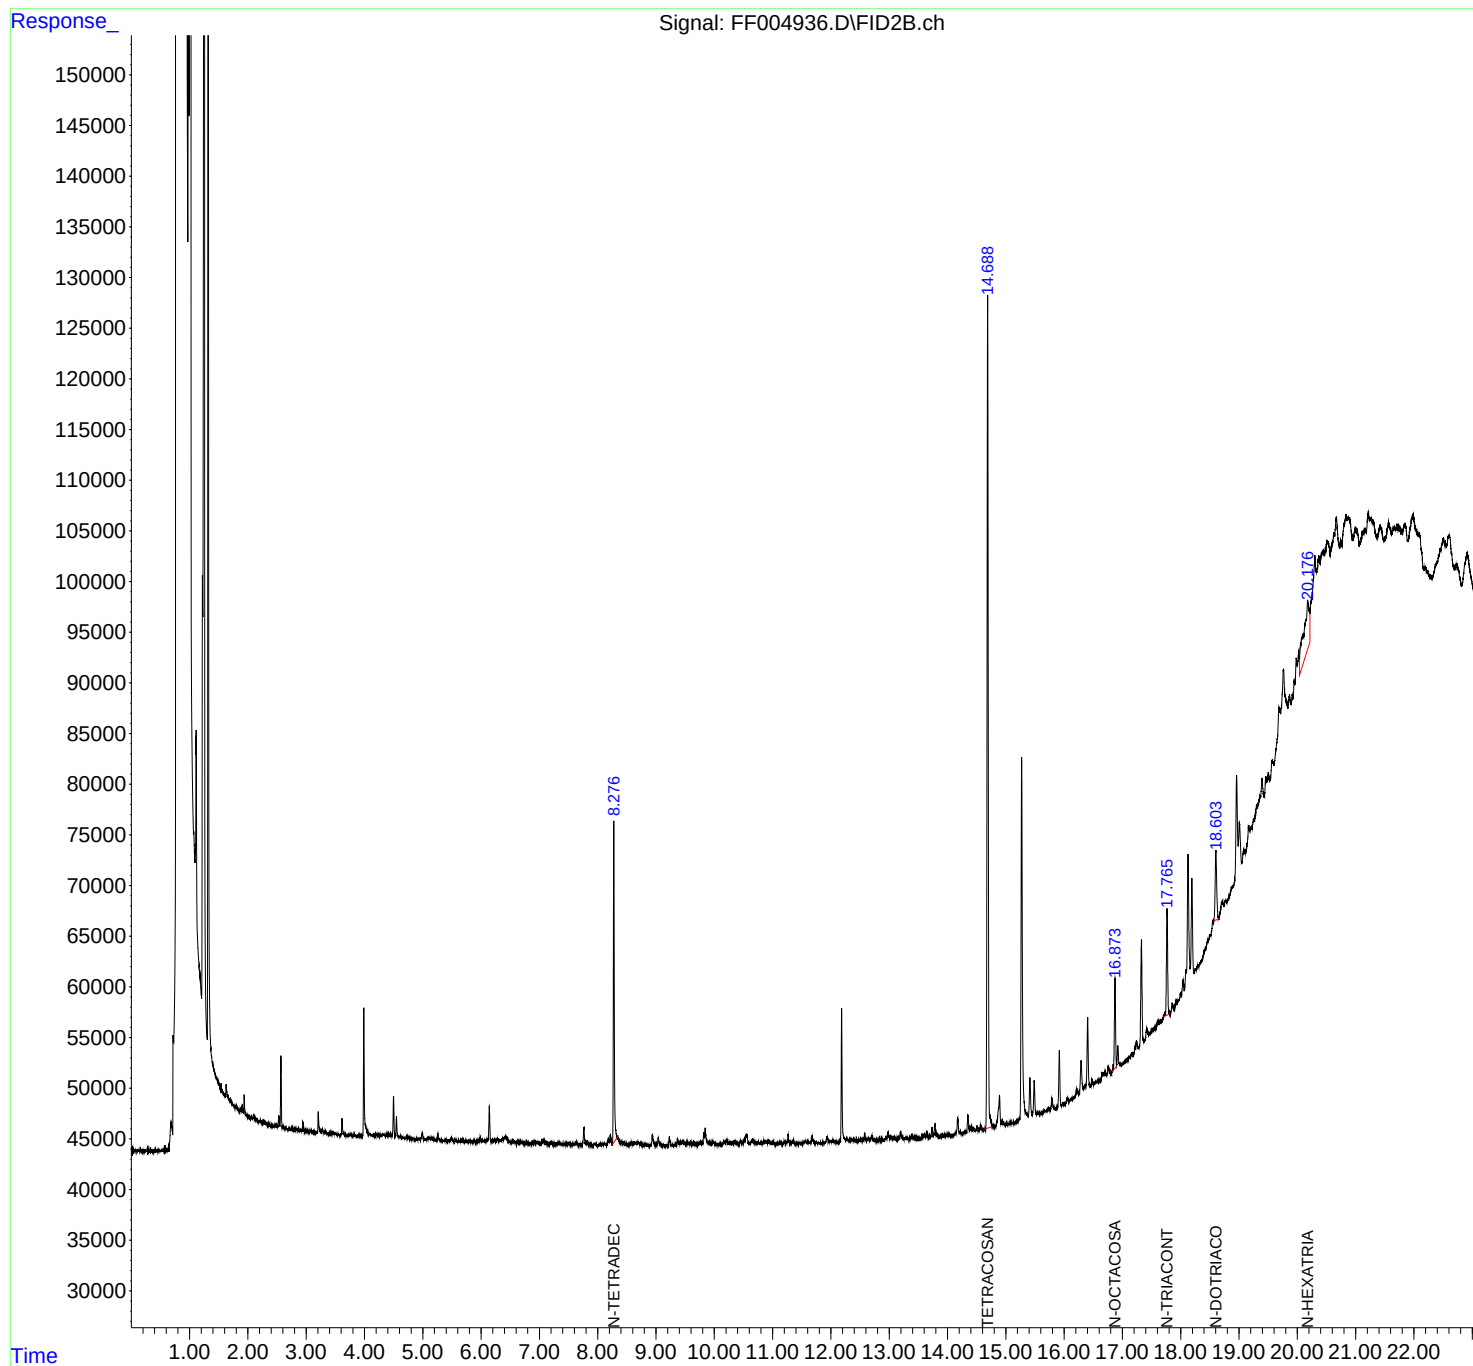


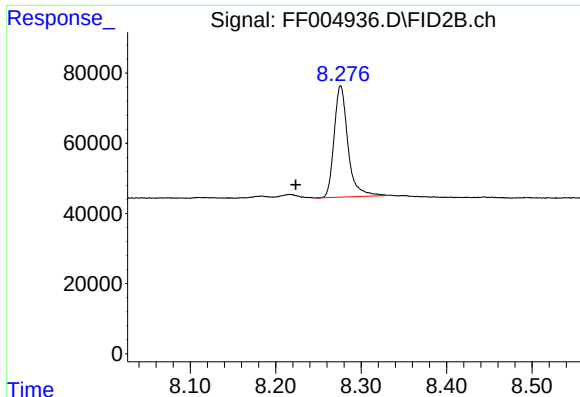

#4 N-TETRADECANE


R.T.: 8.276 min
Delta R.T.: 0.053 min
Response: 356257
Conc: 2.85 ug/ml

Instrument :
FID_F
ClientSampleId :
SAMPLE-18A

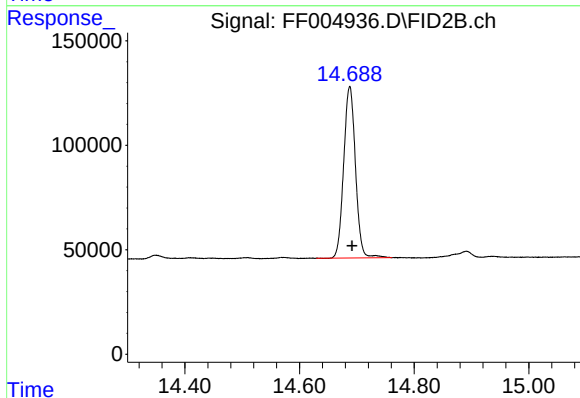


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.688 min
Delta R.T.: -0.004 min
Response: 1172316
Conc: 12.05 ug/ml

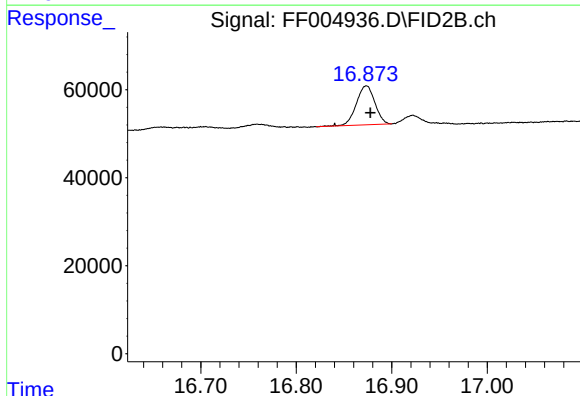


#12 N-OCTACOSANE

R.T.: 16.874 min
Delta R.T.: -0.004 min
Response: 118635
Conc: 1.06 ug/ml

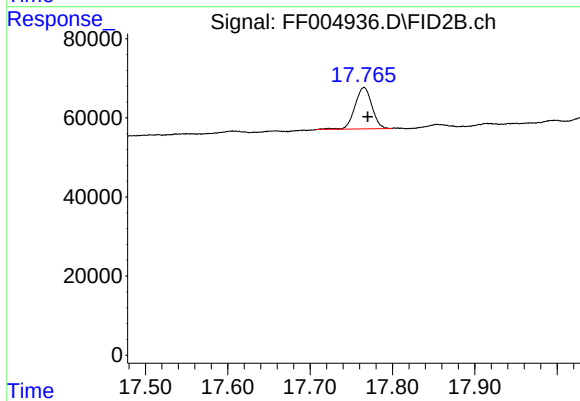

#13 N-TRIACONTANE


R.T.: 17.765 min
Delta R.T.: -0.004 min
Response: 149362
Conc: 1.33 ug/ml

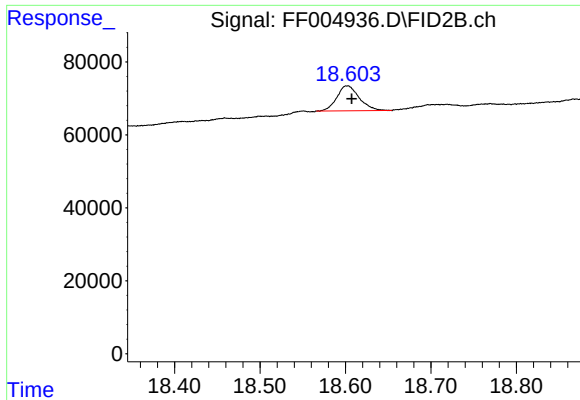

#14 N-DOTRIACONTANE

R.T.: 18.602 min
Delta R.T.: -0.005 min
Response: 124941
Conc: 1.10 ug/ml

Instrument :
FID_F
ClientSampleId :
SAMPLE-18A

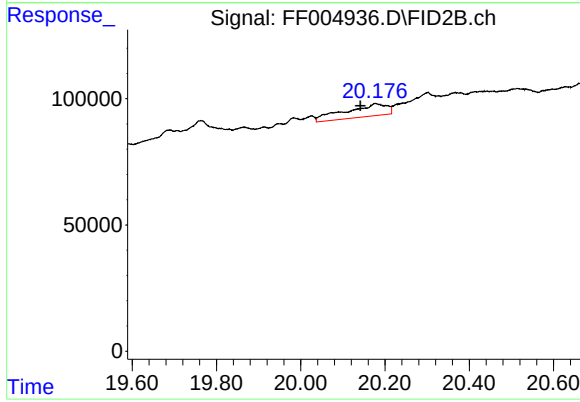

#16 N-HEXATRIACONTANE

R.T.: 20.177 min
Delta R.T.: 0.036 min
Response: 340800
Conc: 3.29 ug/ml