

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF070219\
 Data File : FF004938.D
 Signal(s) : FID2B.ch
 Acq On : 02 Jul 2019 22:05
 Operator : DD\AJ
 Sample : K3555-11
 Misc :
 ALS Vial : 63 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :
 SAMPLE-9A

Integration File: autoint1.e
 Quant Time: Jul 03 01:00:03 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF062619.M
 Quant Title :
 QLast Update : Wed Jun 26 14:27:24 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.687	1579943	16.245 ug/ml
Target Compounds			
4) N-TETRADECANE	8.276f	573327	4.582 ug/ml
6) N-OCTADECANE	11.265	93296	0.788 ug/ml
12) N-OCTACOSANE	16.873	273738	2.454 ug/ml
13) N-TRIACONTANE	17.766	335538	2.987 ug/ml
14) N-DOTRIACONTANE	18.603	284656	2.499 ug/ml
16) N-HEXATRIACONTANE	20.152	12243	0.118 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF070219\
Data File : FF004938.D
Signal(s) : FID2B.ch
Acq On : 02 Jul 2019 22:05
Operator : DD\AJ
Sample : K3555-11
Misc :
ALS Vial : 63 Sample Multiplier: 1

Instrument :
FID_F
ClientSampled :
SAMPLE-9A

Integration File: autoint1.e
Quant Time: Jul 03 01:00:03 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF062619.M
Quant Title :
QLast Update : Wed Jun 26 14:27:24 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

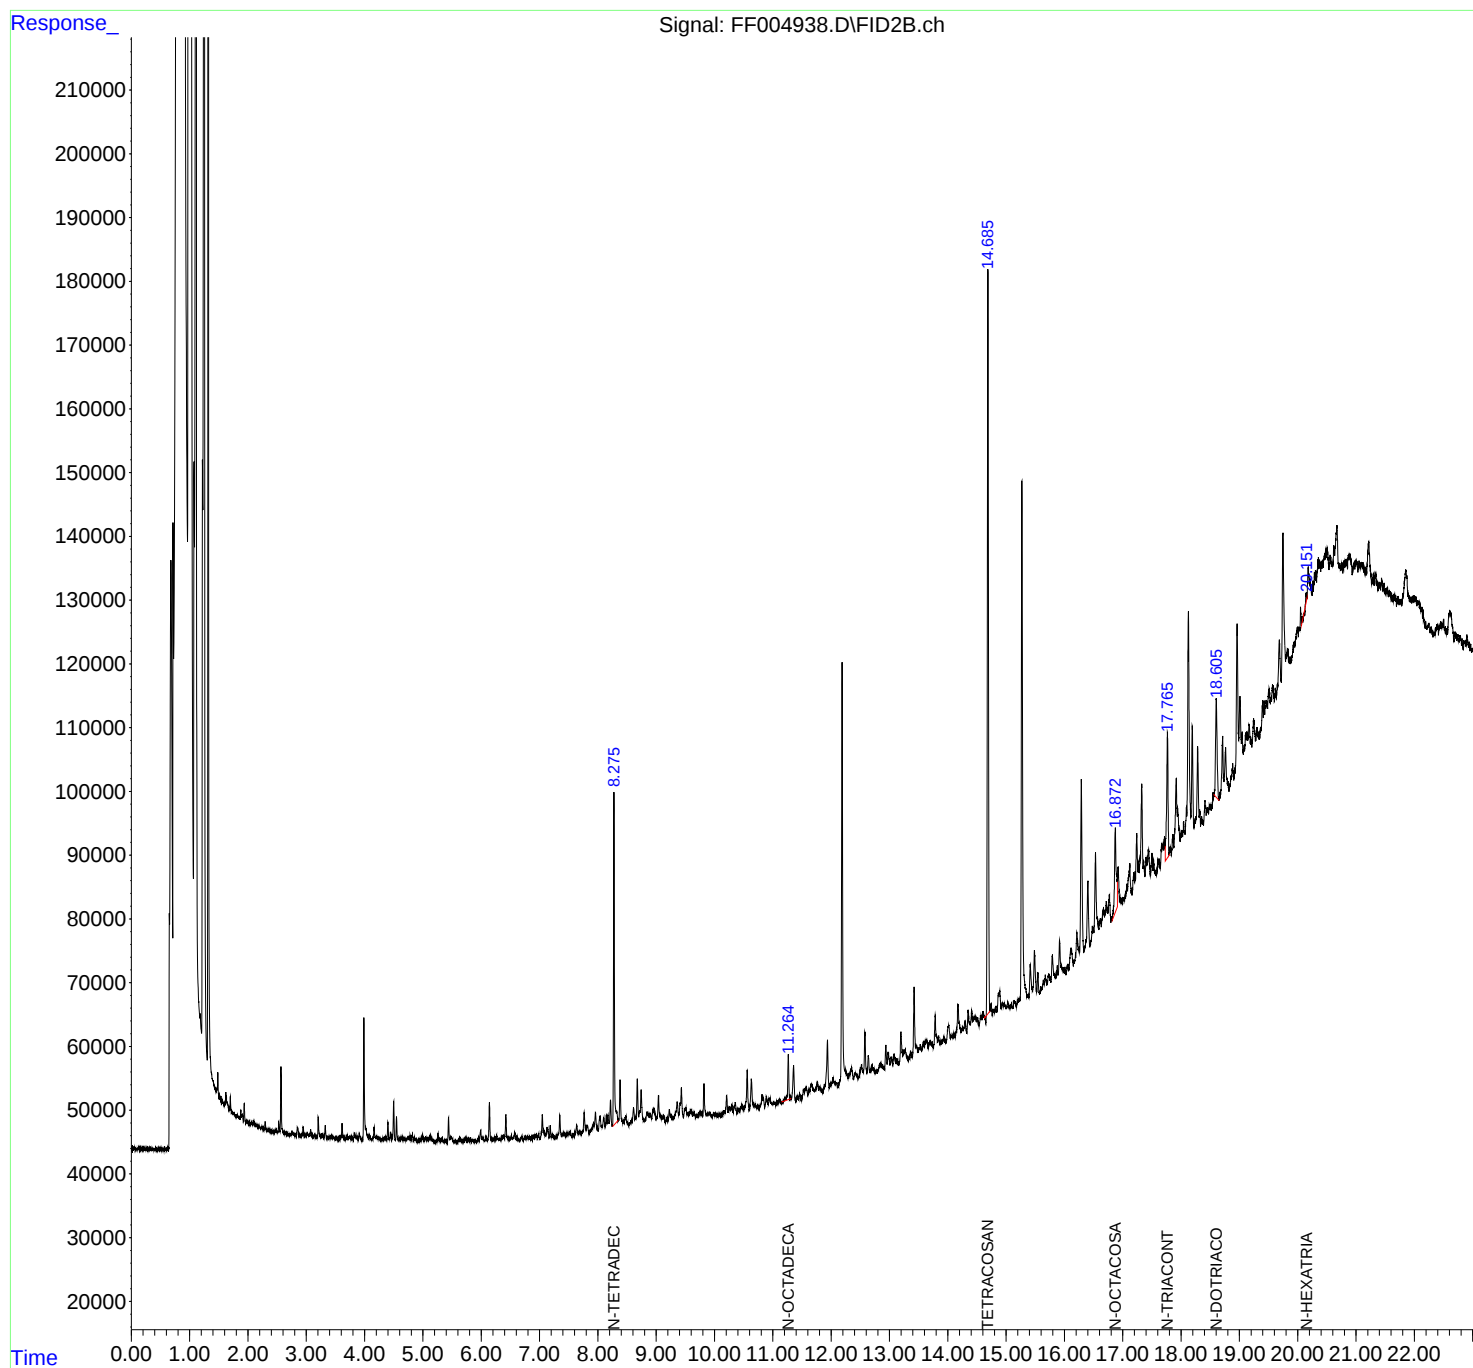


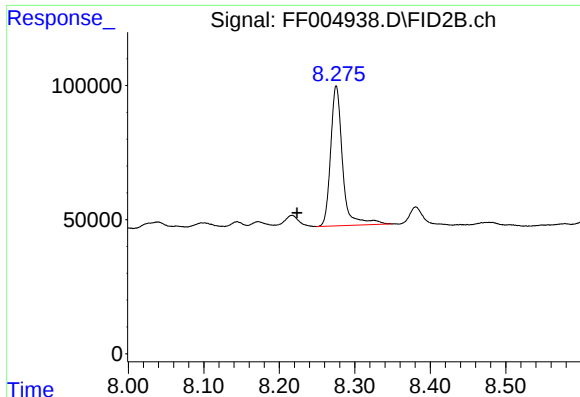

#4 N-TETRADECANE


R.T.: 8.276 min
Delta R.T.: 0.052 min
Response: 573327
Conc: 4.58 ug/ml

Instrument :
FID_F
ClientSampleId :
SAMPLE-9A

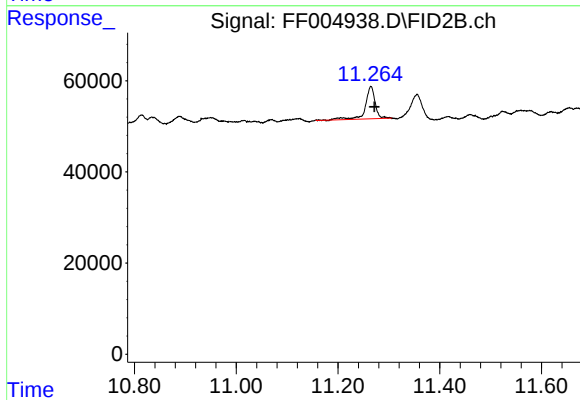


#6 N-OCTADECANE

R.T.: 11.265 min
Delta R.T.: -0.007 min
Response: 93296
Conc: 0.79 ug/ml

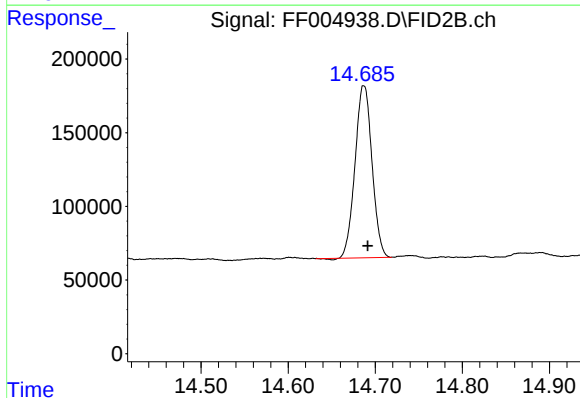


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.687 min
Delta R.T.: -0.005 min
Response: 1579943
Conc: 16.24 ug/ml

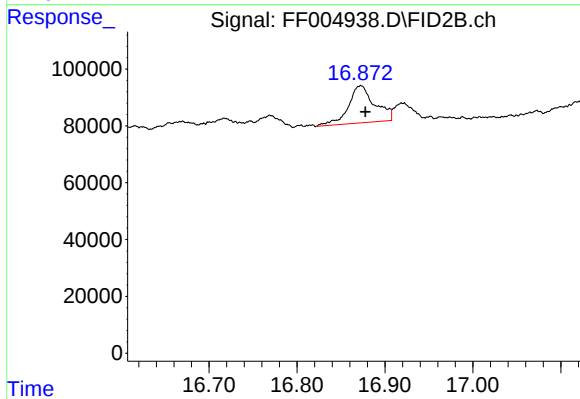

#12 N-OCTACOSANE


R.T.: 16.873 min
Delta R.T.: -0.005 min
Response: 273738
Conc: 2.45 ug/ml

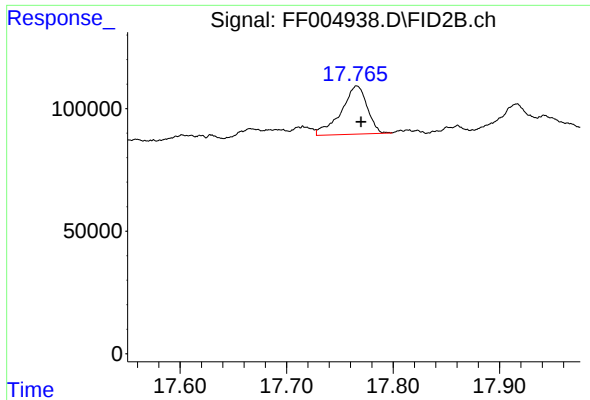

#13 N-TRIACONTANE


R.T.: 17.766 min
Delta R.T.: -0.004 min
Response: 335538
Conc: 2.99 ug/ml

Instrument :
FID_F
ClientSampleId :
SAMPLE-9A

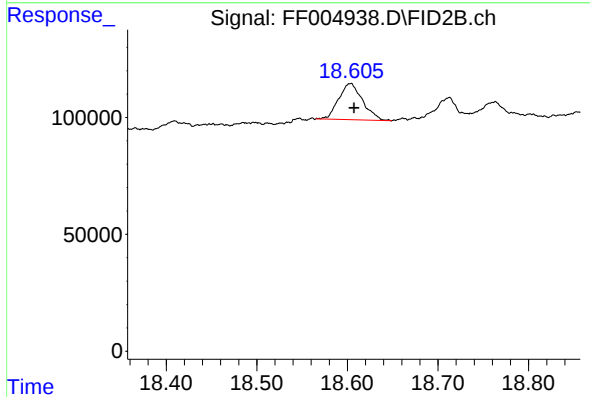

#14 N-DOTRIACONTANE

R.T.: 18.603 min
Delta R.T.: -0.004 min
Response: 284656
Conc: 2.50 ug/ml

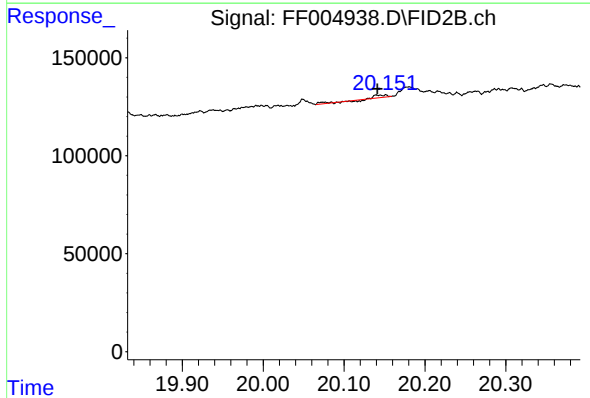

#16 N-HEXATRIACONTANE

R.T.: 20.152 min
Delta R.T.: 0.010 min
Response: 12243
Conc: 0.12 ug/ml