

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF070219\
 Data File : FF004940.D
 Signal(s) : FID2B.ch
 Acq On : 02 Jul 2019 23:04
 Operator : DD\AJ
 Sample : K3555-15
 Misc :
 ALS Vial : 65 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :
 SAMPLE-12A

Integration File: autoint1.e
 Quant Time: Jul 03 01:00:37 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF062619.M
 Quant Title :
 QLast Update : Wed Jun 26 14:27:24 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.686	2461511	25.309 ug/ml
Target Compounds			
4) N-TETRADECANE	8.275f	739116	5.907 ug/ml
12) N-OCTACOSANE	16.872	180304	1.617 ug/ml
13) N-TRIACONTANE	17.764	274417	2.443 ug/ml
14) N-DOTRIACONTANE	18.600	332332	2.918 ug/ml
15) N-TETRATRIACONTANE	19.399	142403	1.312 ug/ml
16) N-HEXATRIACONTANE	20.138	123009	1.188 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF070219\
Data File : FF004940.D
Signal(s) : FID2B.ch
Acq On : 02 Jul 2019 23:04
Operator : DD\AJ
Sample : K3555-15
Misc :
ALS Vial : 65 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
SAMPLE-12A

Integration File: autoint1.e
Quant Time: Jul 03 01:00:37 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF062619.M
Quant Title :
QLast Update : Wed Jun 26 14:27:24 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

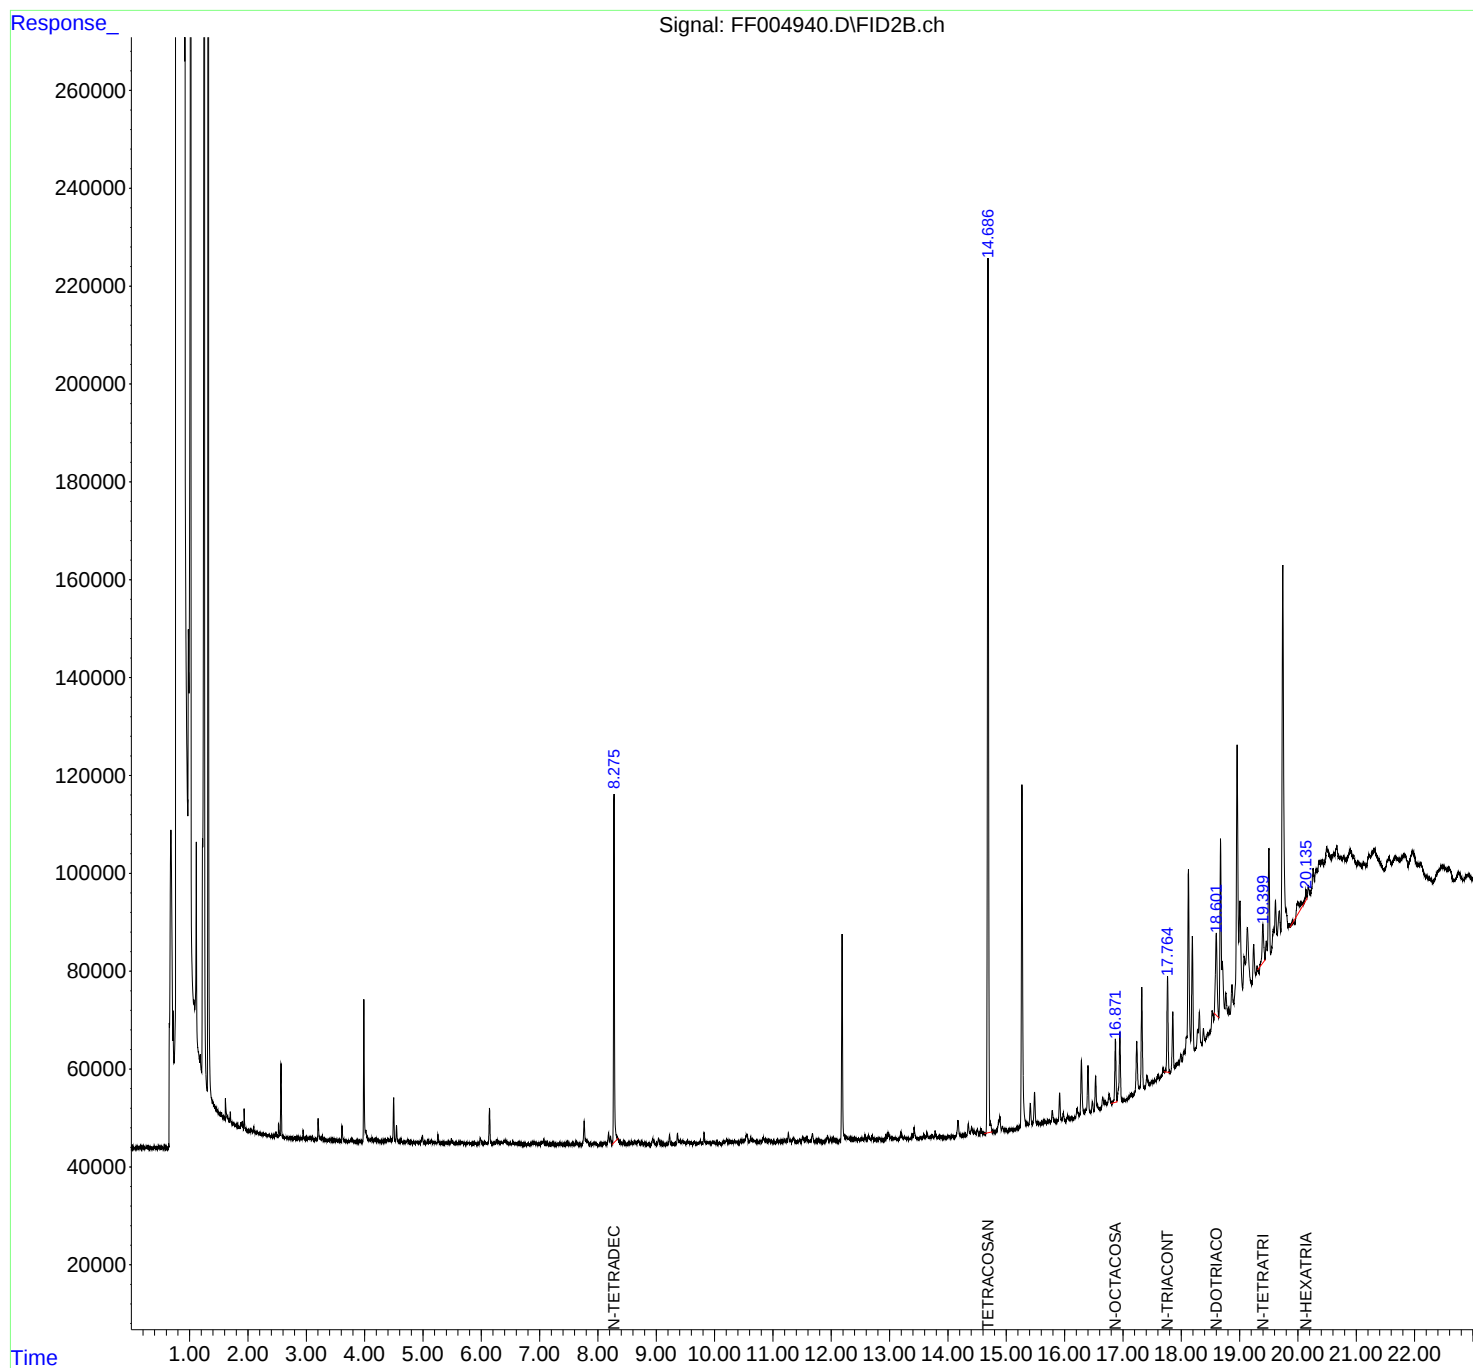


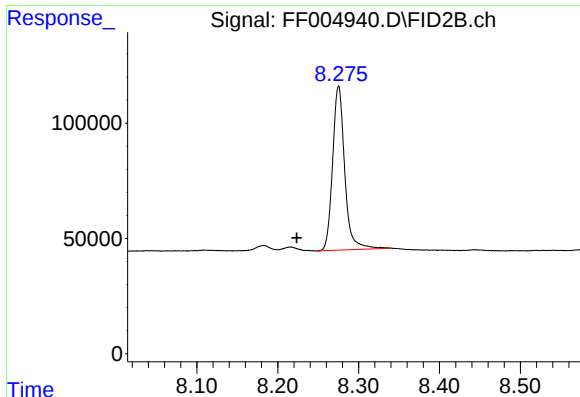

#4 N-TETRADECANE


R.T.: 8.275 min
Delta R.T.: 0.052 min
Response: 739116
Conc: 5.91 ug/ml

Instrument :
FID_F
ClientSampleId :
SAMPLE-12A

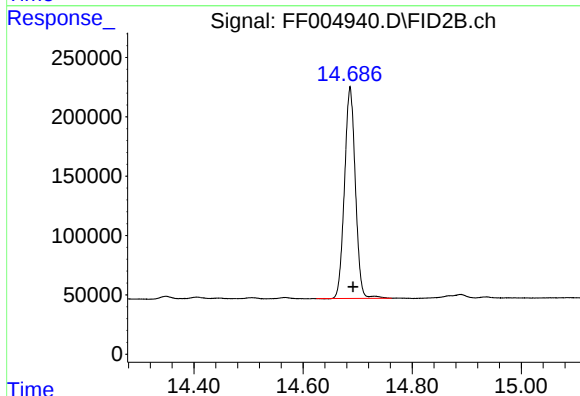


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.686 min
Delta R.T.: -0.005 min
Response: 2461511
Conc: 25.31 ug/ml

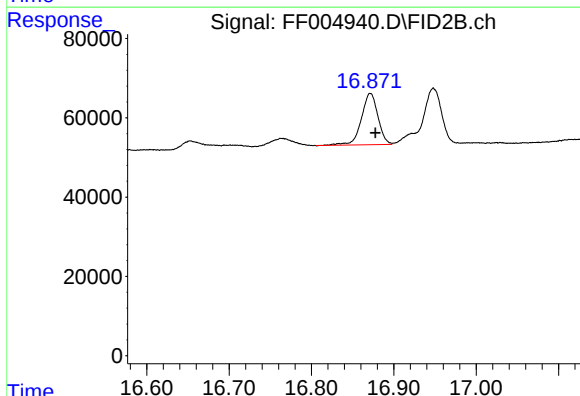


#12 N-OCTACOSANE

R.T.: 16.872 min
Delta R.T.: -0.006 min
Response: 180304
Conc: 1.62 ug/ml

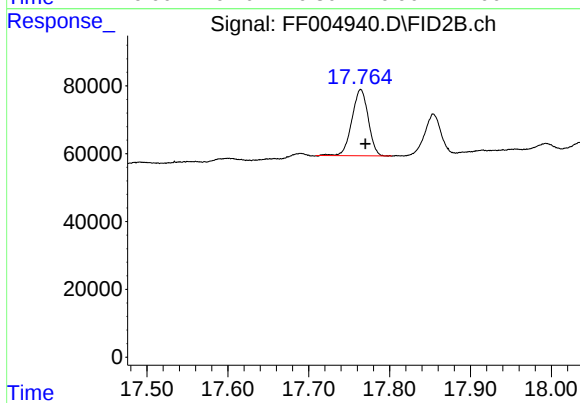

#13 N-TRIACONTANE


R.T.: 17.764 min
Delta R.T.: -0.006 min
Response: 274417
Conc: 2.44 ug/ml

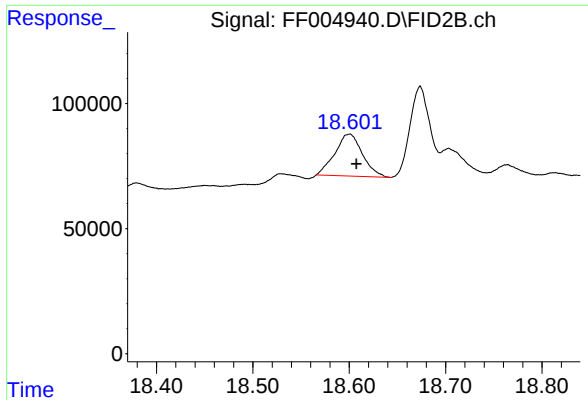

#14 N-DOTRIACONTANE


R.T.: 18.600 min
Delta R.T.: -0.007 min
Response: 332332
Conc: 2.92 ug/ml

Instrument :
FID_F
ClientSampleId :
SAMPLE-12A

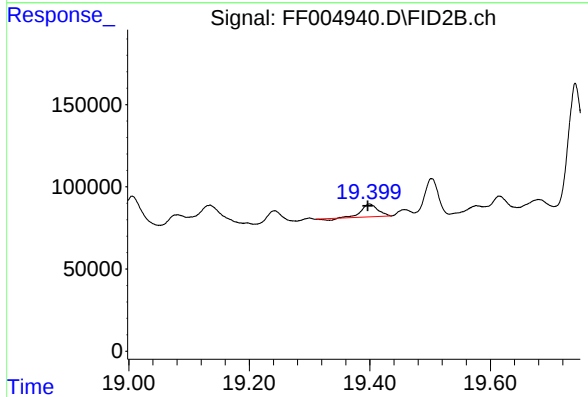

#15 N-TETRATRIACONTANE

R.T.: 19.399 min
Delta R.T.: 0.003 min
Response: 142403
Conc: 1.31 ug/ml

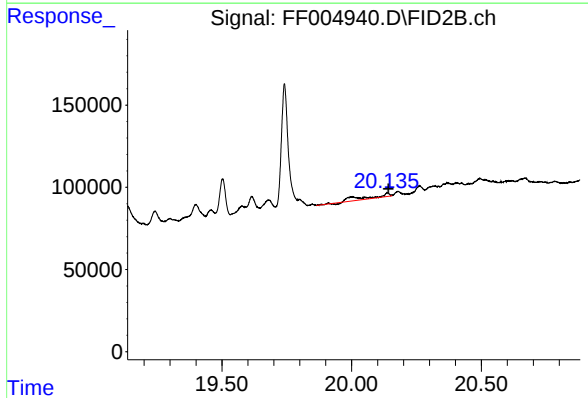

#16 N-HEXATRIACONTANE

R.T.: 20.138 min
Delta R.T.: -0.004 min
Response: 123009
Conc: 1.19 ug/ml