

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF070219\
 Data File : FF004946.D
 Signal(s) : FID2B.ch
 Acq On : 03 Jul 2019 02:00
 Operator : DD\AJ
 Sample : RT MARKER
 Misc :
 ALS Vial : 54 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :
 RT MARKER

Integration File: autoint1.e
 Quant Time: Jul 03 05:23:23 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF062619.M
 Quant Title :
 QLast Update : Wed Jun 26 14:27:24 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.726	136168	1.400 ug/ml
Target Compounds			
3) N-DODECANE	6.425	7175525	56.552 ug/ml
11) N-HEXACOSANE	15.914	93575	0.846 ug/ml
12) N-OCTACOSANE	16.874	7050346	63.210 ug/ml
13) N-TRIACONTANE	17.762	479216	4.266 ug/ml
14) N-DOTRIACONTANE	18.599	515990	4.531 ug/ml
15) N-TETRATRIACONTANE	19.389	401987	3.703 ug/ml
16) N-HEXATRIACONTANE	20.135	194671	1.880 ug/ml
17) N-OCTATRIACONTANE	20.886	153786	1.612 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF070219\
Data File : FF004946.D
Signal(s) : FID2B.ch
Acq On : 03 Jul 2019 02:00
Operator : DD\AJ
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
RT MARKER

Integration File: autoint1.e
Quant Time: Jul 03 05:23:23 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF062619.M
Quant Title :
QLast Update : Wed Jun 26 14:27:24 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

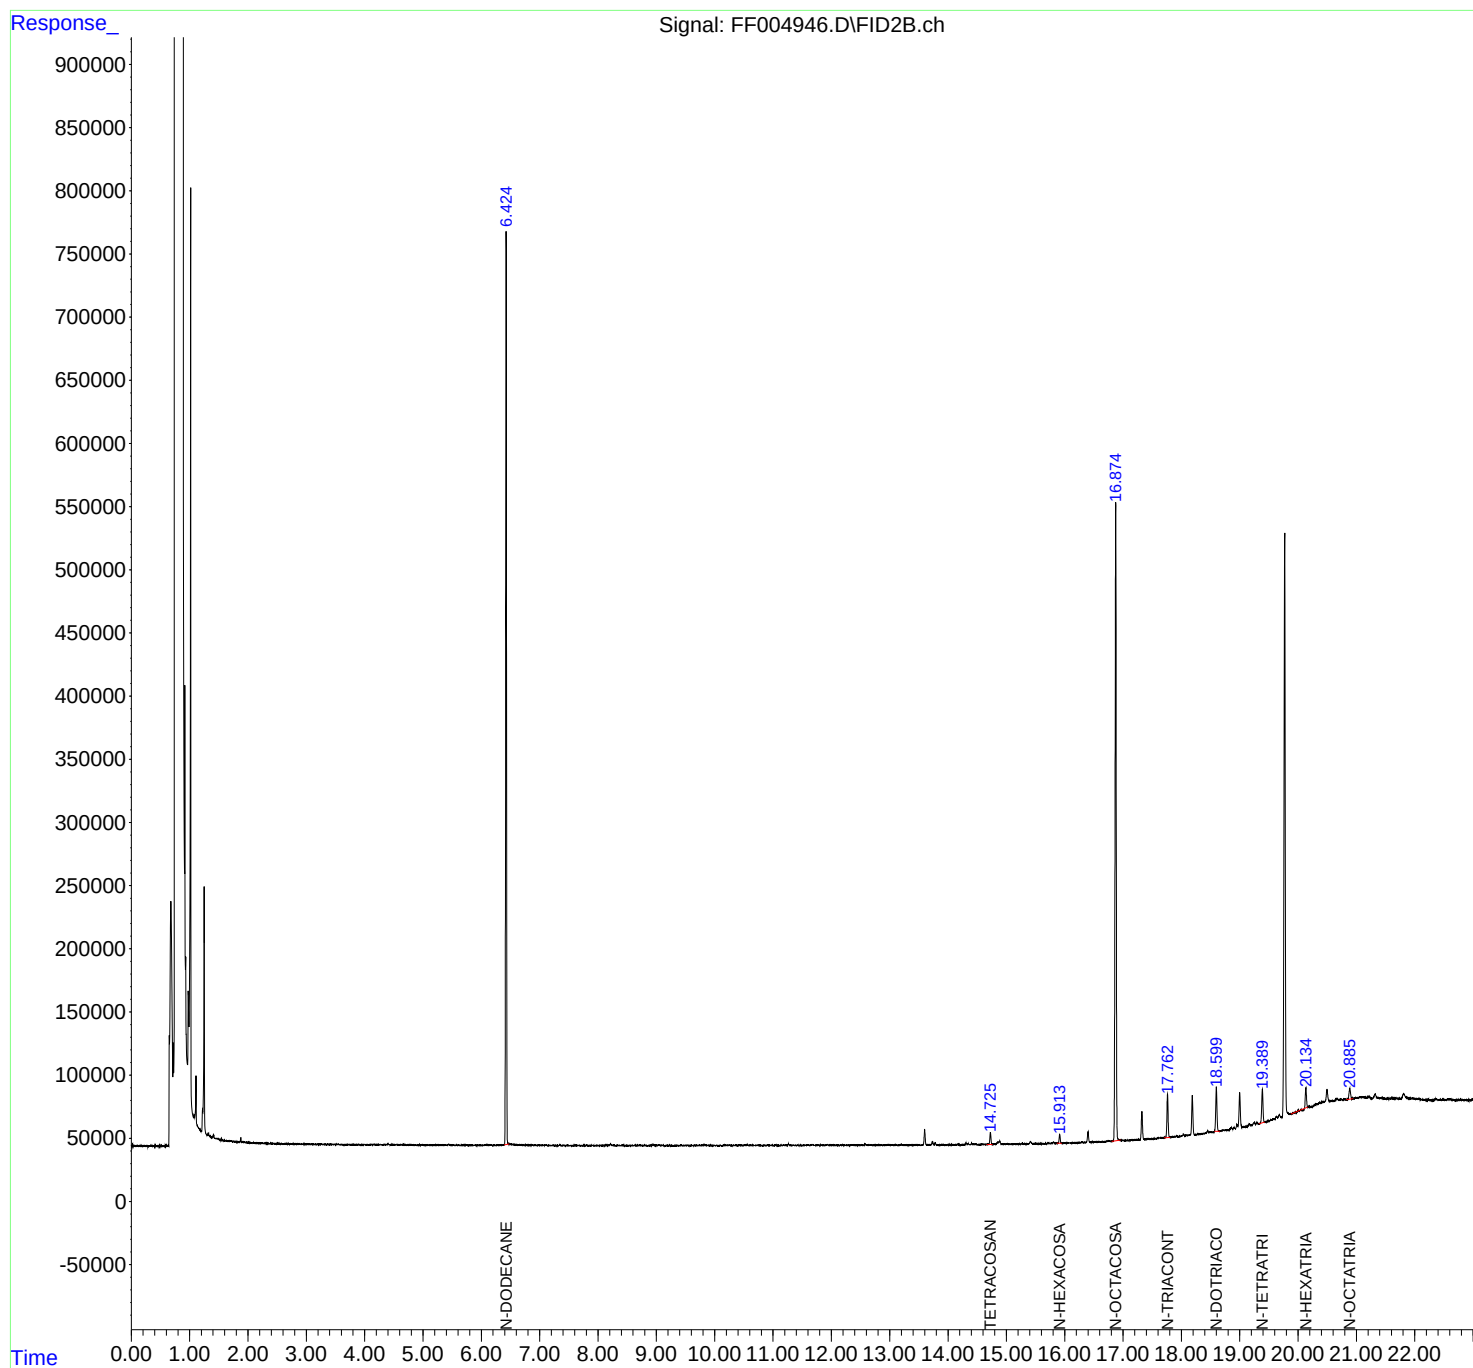


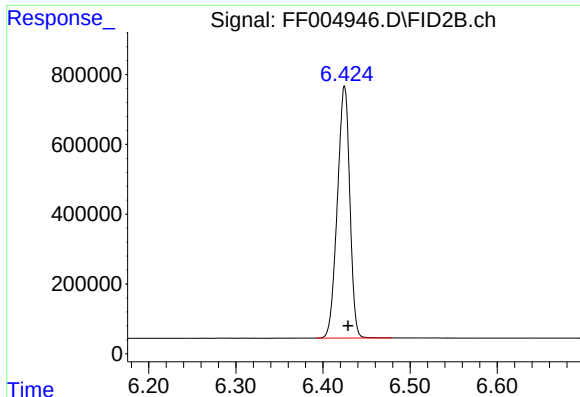

#3 N-DODECANE


R.T.: 6.425 min
Delta R.T.: -0.004 min
Response: 7175525
Conc: 56.55 ug/ml

Instrument :
FID_F
ClientSampleId :
RT MARKER

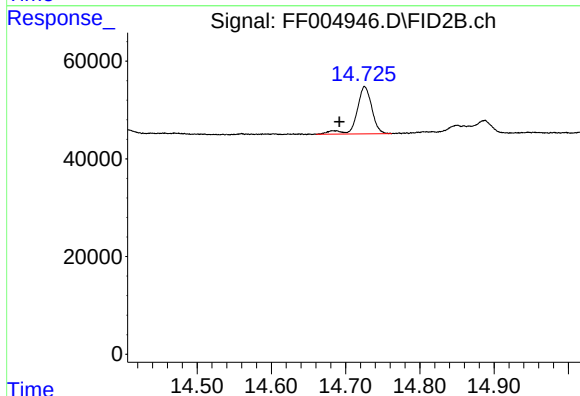


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.726 min
Delta R.T.: 0.034 min
Response: 136168
Conc: 1.40 ug/ml

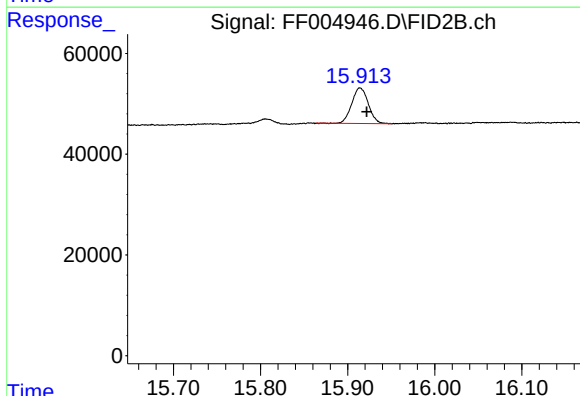


#11 N-HEXACOSANE

R.T.: 15.914 min
Delta R.T.: -0.008 min
Response: 93575
Conc: 0.85 ug/ml

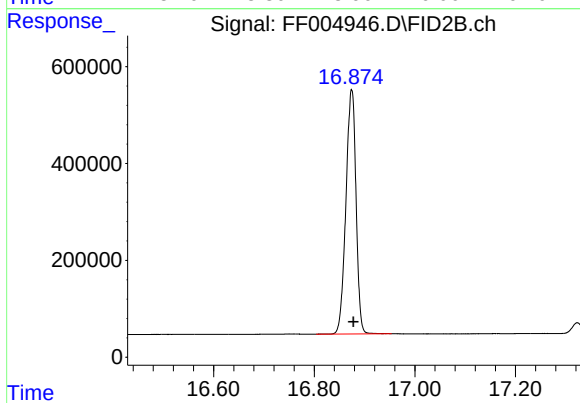

#12 N-OCTACOSANE


R.T.: 16.874 min
Delta R.T.: -0.003 min
Response: 7050346
Conc: 63.21 ug/ml

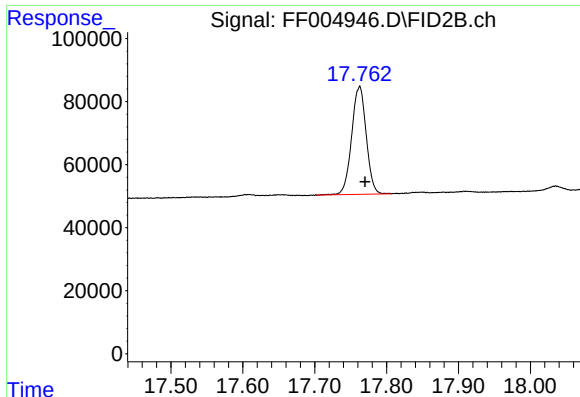

#13 N-TRIACONTANE


R.T.: 17.762 min
Delta R.T.: -0.008 min
Response: 479216
Conc: 4.27 ug/ml

Instrument :
FID_F
ClientSampleId :
RT MARKER

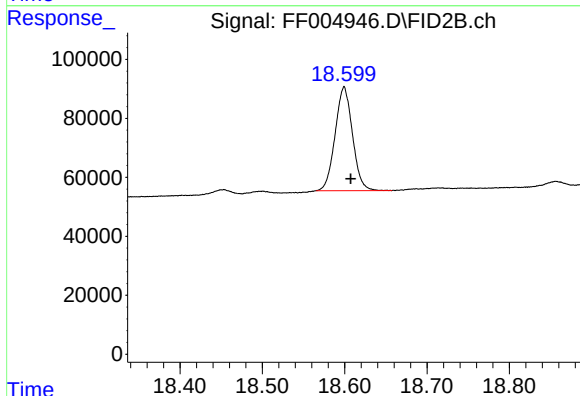


#14 N-DOTRIACONTANE

R.T.: 18.599 min
Delta R.T.: -0.008 min
Response: 515990
Conc: 4.53 ug/ml

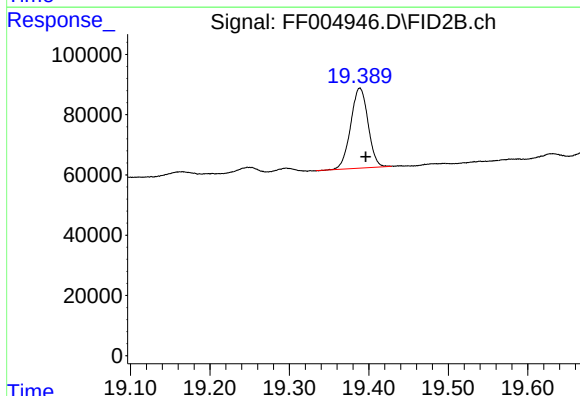


#15 N-TETRATRIACONTANE

R.T.: 19.389 min
Delta R.T.: -0.008 min
Response: 401987
Conc: 3.70 ug/ml

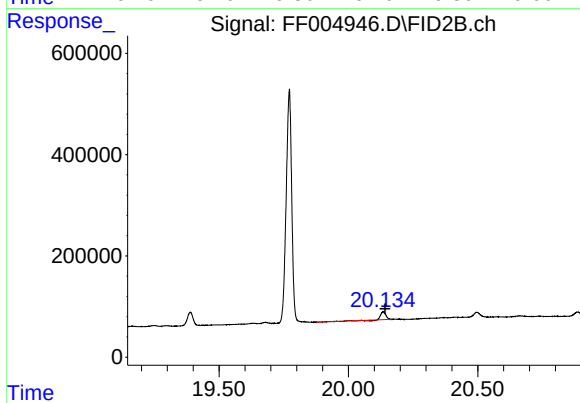

#16 N-HEXATRIACONTANE

R.T.: 20.135 min
Delta R.T.: -0.007 min
Response: 194671
Conc: 1.88 ug/ml

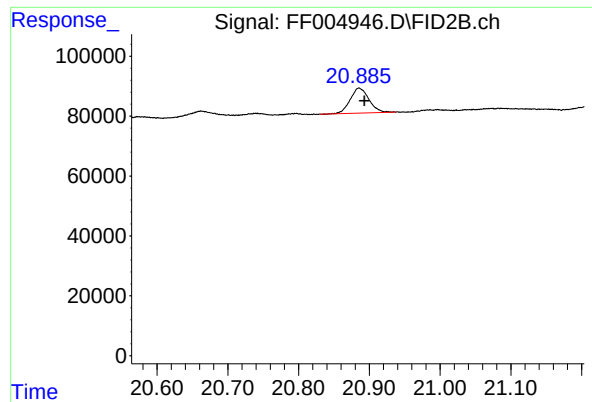

#17 N-OCTATRIACONTANE

R.T.: 20.886 min
Delta R.T.: -0.007 min
Response: 153786
Conc: 1.61 ug/ml

Instrument :
FID_F
ClientSampleId :
RT MARKER