

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF070219\
 Data File : FF004950.D
 Signal(s) : FID2B.ch
 Acq On : 03 Jul 2019 03:58
 Operator : DD\AJ
 Sample : K3610-01
 Misc :
 ALS Vial : 70 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :
 CSIMW-01-20190628

Integration File: autoint1.e
 Quant Time: Jul 03 05:24:33 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF062619.M
 Quant Title :
 QLast Update : Wed Jun 26 14:27:24 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.684	2175916	22.372 ug/ml
Target Compounds			
12) N-OCTACOSANE	16.867	114389	1.026 ug/ml
13) N-TRIACONTANE	17.759	151467	1.348 ug/ml
14) N-DOTRIACONTANE	18.597	116737	1.025 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF070219\
Data File : FF004950.D
Signal(s) : FID2B.ch
Acq On : 03 Jul 2019 03:58
Operator : DD\AJ
Sample : K3610-01
Misc :
ALS Vial : 70 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
CSIMW-01-20190628

Integration File: autoint1.e
Quant Time: Jul 03 05:24:33 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF062619.M
Quant Title :
QLast Update : Wed Jun 26 14:27:24 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

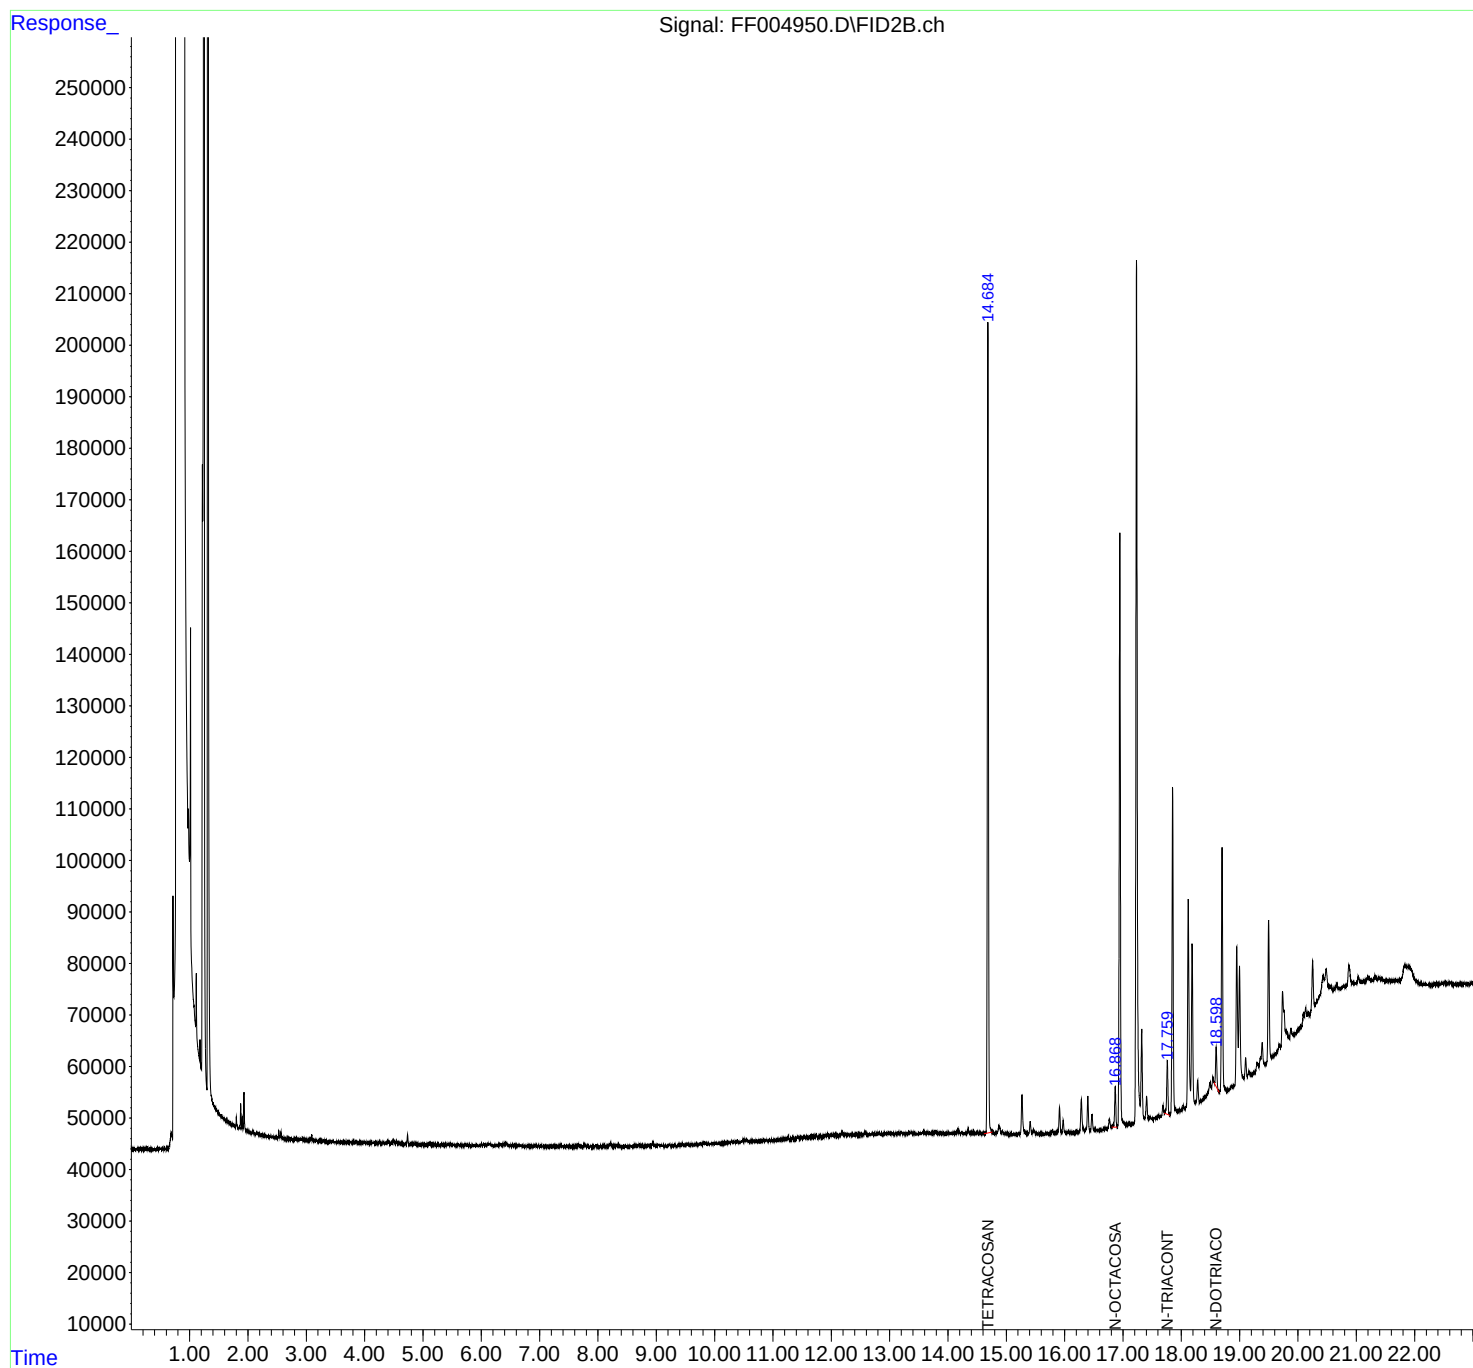


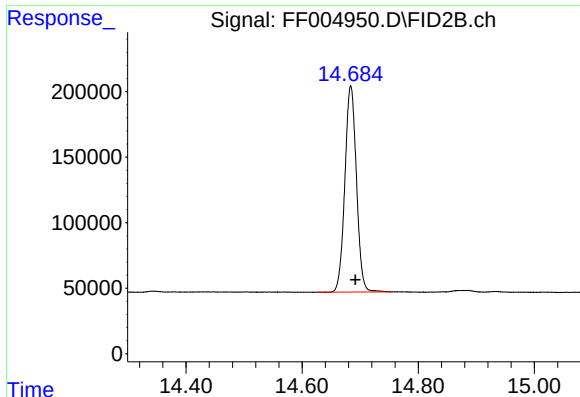

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.684 min
Delta R.T.: -0.008 min
Response: 2175916
Conc: 22.37 ug/ml

Instrument :
FID_F
ClientSampleId :
CSIMW-01-20190628

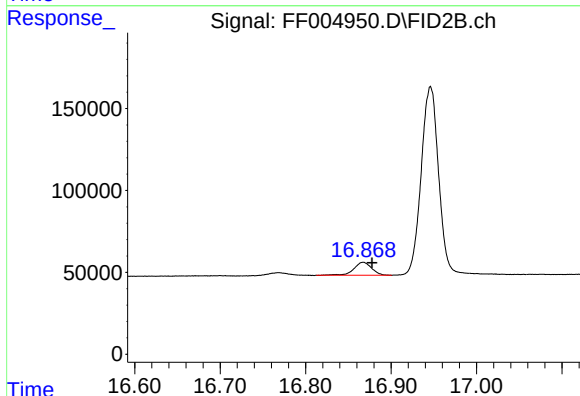


#12 N-OCTACOSANE

R.T.: 16.867 min
Delta R.T.: -0.010 min
Response: 114389
Conc: 1.03 ug/ml

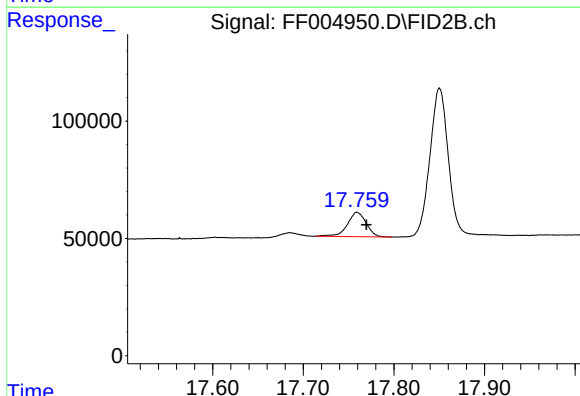

#13 N-TRIACONTANE

R.T.: 17.759 min
Delta R.T.: -0.010 min
Response: 151467
Conc: 1.35 ug/ml

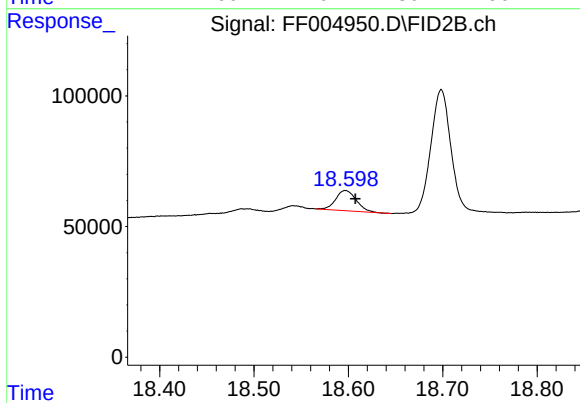

#14 N-DOTRIACONTANE

R.T.: 18.597 min
Delta R.T.: -0.011 min
Response: 116737
Conc: 1.02 ug/ml