

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF070219\
 Data File : FF004952.D
 Signal(s) : FID2B.ch
 Acq On : 03 Jul 2019 04:57
 Operator : DD\AJ
 Sample : K3610-03
 Misc :
 ALS Vial : 72 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jul 03 05:24:59 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF062619.M
 Quant Title :
 QLast Update : Wed Jun 26 14:27:24 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.684	2199872	22.619 ug/ml
Target Compounds			
2) N-DECANE	4.345f	217660	1.724 ug/ml
3) N-DODECANE	6.418	592371	4.669 ug/ml
4) N-TETRADECANE	8.214	336192	2.687 ug/ml
5) N-HEXADECANE	9.824	702883	5.692 ug/ml
6) N-OCTADECANE	11.273	785591	6.631 ug/ml
7) N-EICOSANE	12.642f	332832	2.869 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF070219\
Data File : FF004952.D
Signal(s) : FID2B.ch
Acq On : 03 Jul 2019 04:57
Operator : DD\AJ
Sample : K3610-03
Misc :
ALS Vial : 72 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jul 03 05:24:59 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF062619.M
Quant Title :
QLast Update : Wed Jun 26 14:27:24 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

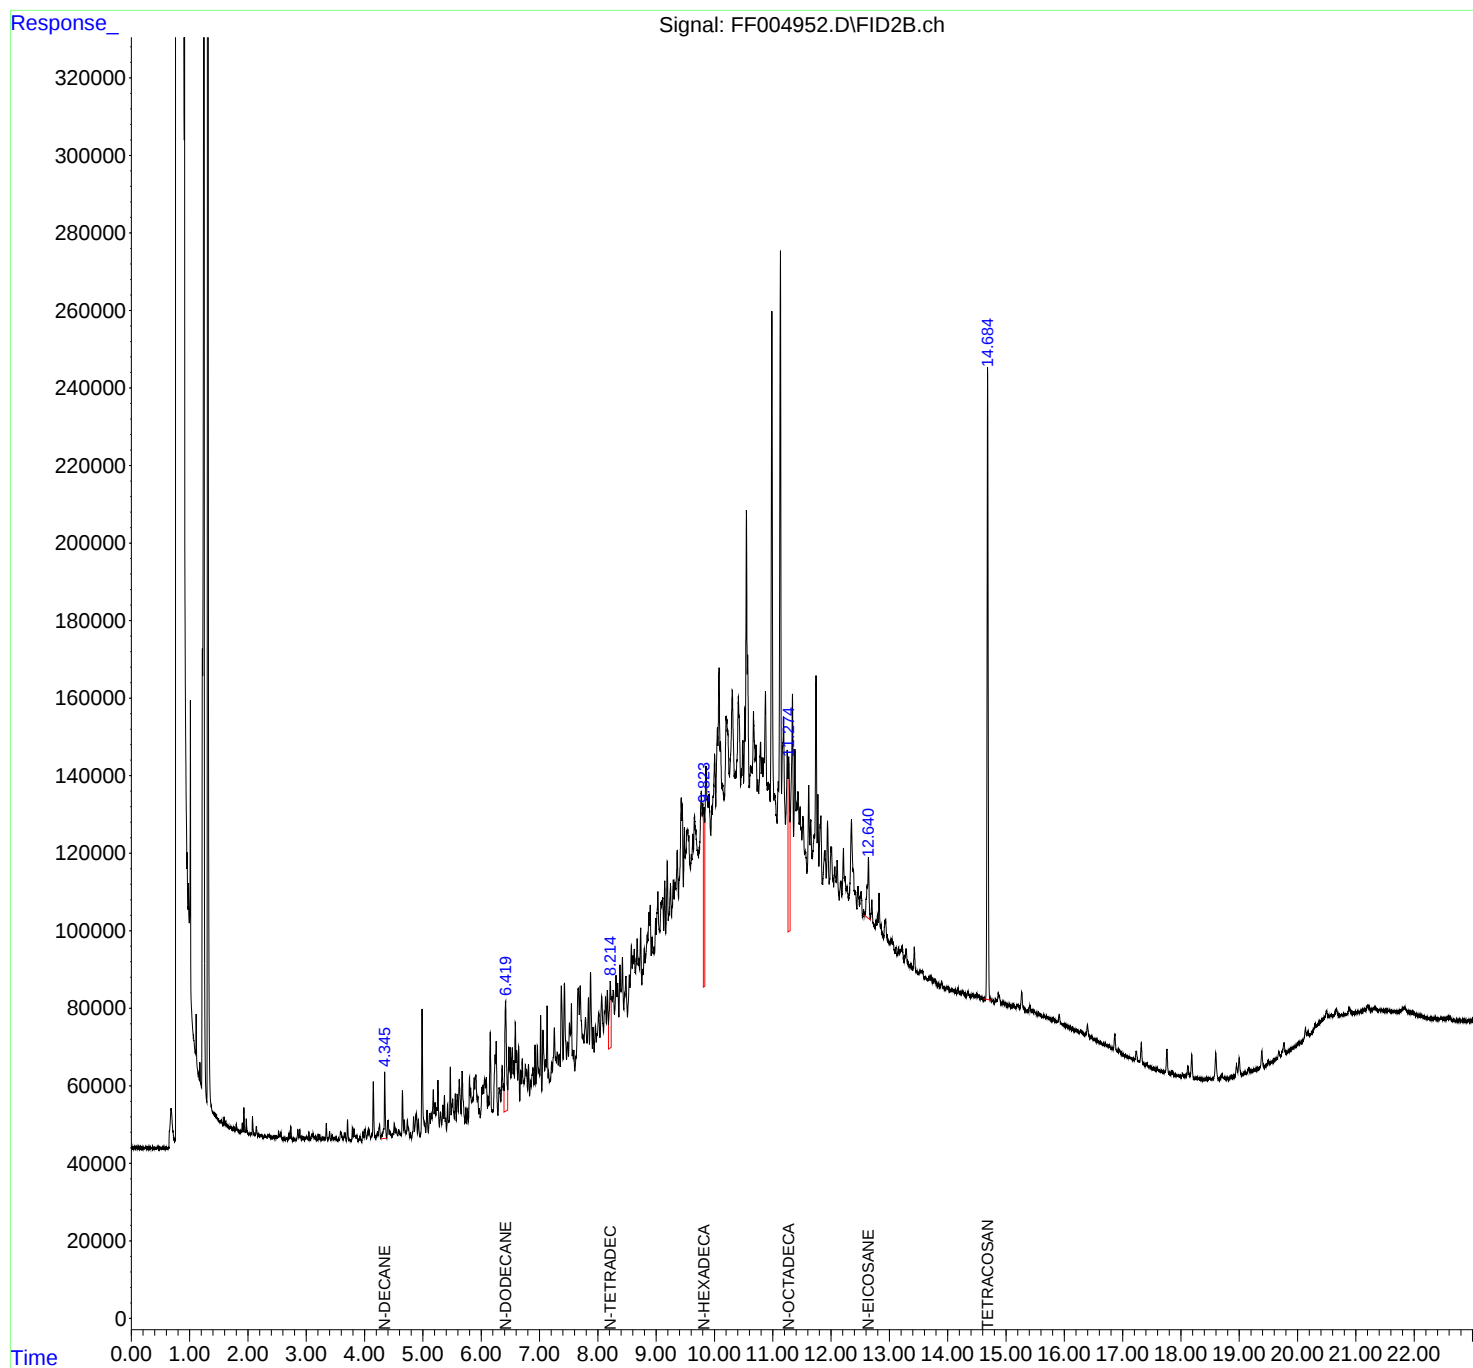


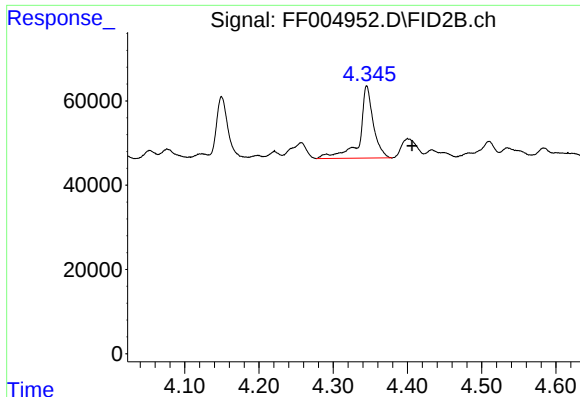

#2 N-DECANE


R.T.: 4.345 min
Delta R.T.: -0.061 min
Response: 217660
Conc: 1.72 ug/ml

Instrument :
FID_F
ClientSampleId :

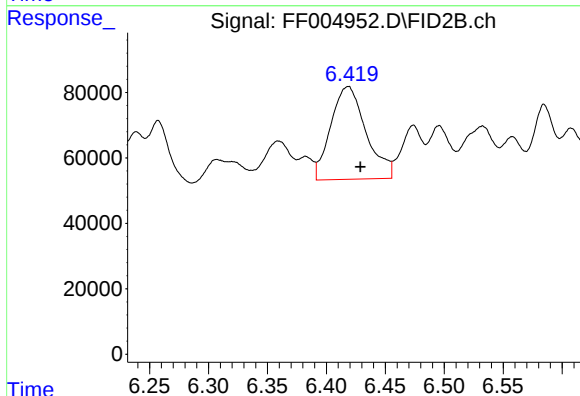


#3 N-DODECANE

R.T.: 6.418 min
Delta R.T.: -0.010 min
Response: 592371
Conc: 4.67 ug/ml

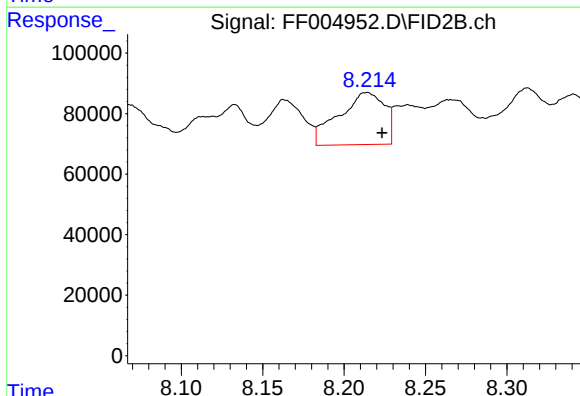


#4 N-TETRADECANE

R.T.: 8.214 min
Delta R.T.: -0.010 min
Response: 336192
Conc: 2.69 ug/ml

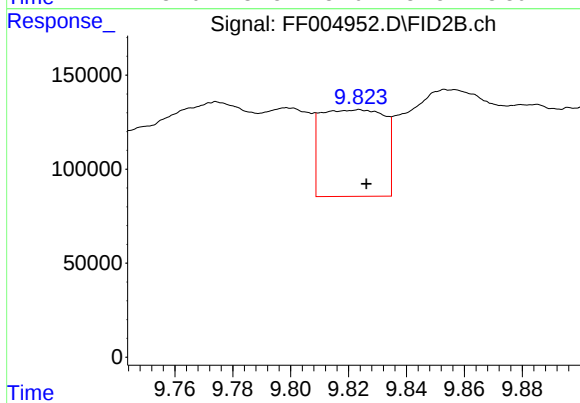

#5 N-HEXADECANE


R.T.: 9.824 min
Delta R.T.: -0.002 min
Response: 702883
Conc: 5.69 ug/ml

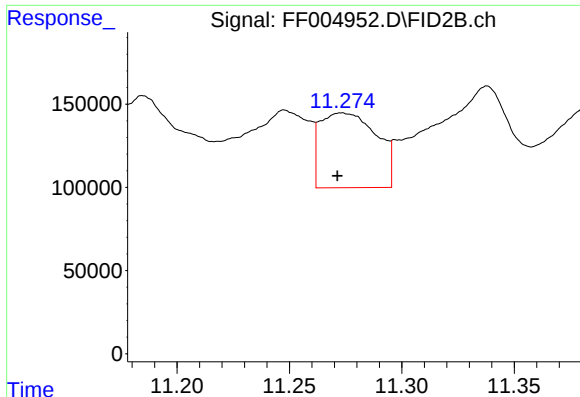

#6 N-OCTADECANE


R.T.: 11.273 min
Delta R.T.: 0.002 min
Response: 785591
Conc: 6.63 ug/ml

Instrument :
FID_F
ClientSampleId :

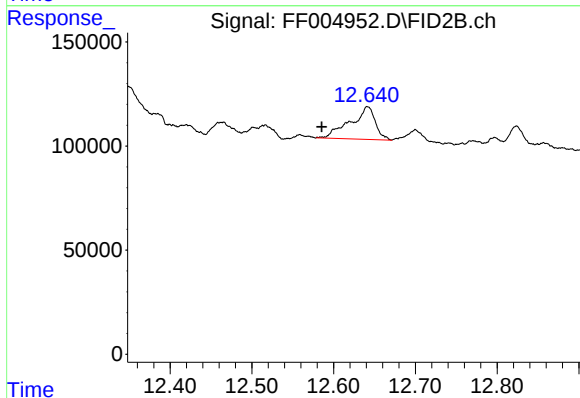

#7 N-EICOSANE

R.T.: 12.642 min
Delta R.T.: 0.056 min
Response: 332832
Conc: 2.87 ug/ml

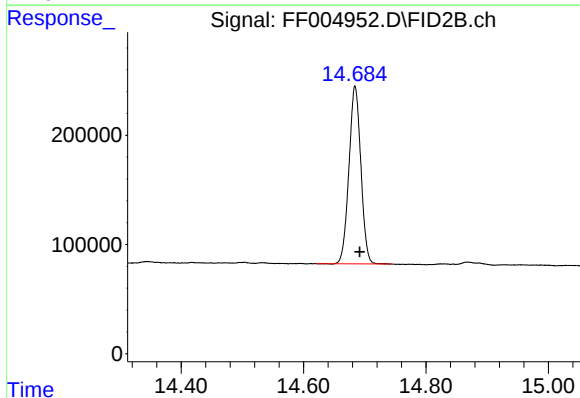

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.684 min
Delta R.T.: -0.007 min
Response: 2199872
Conc: 22.62 ug/ml