

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF070219\
Data File : FF004953.D
Signal(s) : FID2B.ch
Acq On : 03 Jul 2019 07:23
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jul 03 08:21:09 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF062619.M
Quant Title :
QLast Update : Wed Jun 26 14:27:24 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.682	2313371	23.786 ug/ml
Target Compounds			
10) N-TETRACOSANE	14.863	185240	1.664 ug/ml
14) N-DOTRIACONTANE	18.609	152180	1.336 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF070219\
Data File : FF004953.D
Signal(s) : FID2B.ch
Acq On : 03 Jul 2019 07:23
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jul 03 08:21:09 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF062619.M
Quant Title :
QLast Update : Wed Jun 26 14:27:24 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

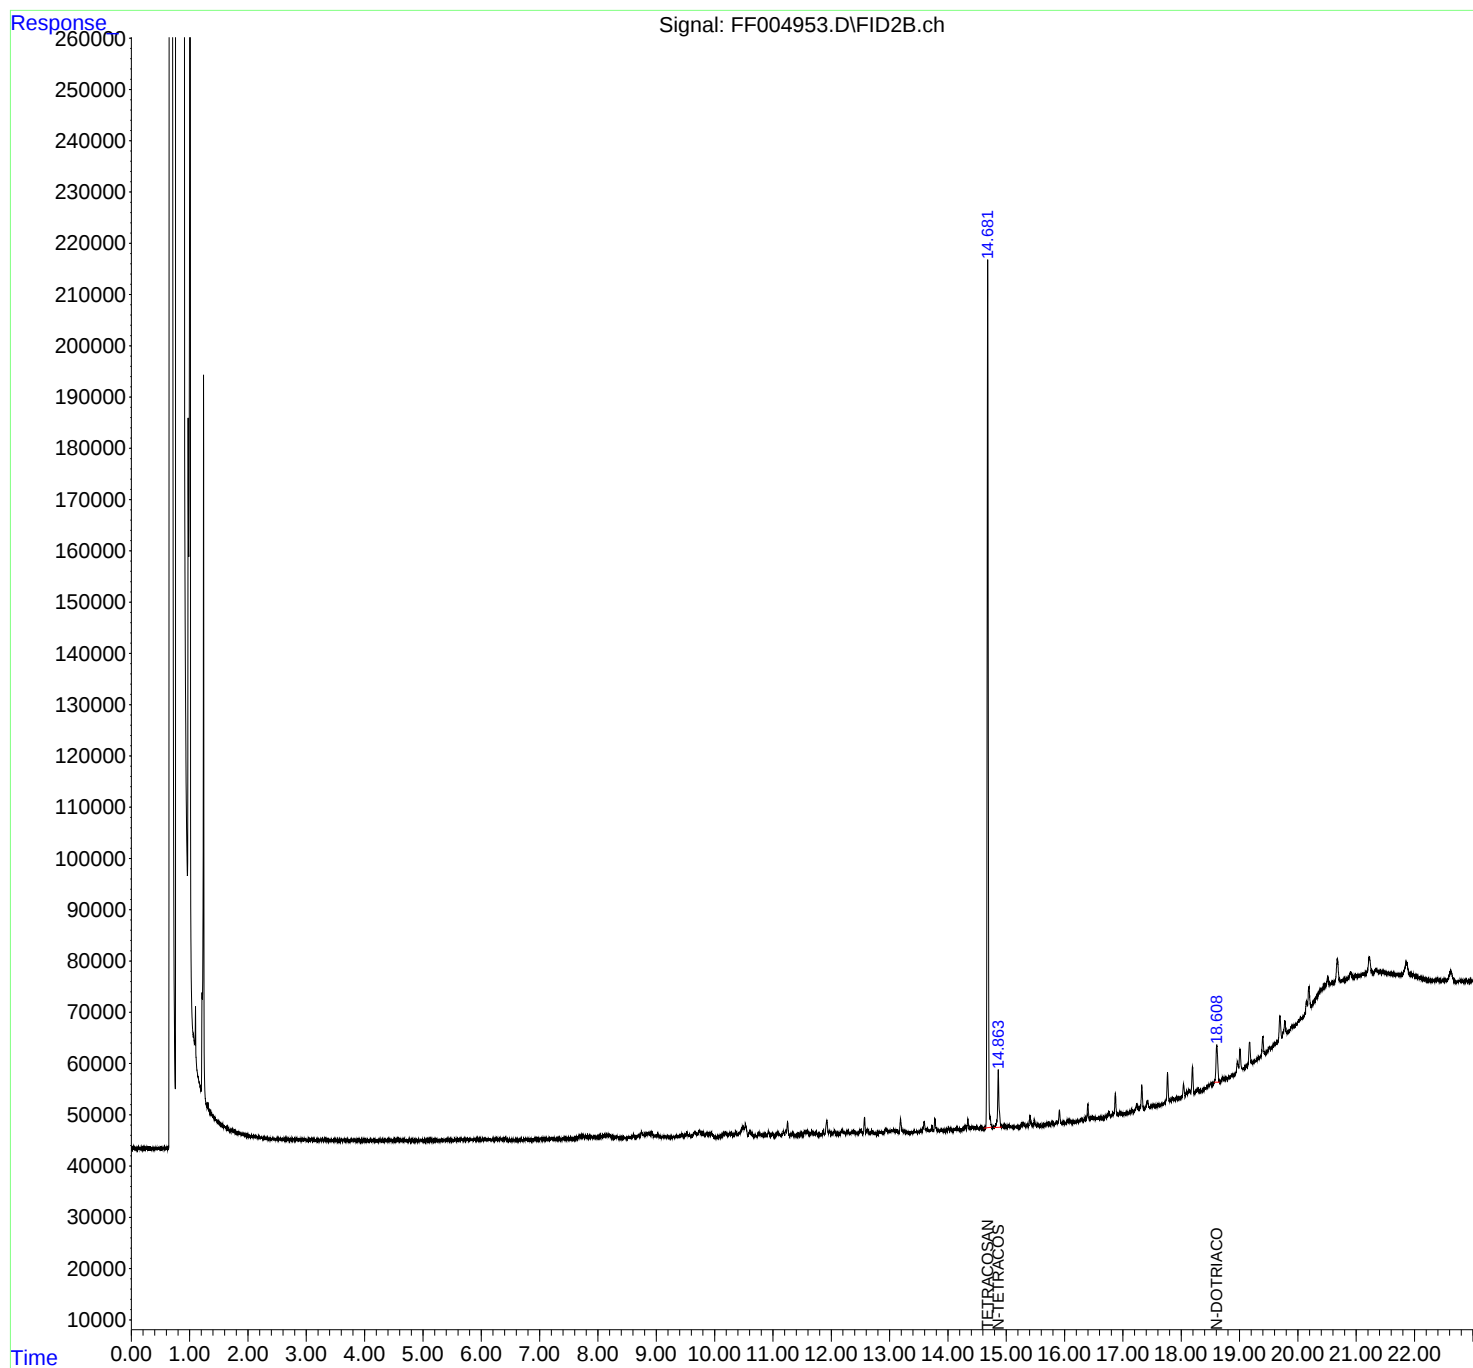


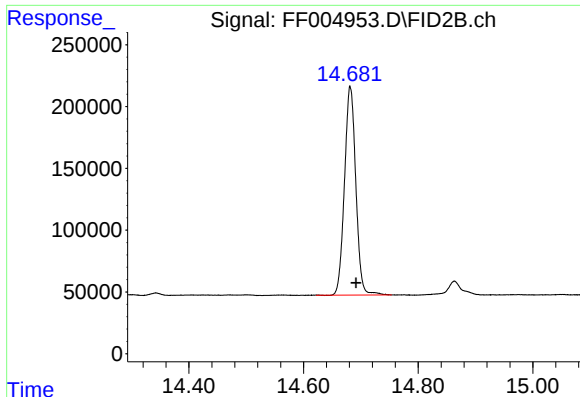

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.682 min
Delta R.T.: -0.010 min
Response: 2313371
Conc: 23.79 ug/ml

Instrument :
FID_F
ClientSampleId :

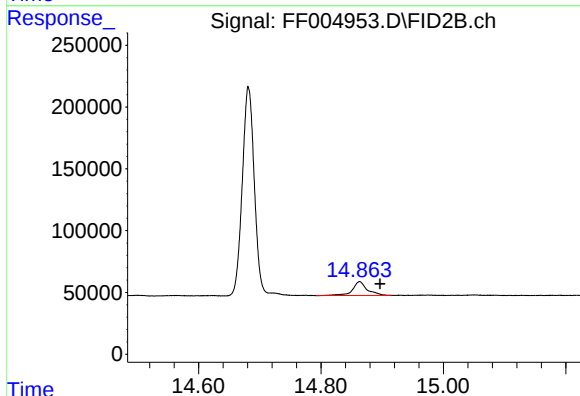

#10 N-TETRACOSANE

R.T.: 14.863 min
Delta R.T.: -0.033 min
Response: 185240
Conc: 1.66 ug/ml

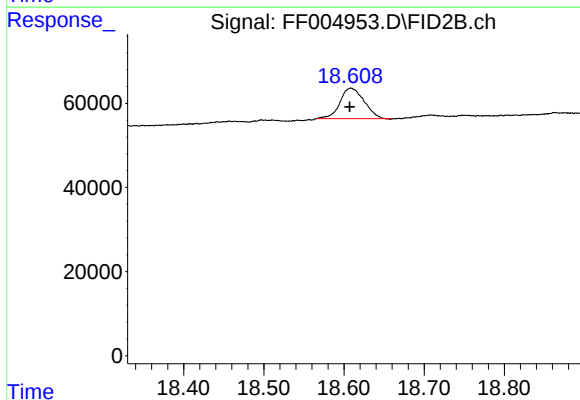

#14 N-DOTRIACONTANE

R.T.: 18.609 min
Delta R.T.: 0.001 min
Response: 152180
Conc: 1.34 ug/ml