

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF070219\
 Data File : FF004955.D
 Signal(s) : FID2B.ch
 Acq On : 03 Jul 2019 09:07
 Operator : DD\AJ
 Sample : K3610-03 5X
 Misc :
 ALS Vial : 55 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jul 03 11:15:57 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF062619.M
 Quant Title :
 QLast Update : Wed Jun 26 14:27:24 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.682	605302	6.224 ug/ml
Target Compounds			
3) N-DODECANE	6.411	107286	0.846 ug/ml
10) N-TETRACOSANE	14.865	130785	1.175 ug/ml
13) N-TRIACONTANE	17.762	93709	0.834 ug/ml
14) N-DOTRIACONTANE	18.604	139005	1.220 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF070219\
Data File : FF004955.D
Signal(s) : FID2B.ch
Acq On : 03 Jul 2019 09:07
Operator : DD\AJ
Sample : K3610-03 5X
Misc :
ALS Vial : 55 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jul 03 11:15:57 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF062619.M
Quant Title :
QLast Update : Wed Jun 26 14:27:24 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

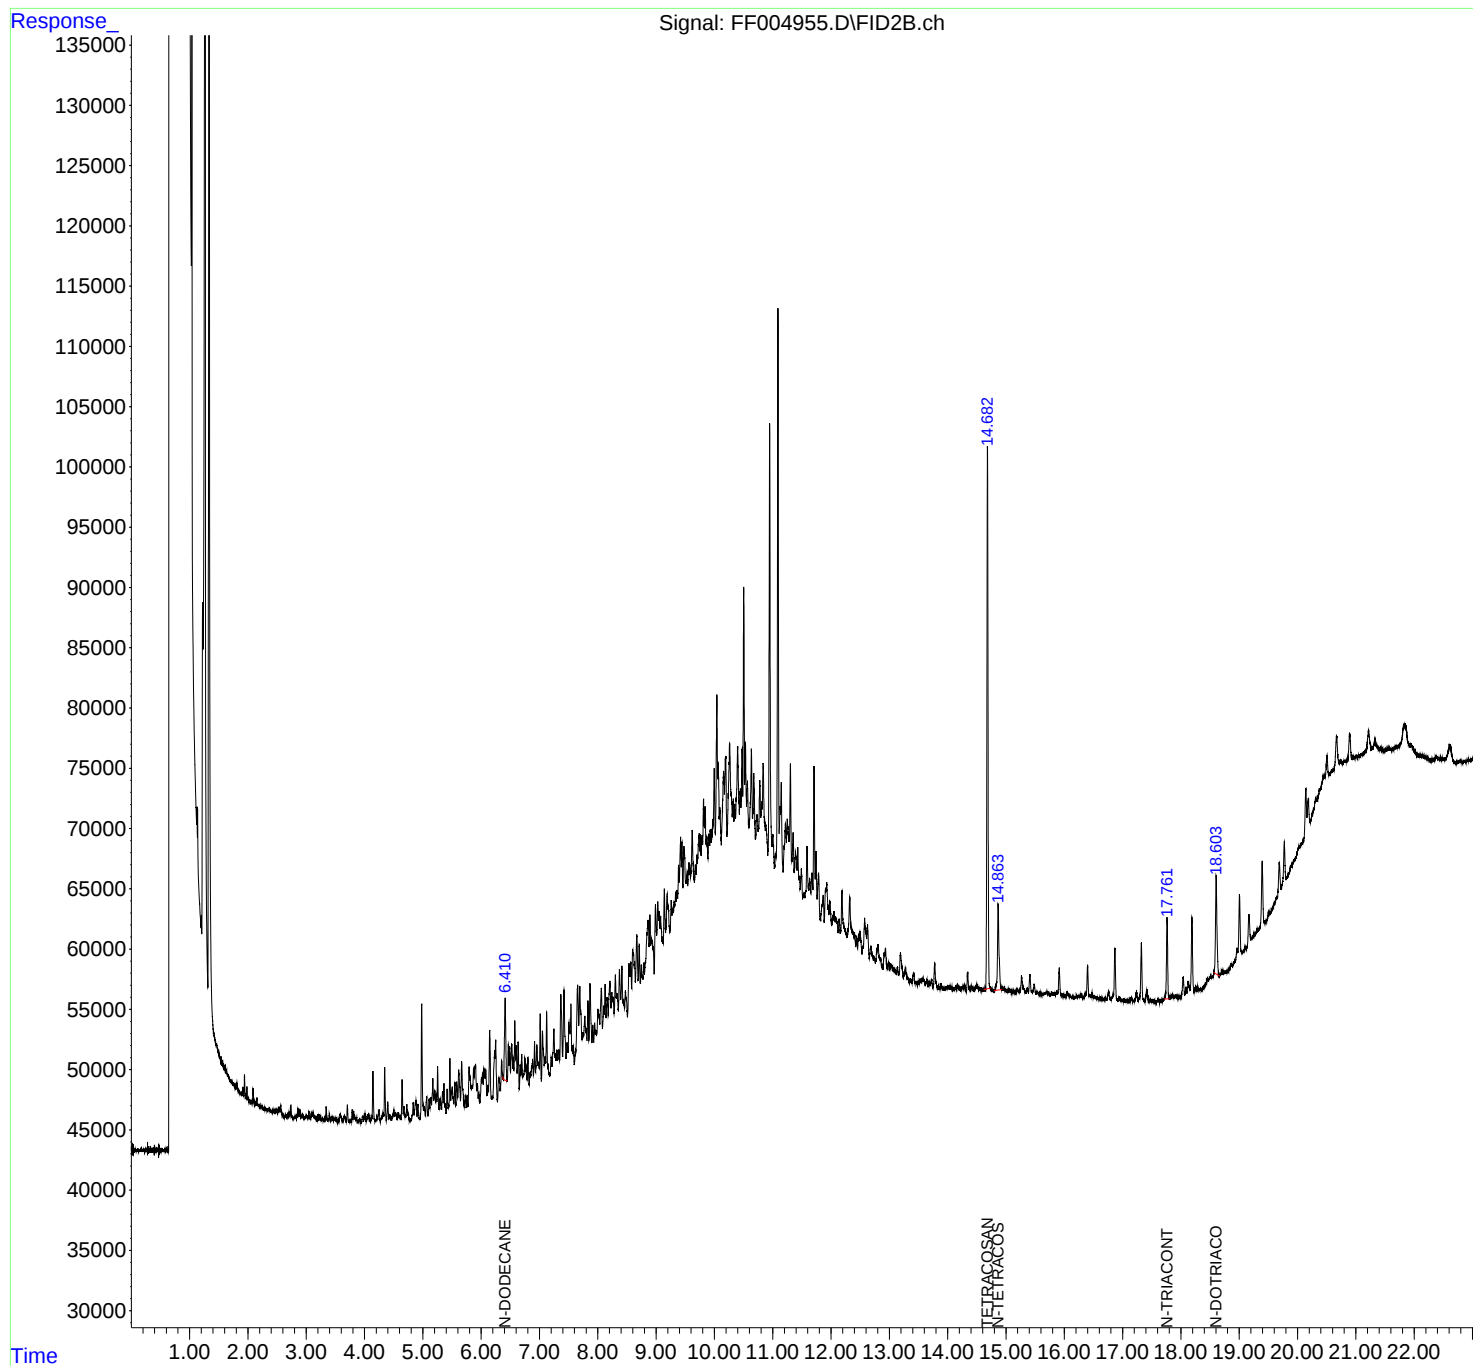


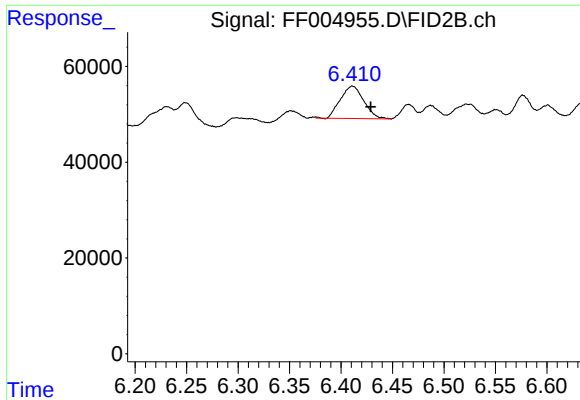

#3 N-DODECANE


R.T.: 6.411 min
Delta R.T.: -0.018 min
Response: 107286
Conc: 0.85 ug/ml

Instrument :
FID_F
ClientSampleId :

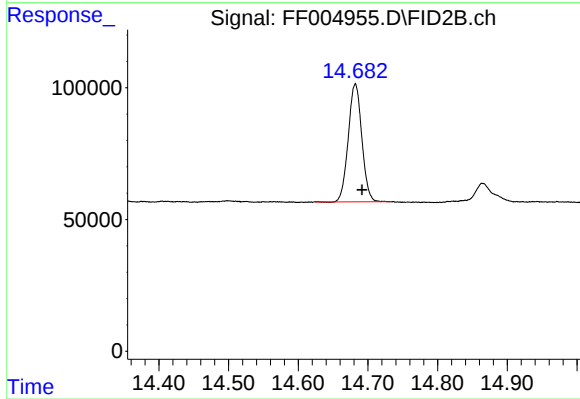


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.682 min
Delta R.T.: -0.010 min
Response: 605302
Conc: 6.22 ug/ml

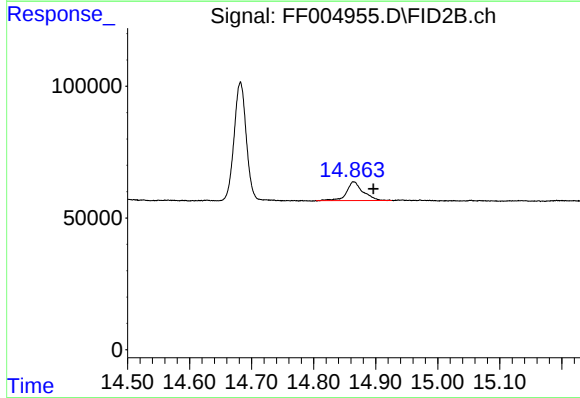


#10 N-TETRACOSANE

R.T.: 14.865 min
Delta R.T.: -0.032 min
Response: 130785
Conc: 1.17 ug/ml

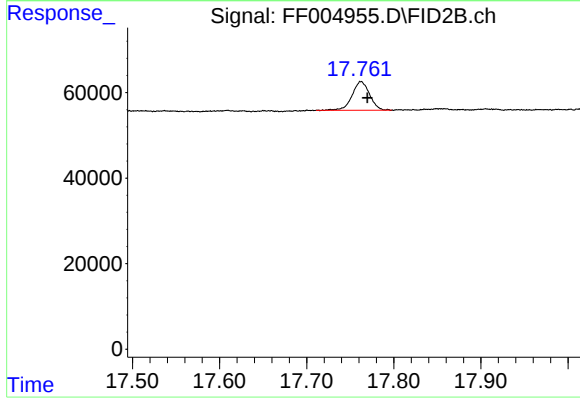

#13 N-TRIACONTANE

R.T.: 17.762 min
Delta R.T.: -0.007 min
Response: 93709
Conc: 0.83 ug/ml

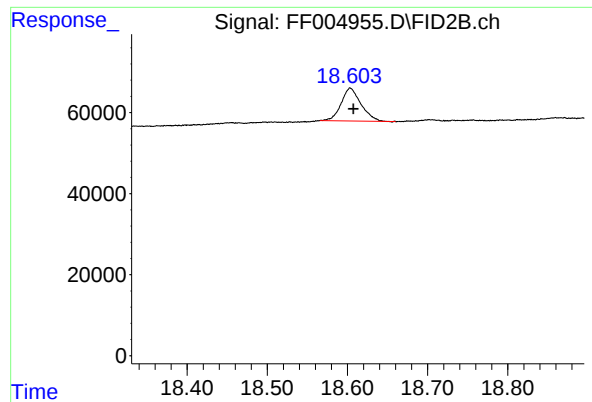

#14 N-DOTRIACONTANE

R.T.: 18.604 min
Delta R.T.: -0.004 min
Response: 139005
Conc: 1.22 ug/ml

Instrument :
FID_F
ClientSampleId :