

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF070219\
Data File : FF004947.D
Signal(s) : FID2B.ch
Acq On : 03 Jul 2019 02:30
Operator : DD\AJ
Sample : PB121097BL
Misc :
ALS Vial : 67 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
PB121097BL

Integration File: Sample.e
Quant Time: Jul 03 05:23:39 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF062619.M
Quant Title :
QLast Update : Wed Jun 26 14:27:24 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.685	2194822	22.567 ug/ml

Target Compounds

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF070219\
Data File : FF004947.D
Signal(s) : FID2B.ch
Acq On : 03 Jul 2019 02:30
Operator : DD\AJ
Sample : PB121097BL
Misc :
ALS Vial : 67 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
PB121097BL

Integration File: Sample.e
Quant Time: Jul 03 05:23:39 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF062619.M
Quant Title :
QLast Update : Wed Jun 26 14:27:24 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

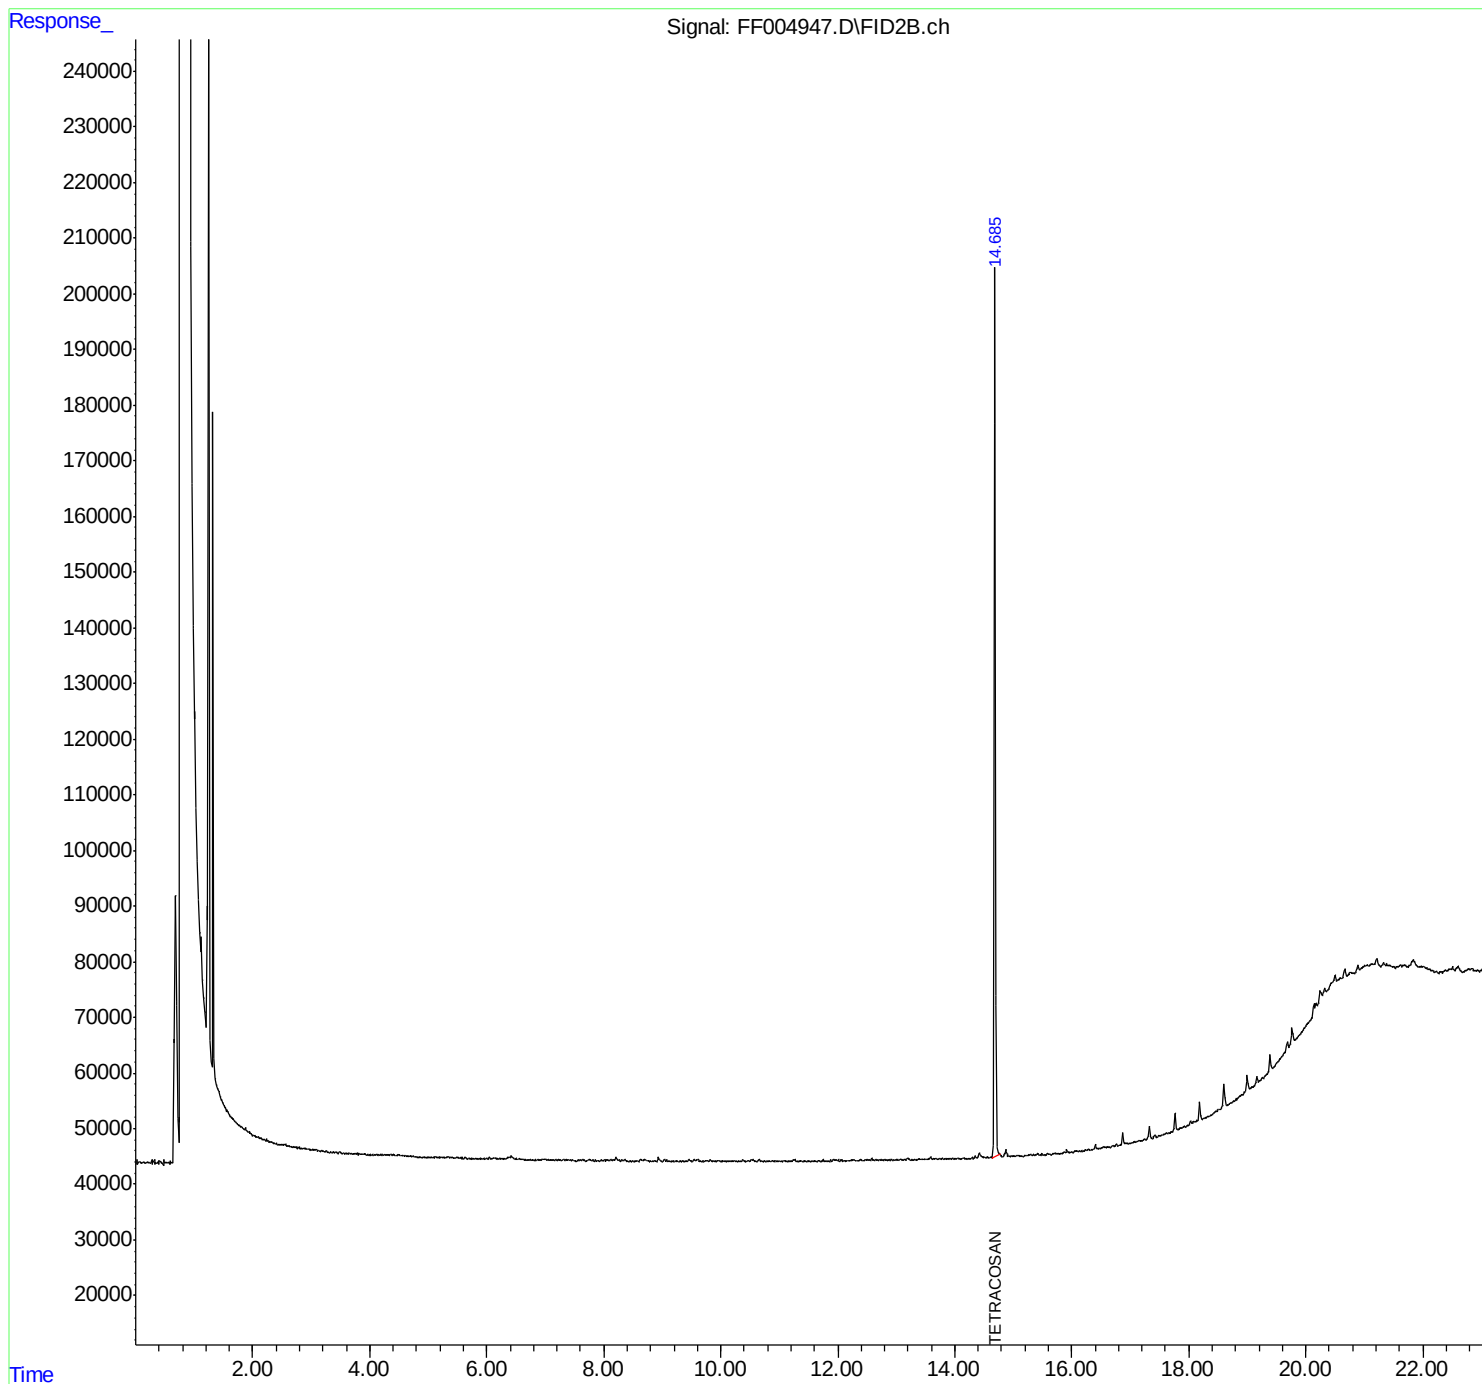

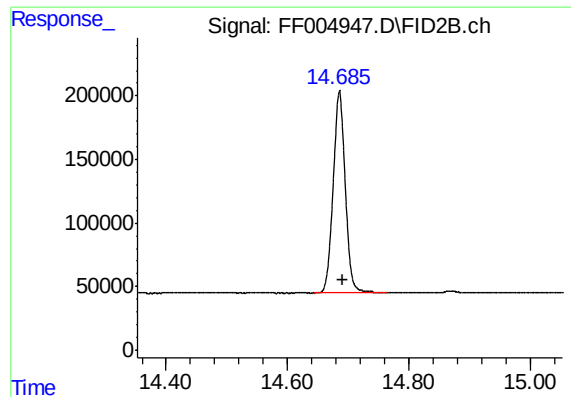

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.685 min
Delta R.T.: -0.006 min
Response: 2194822
Conc: 22.57 ug/ml

Instrument :
FID_F
ClientSampleId :
PB121097BL