

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF070221\
Data File : FF008713.D
Signal(s) : FID2B.ch
Acq On : 02 Jul 2021 10:27
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jul 02 22:42:36 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF062321.M
Quant Title :
QLast Update : Thu Jun 24 08:07:11 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.743	1945480	17.070 ug/ml
Target Compounds			
14) N-DOTRIACONTANE	18.636	611924	5.223 ug/ml
18) N-TETRACONTANE	21.864	1101588	11.903 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF070221\
Data File : FF008713.D
Signal(s) : FID2B.ch
Acq On : 02 Jul 2021 10:27
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jul 02 22:42:36 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF062321.M
Quant Title :
QLast Update : Thu Jun 24 08:07:11 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

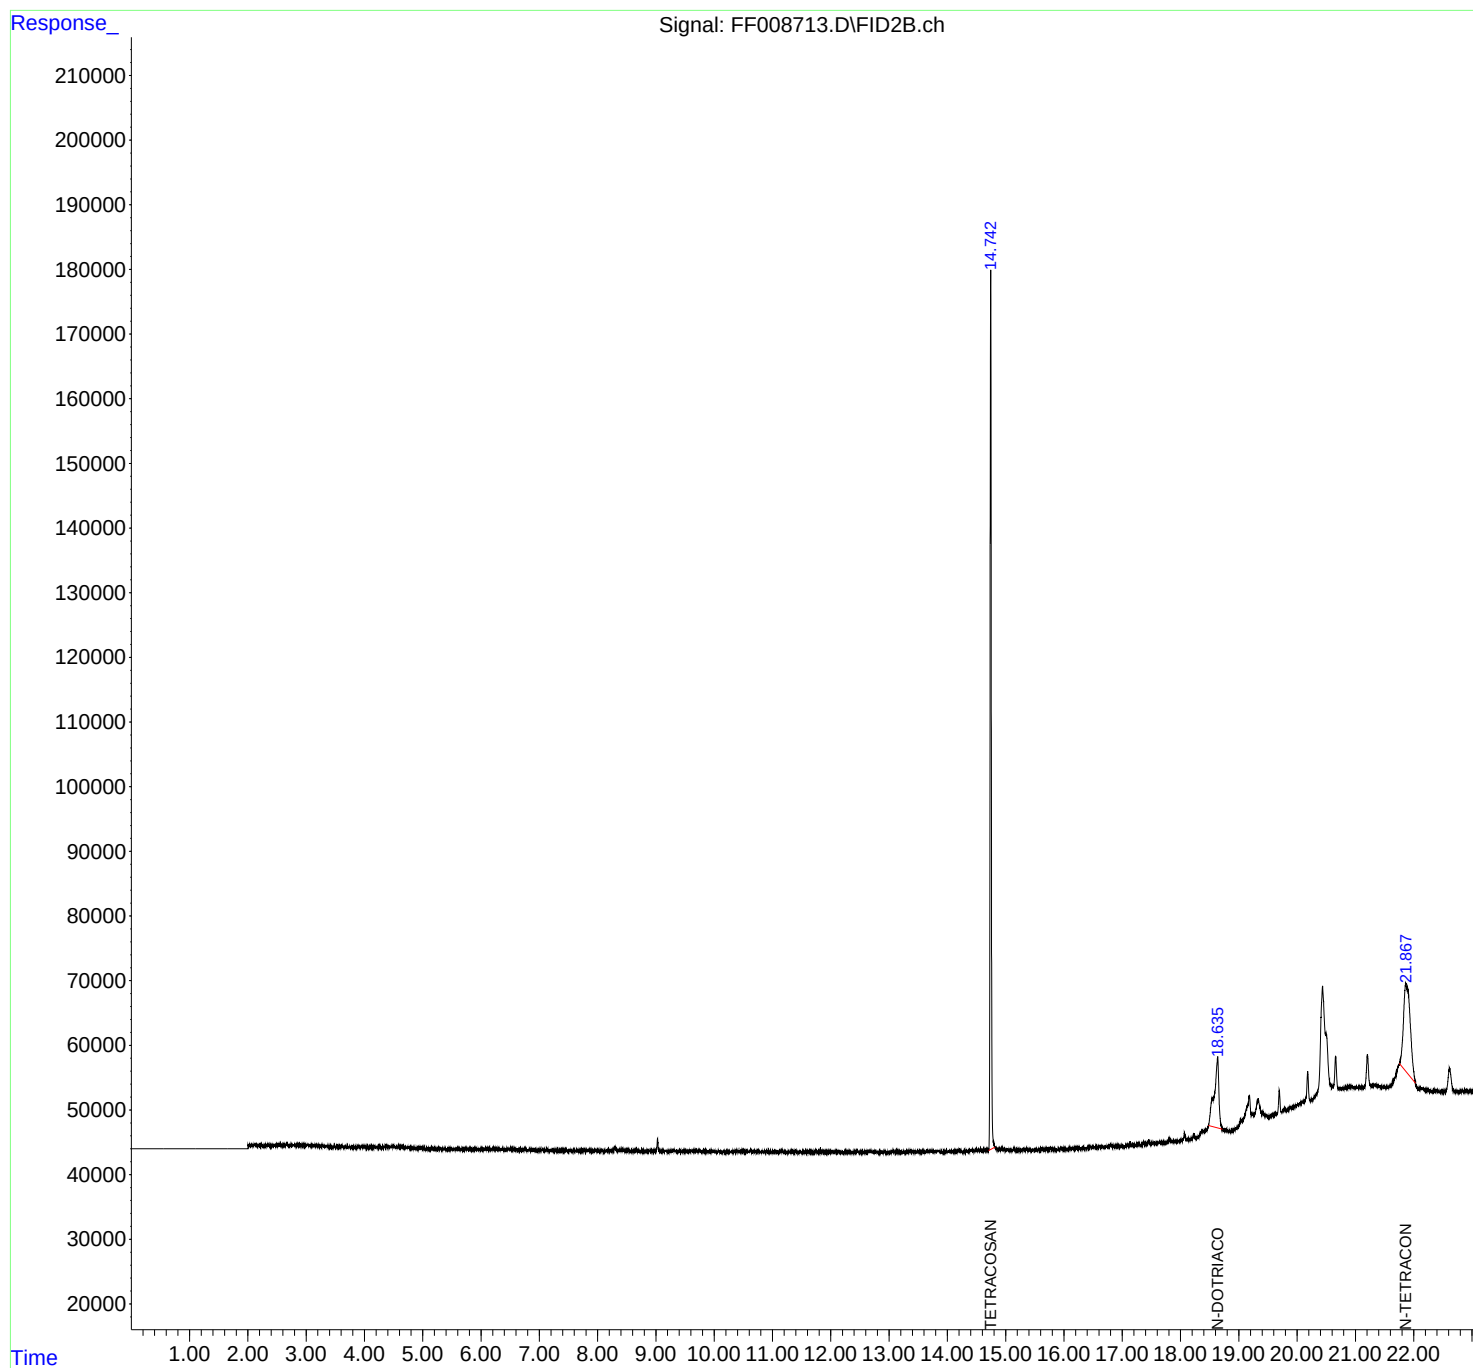


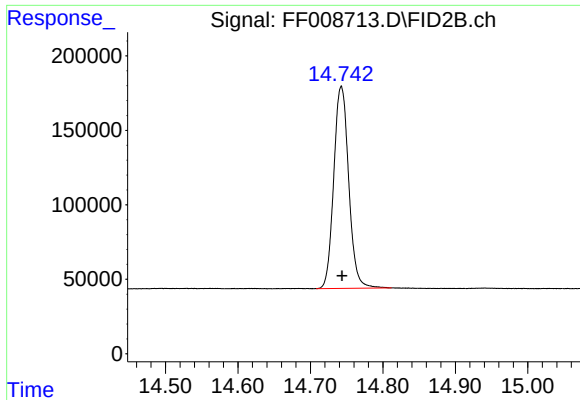

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.743 min
Delta R.T.: -0.001 min
Response: 1945480
Conc: 17.07 ug/ml

Instrument :
FID_F
ClientSampleId :

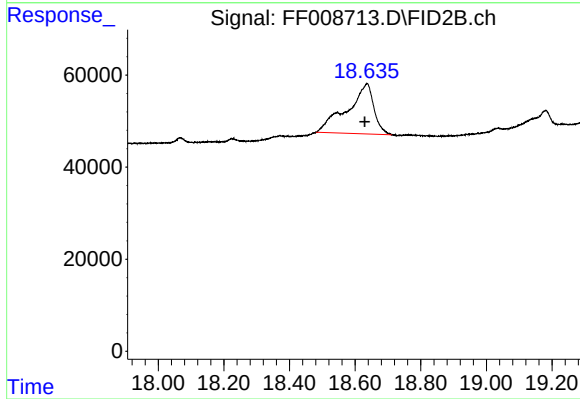

#14 N-DOTRIACONTANE

R.T.: 18.636 min
Delta R.T.: 0.007 min
Response: 611924
Conc: 5.22 ug/ml

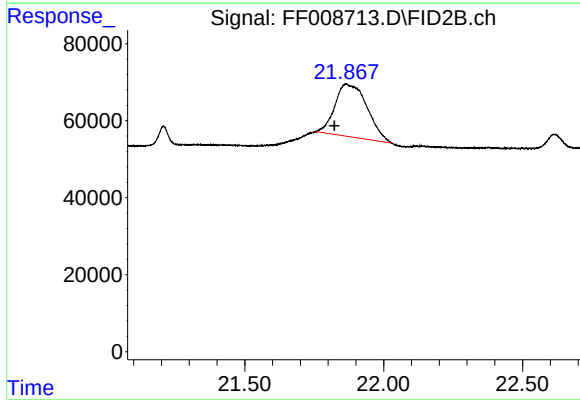

#18 N-TETRACONTANE

R.T.: 21.864 min
Delta R.T.: 0.041 min
Response: 1101588
Conc: 11.90 ug/ml