

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF070221\
 Data File : FF008716.D
 Signal(s) : FID2B.ch
 Acq On : 02 Jul 2021 13:05
 Operator : DD\AJ
 Sample : PB137486BL
 Misc :
 ALS Vial : 55 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jul 02 22:42:58 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF062321.M
 Quant Title :
 QLast Update : Thu Jun 24 08:07:11 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.740	2070817	18.170 ug/ml
Target Compounds			
14) N-DOTRIACONTANE	18.638	229081	1.955 ug/ml
16) N-HEXATRIACONTANE	20.183	386975	4.120 ug/ml
18) N-TETRACONTANE	21.851	810763	8.760 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF070221\
Data File : FF008716.D
Signal(s) : FID2B.ch
Acq On : 02 Jul 2021 13:05
Operator : DD\AJ
Sample : PB137486BL
Misc :
ALS Vial : 55 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jul 02 22:42:58 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF062321.M
Quant Title :
QLast Update : Thu Jun 24 08:07:11 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

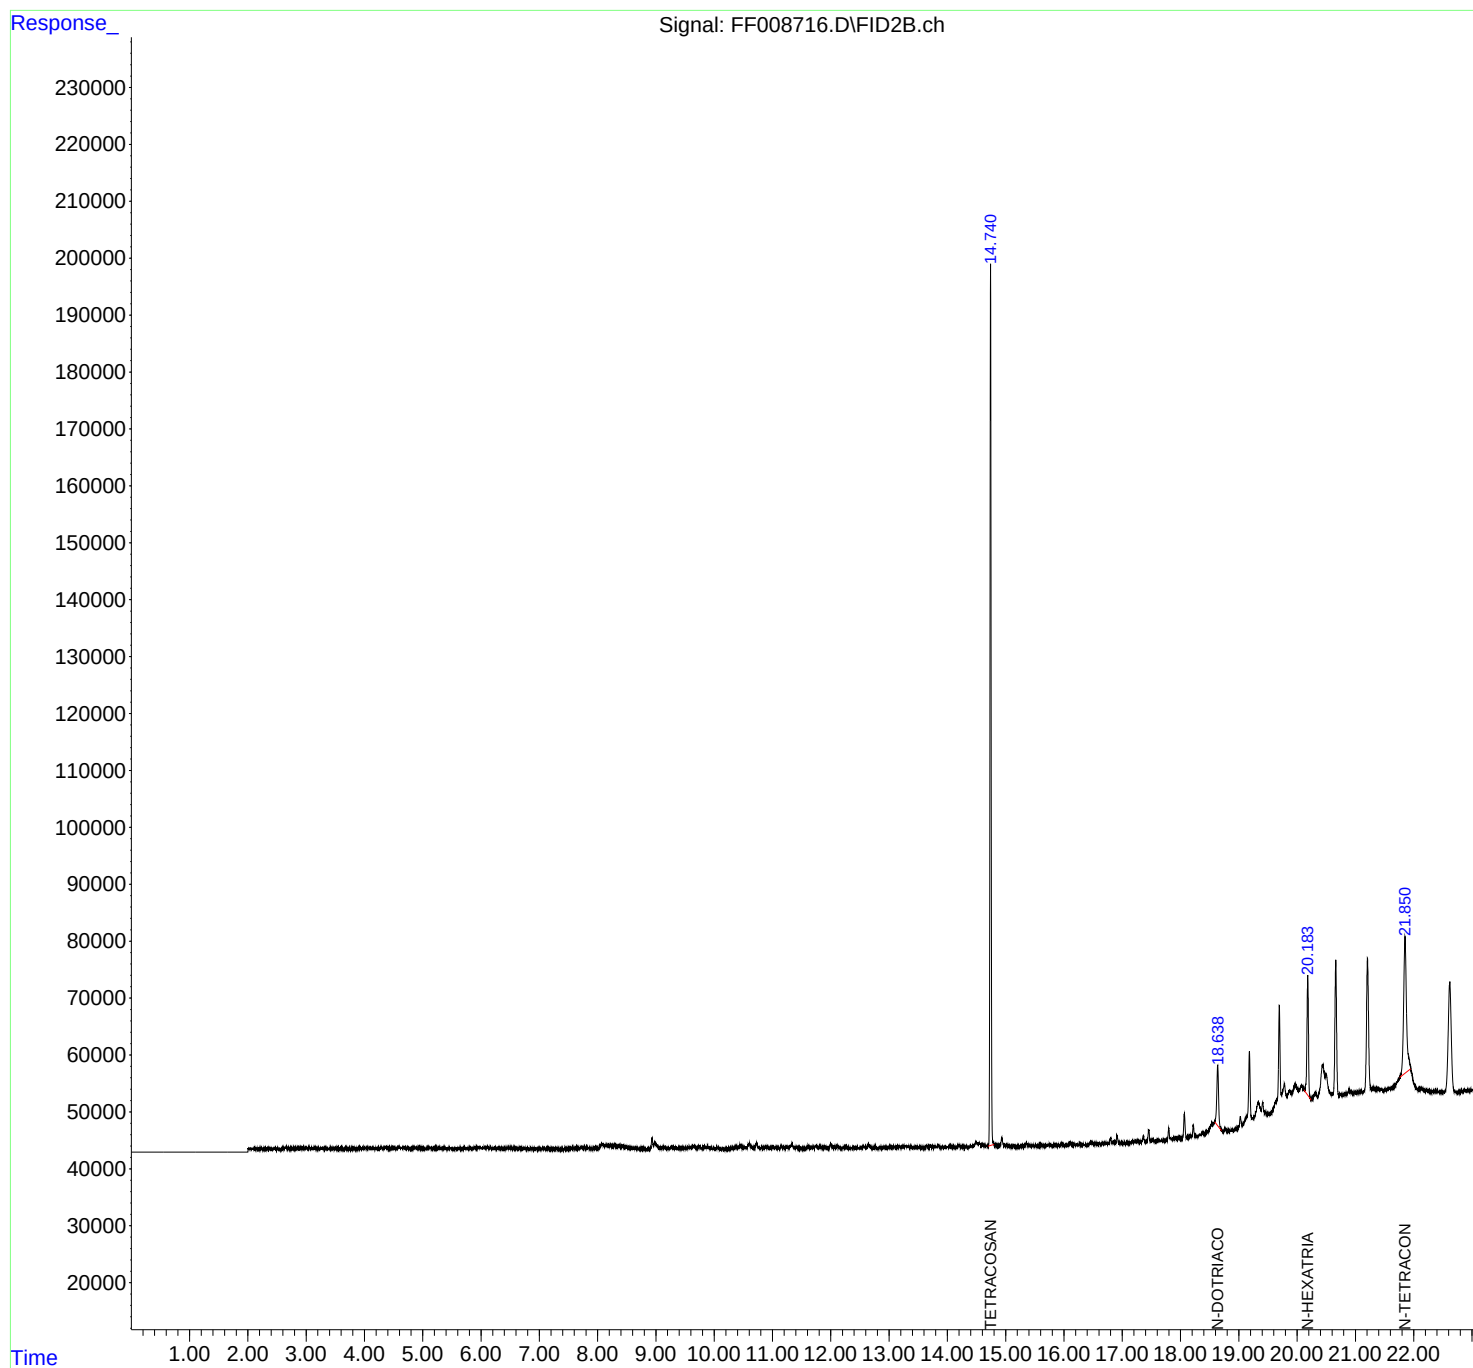


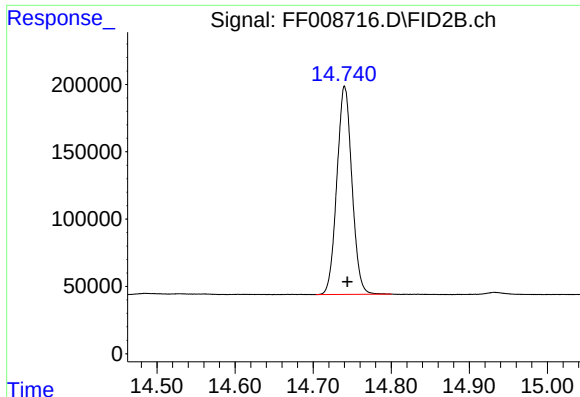

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.740 min
Delta R.T.: -0.004 min
Response: 2070817
Conc: 18.17 ug/ml

Instrument :
FID_F
ClientSampleId :

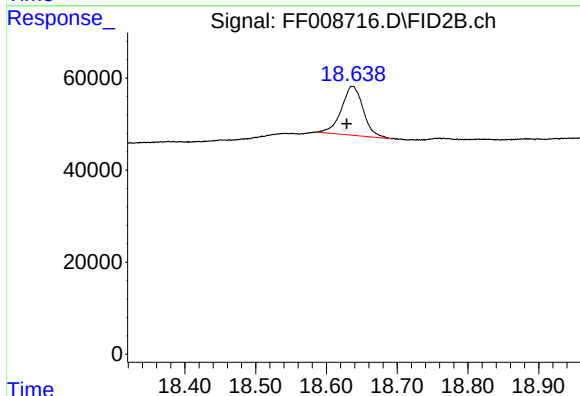


#14 N-DOTRIACONTANE

R.T.: 18.638 min
Delta R.T.: 0.010 min
Response: 229081
Conc: 1.96 ug/ml

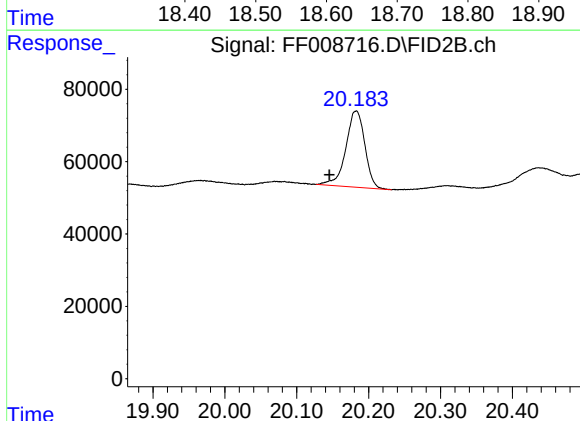

#16 N-HEXATRIACONTANE

R.T.: 20.183 min
Delta R.T.: 0.038 min
Response: 386975
Conc: 4.12 ug/ml

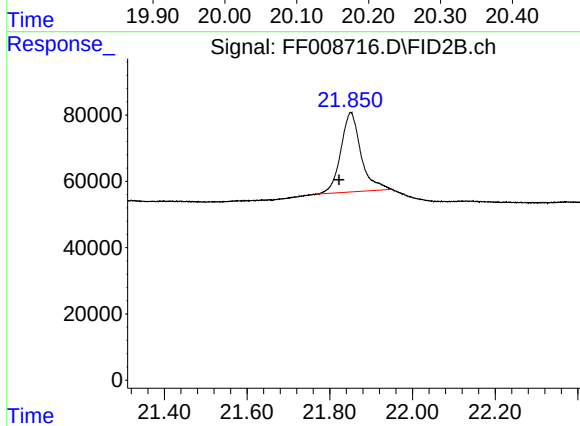

#18 N-TETRACONTANE

R.T.: 21.851 min
Delta R.T.: 0.028 min
Response: 810763
Conc: 8.76 ug/ml