

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF070221\
 Data File : FF008721.D
 Signal(s) : FID2B.ch
 Acq On : 02 Jul 2021 15:40
 Operator : DD\AJ
 Sample : M2913-07
 Misc :
 ALS Vial : 60 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jul 02 22:43:37 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF062321.M
 Quant Title :
 QLast Update : Thu Jun 24 08:07:11 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.749	1555752	13.651 ug/ml
Target Compounds			
4) N-TETRADECANE	8.248f	84379	0.625 ug/ml
7) N-EICOSANE	12.649	178179	1.300 ug/ml
8) N-DOCOSANE	13.893	249978	1.868 ug/ml
10) N-TETRACOSANE	14.945	769572	5.840 ug/ml
12) N-OCTACOSANE	16.946	216618	1.751 ug/ml
13) N-TRIACONTANE	17.801	226962	1.894 ug/ml
14) N-DOTRIACONTANE	18.639	414409	3.537 ug/ml
15) N-TETRATRIACONTANE	19.417	401905	3.844 ug/ml
16) N-HEXATRIACONTANE	20.145	279212	2.973 ug/ml
17) N-OCTATRIACONTANE	20.897	205540	2.493 ug/ml
18) N-TETRACONTANE	21.851	2246385	24.272 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF070221\
Data File : FF008721.D
Signal(s) : FID2B.ch
Acq On : 02 Jul 2021 15:40
Operator : DD\AJ
Sample : M2913-07
Misc :
ALS Vial : 60 Sample Multiplier: 1

Instrument :
FID_F
ClientSampled :

Integration File: autoint1.e
Quant Time: Jul 02 22:43:37 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF062321.M
Quant Title :
QLast Update : Thu Jun 24 08:07:11 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

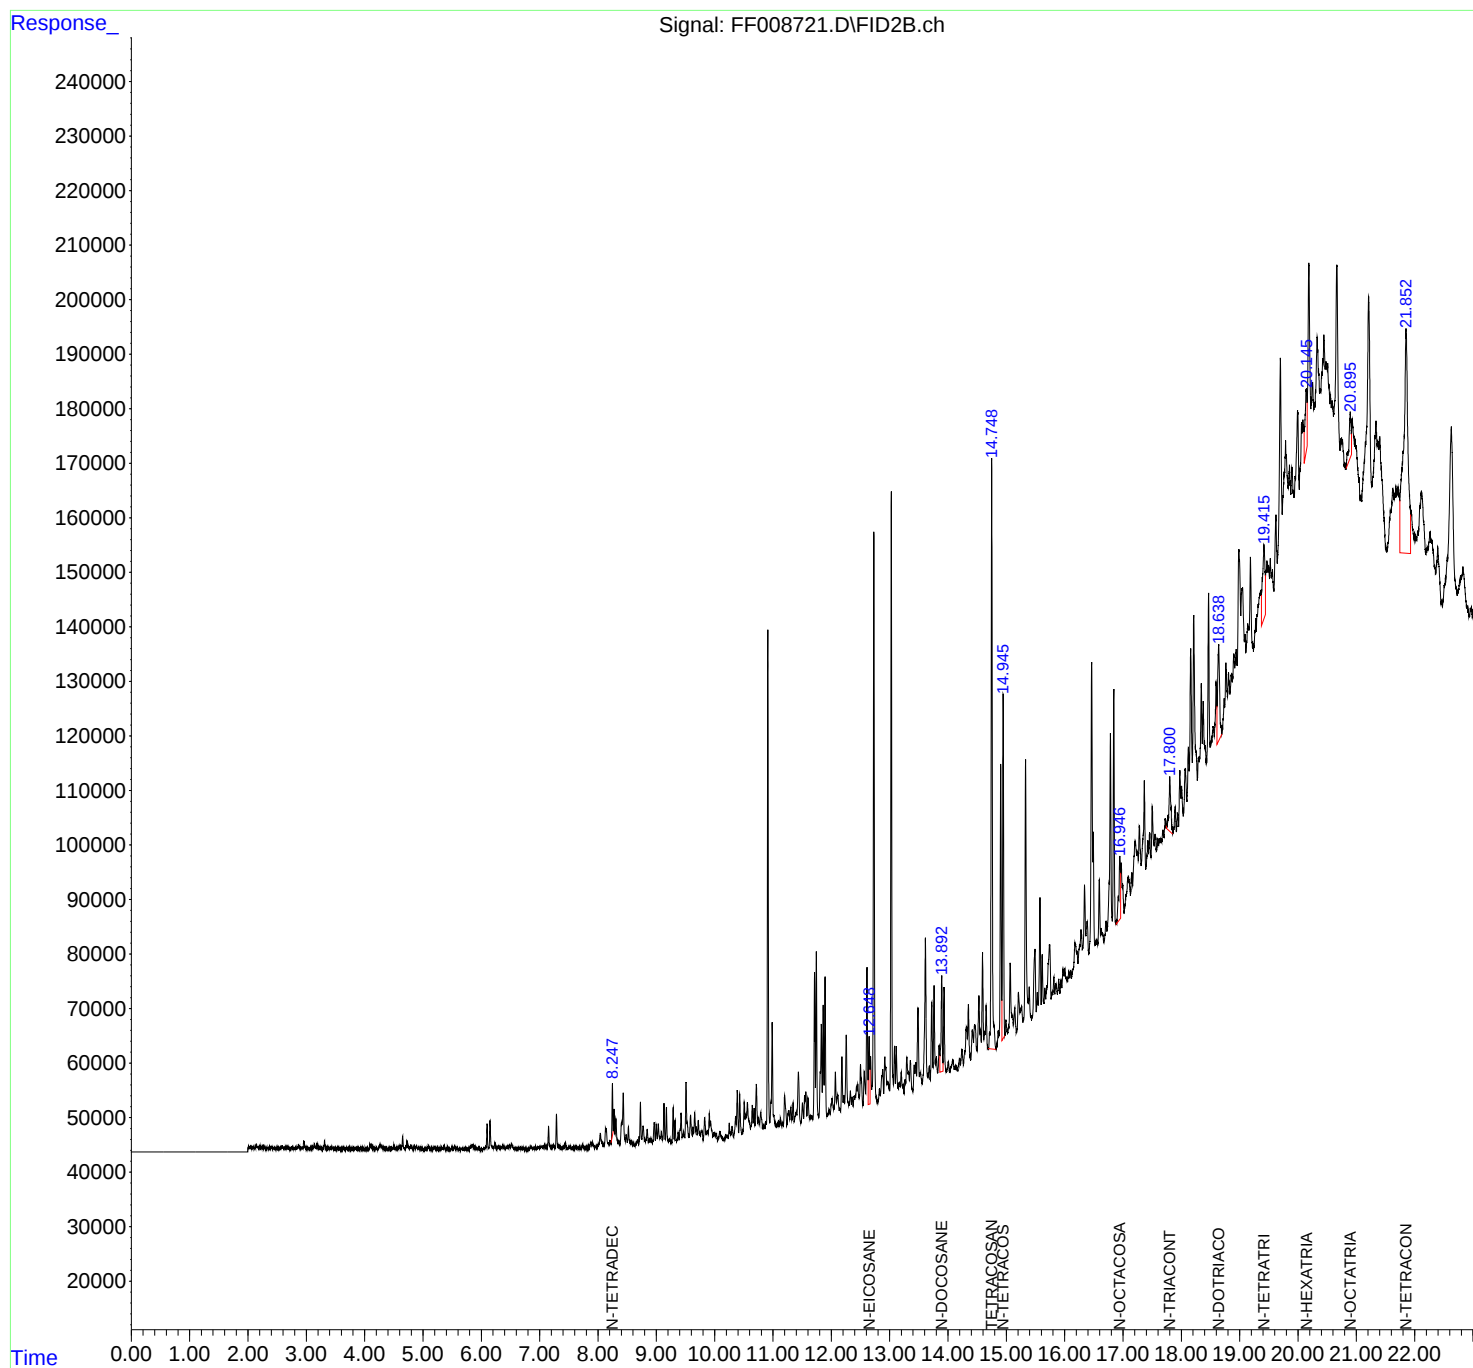


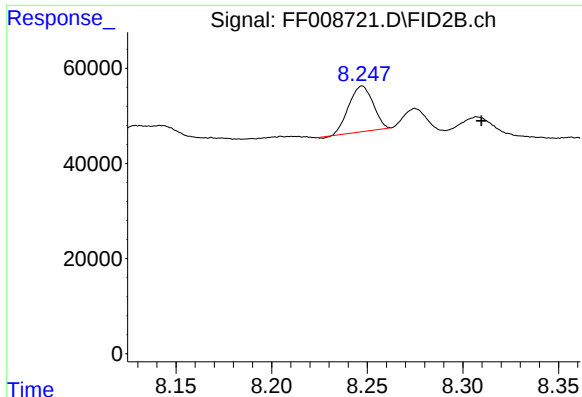

#4 N-TETRADECANE


R.T.: 8.248 min
Delta R.T.: -0.062 min
Response: 84379
Conc: 0.63 ug/ml

Instrument :
FID_F
ClientSampleId :

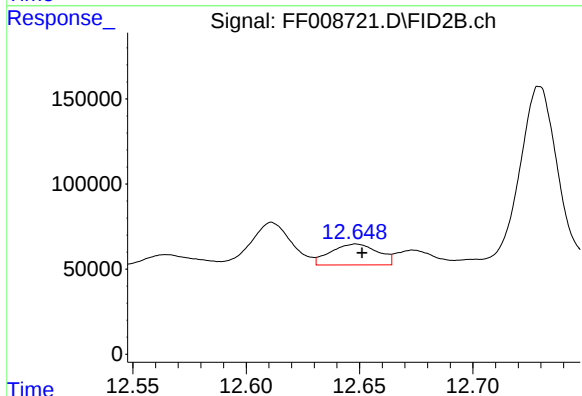


#7 N-EICOSANE

R.T.: 12.649 min
Delta R.T.: -0.003 min
Response: 178179
Conc: 1.30 ug/ml

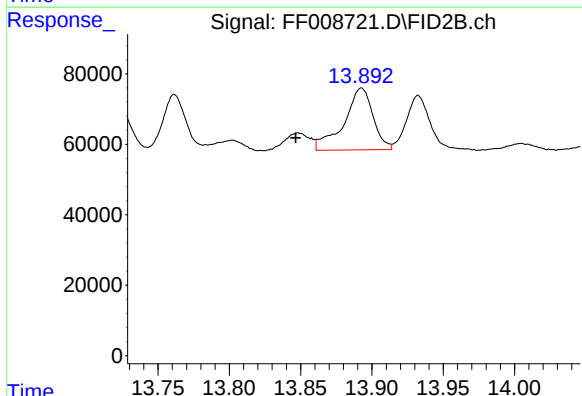


#8 N-DOCOSANE

R.T.: 13.893 min
Delta R.T.: 0.046 min
Response: 249978
Conc: 1.87 ug/ml

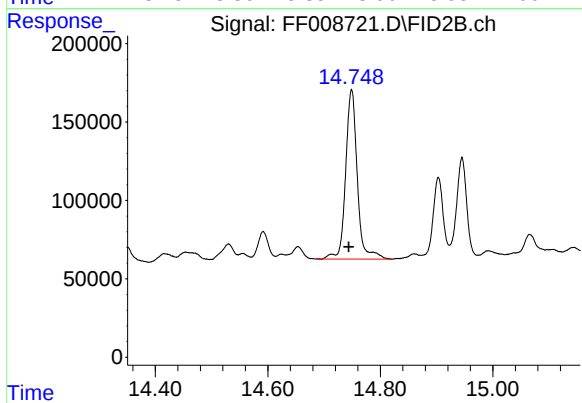

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.749 min
Delta R.T.: 0.005 min
Response: 1555752
Conc: 13.65 ug/ml

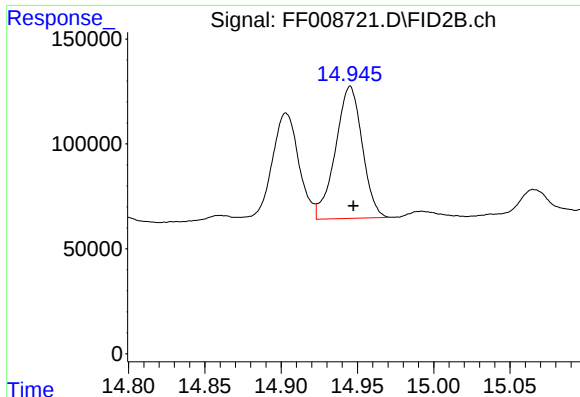

#10 N-TETRACOSANE


R.T.: 14.945 min
Delta R.T.: -0.002 min
Response: 769572
Conc: 5.84 ug/ml

Instrument :
FID_F
ClientSampleId :

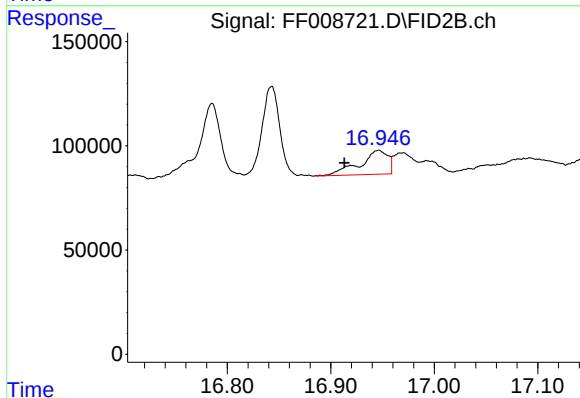


#12 N-OCTACOSANE

R.T.: 16.946 min
Delta R.T.: 0.033 min
Response: 216618
Conc: 1.75 ug/ml

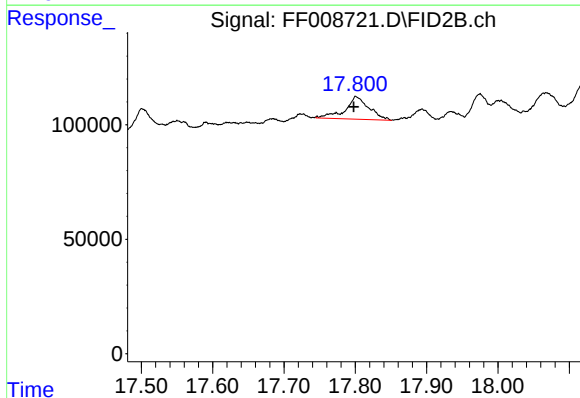


#13 N-TRIACONTANE

R.T.: 17.801 min
Delta R.T.: 0.003 min
Response: 226962
Conc: 1.89 ug/ml

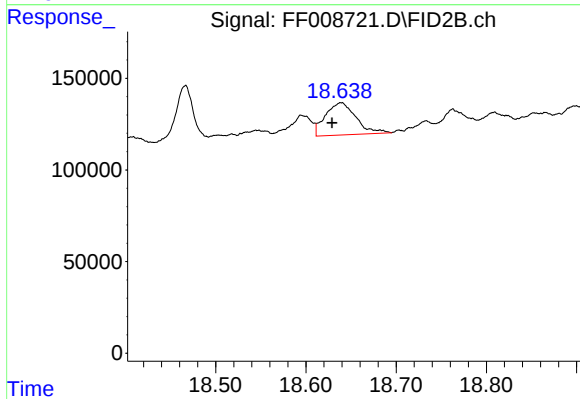

#14 N-DOTRIACONTANE


R.T.: 18.639 min
Delta R.T.: 0.010 min
Response: 414409
Conc: 3.54 ug/ml

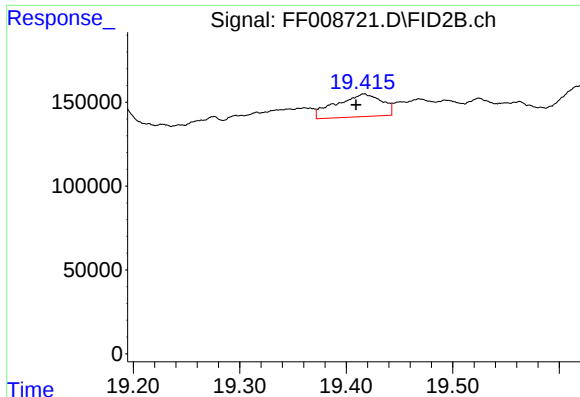

#15 N-TETRATRIACONTANE


R.T.: 19.417 min
Delta R.T.: 0.008 min
Response: 401905
Conc: 3.84 ug/ml

Instrument :
FID_F
ClientSampleId :

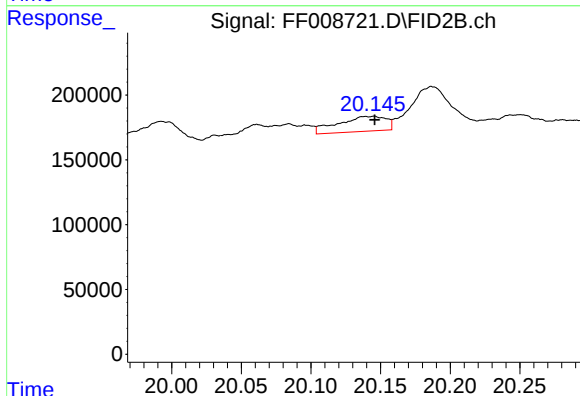


#16 N-HEXATRIACONTANE

R.T.: 20.145 min
Delta R.T.: 0.000 min
Response: 279212
Conc: 2.97 ug/ml

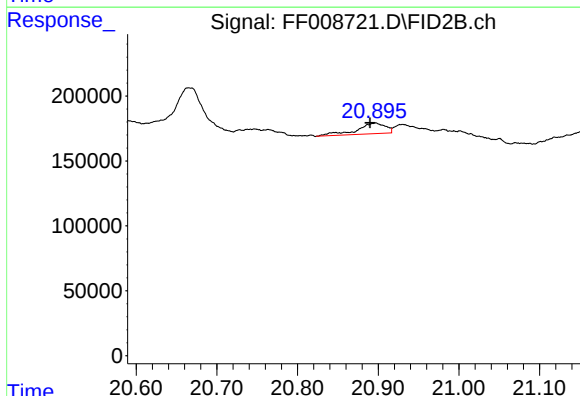

#17 N-OCTATRIACONTANE

R.T.: 20.897 min
Delta R.T.: 0.007 min
Response: 205540
Conc: 2.49 ug/ml

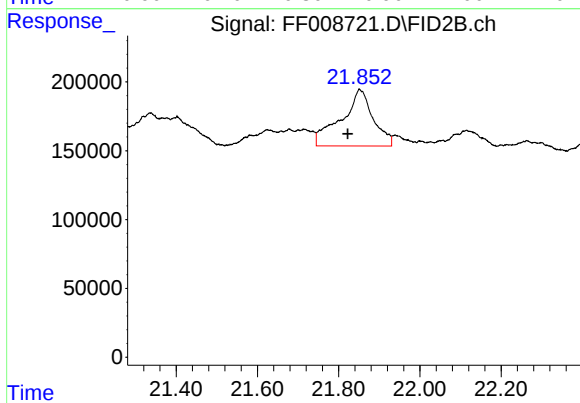

#18 N-TETRACONTANE

R.T.: 21.851 min
Delta R.T.: 0.029 min
Response: 2246385
Conc: 24.27 ug/ml