

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF070221\
 Data File : FF008724.D
 Signal(s) : FID2B.ch
 Acq On : 02 Jul 2021 17:14
 Operator : DD\AJ
 Sample : M2913-01 10X
 Misc :
 ALS Vial : 63 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jul 02 22:44:03 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF062321.M
 Quant Title :
 QLast Update : Thu Jun 24 08:07:11 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.747	162120	1.422 ug/ml
Target Compounds			
10) N-TETRACOSANE	14.944	166365	1.263 ug/ml
14) N-DOTRIACONTANE	18.636	148775	1.270 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF070221\
Data File : FF008724.D
Signal(s) : FID2B.ch
Acq On : 02 Jul 2021 17:14
Operator : DD\AJ
Sample : M2913-01 10X
Misc :
ALS Vial : 63 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jul 02 22:44:03 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF062321.M
Quant Title :
QLast Update : Thu Jun 24 08:07:11 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

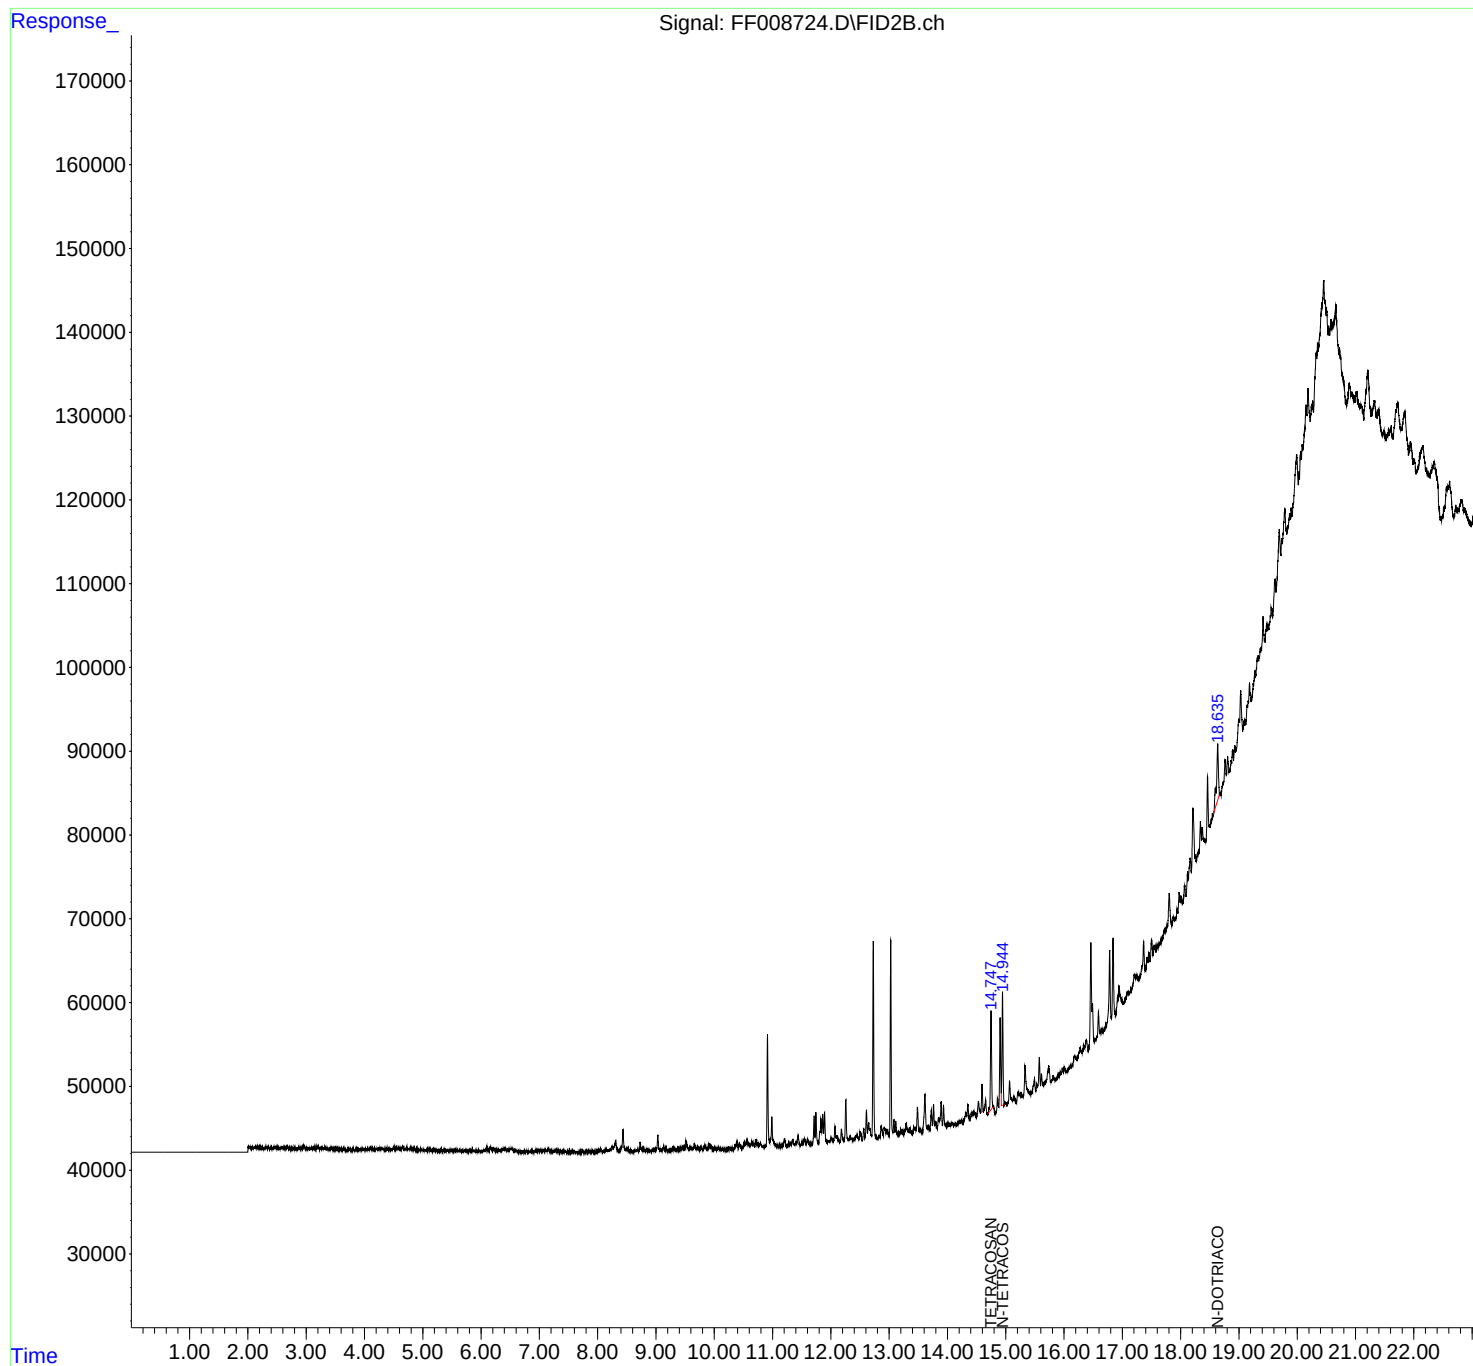


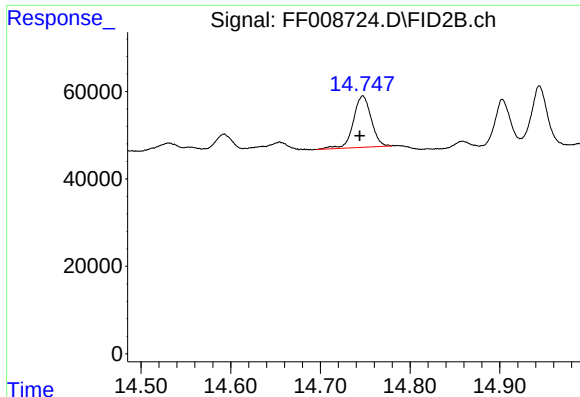

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.747 min
Delta R.T.: 0.004 min
Response: 162120
Conc: 1.42 ug/ml

Instrument :
FID_F
ClientSampleId :

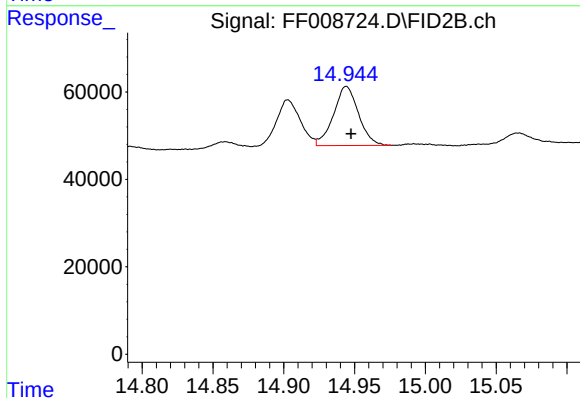

#10 N-TETRACOSANE

R.T.: 14.944 min
Delta R.T.: -0.003 min
Response: 166365
Conc: 1.26 ug/ml

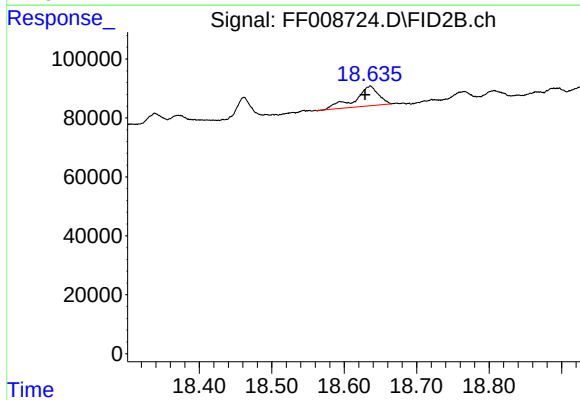

#14 N-DOTRIACONTANE

R.T.: 18.636 min
Delta R.T.: 0.007 min
Response: 148775
Conc: 1.27 ug/ml