

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_F\Data\FF070221\  
 Data File : FF008715.D  
 Signal(s) : FID2B.ch  
 Acq On : 02 Jul 2021 11:32  
 Operator : DD\AJ  
 Sample : RT MARKER  
 Misc :  
 ALS Vial : 54 Sample Multiplier: 1

Instrument :  
 FID\_F  
 ClientSampleId :  
 RT MARKER

Integration File: autoint1.e  
 Quant Time: Jul 02 22:42:51 2021  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_F\Method\FF062321.M  
 Quant Title :  
 QLast Update : Thu Jun 24 08:07:11 2021  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1uL  
 Signal Phase : Rxi-1ms  
 Signal Info : 20mx0.18mmx0.18um

| Compound                    | R.T.   | Response | Conc Units   |
|-----------------------------|--------|----------|--------------|
| -----                       |        |          |              |
| System Monitoring Compounds |        |          |              |
| Target Compounds            |        |          |              |
| 3) N-DODECANE               | 6.515  | 2807451  | 20.642 ug/ml |
| 12) N-OCTACOSANE            | 16.914 | 2397285  | 19.382 ug/ml |
| -----                       |        |          |              |

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_F\Data\FF070221\  
Data File : FF008715.D  
Signal(s) : FID2B.ch  
Acq On : 02 Jul 2021 11:32  
Operator : DD\AJ  
Sample : RT MARKER  
Misc :  
ALS Vial : 54 Sample Multiplier: 1

Instrument :  
FID\_F  
ClientSampleId :  
RT MARKER

Integration File: autoint1.e  
Quant Time: Jul 02 22:42:51 2021  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_F\Method\FF062321.M  
Quant Title :  
QLast Update : Thu Jun 24 08:07:11 2021  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1uL  
Signal Phase : Rxi-1ms  
Signal Info : 20mx0.18mmx0.18um

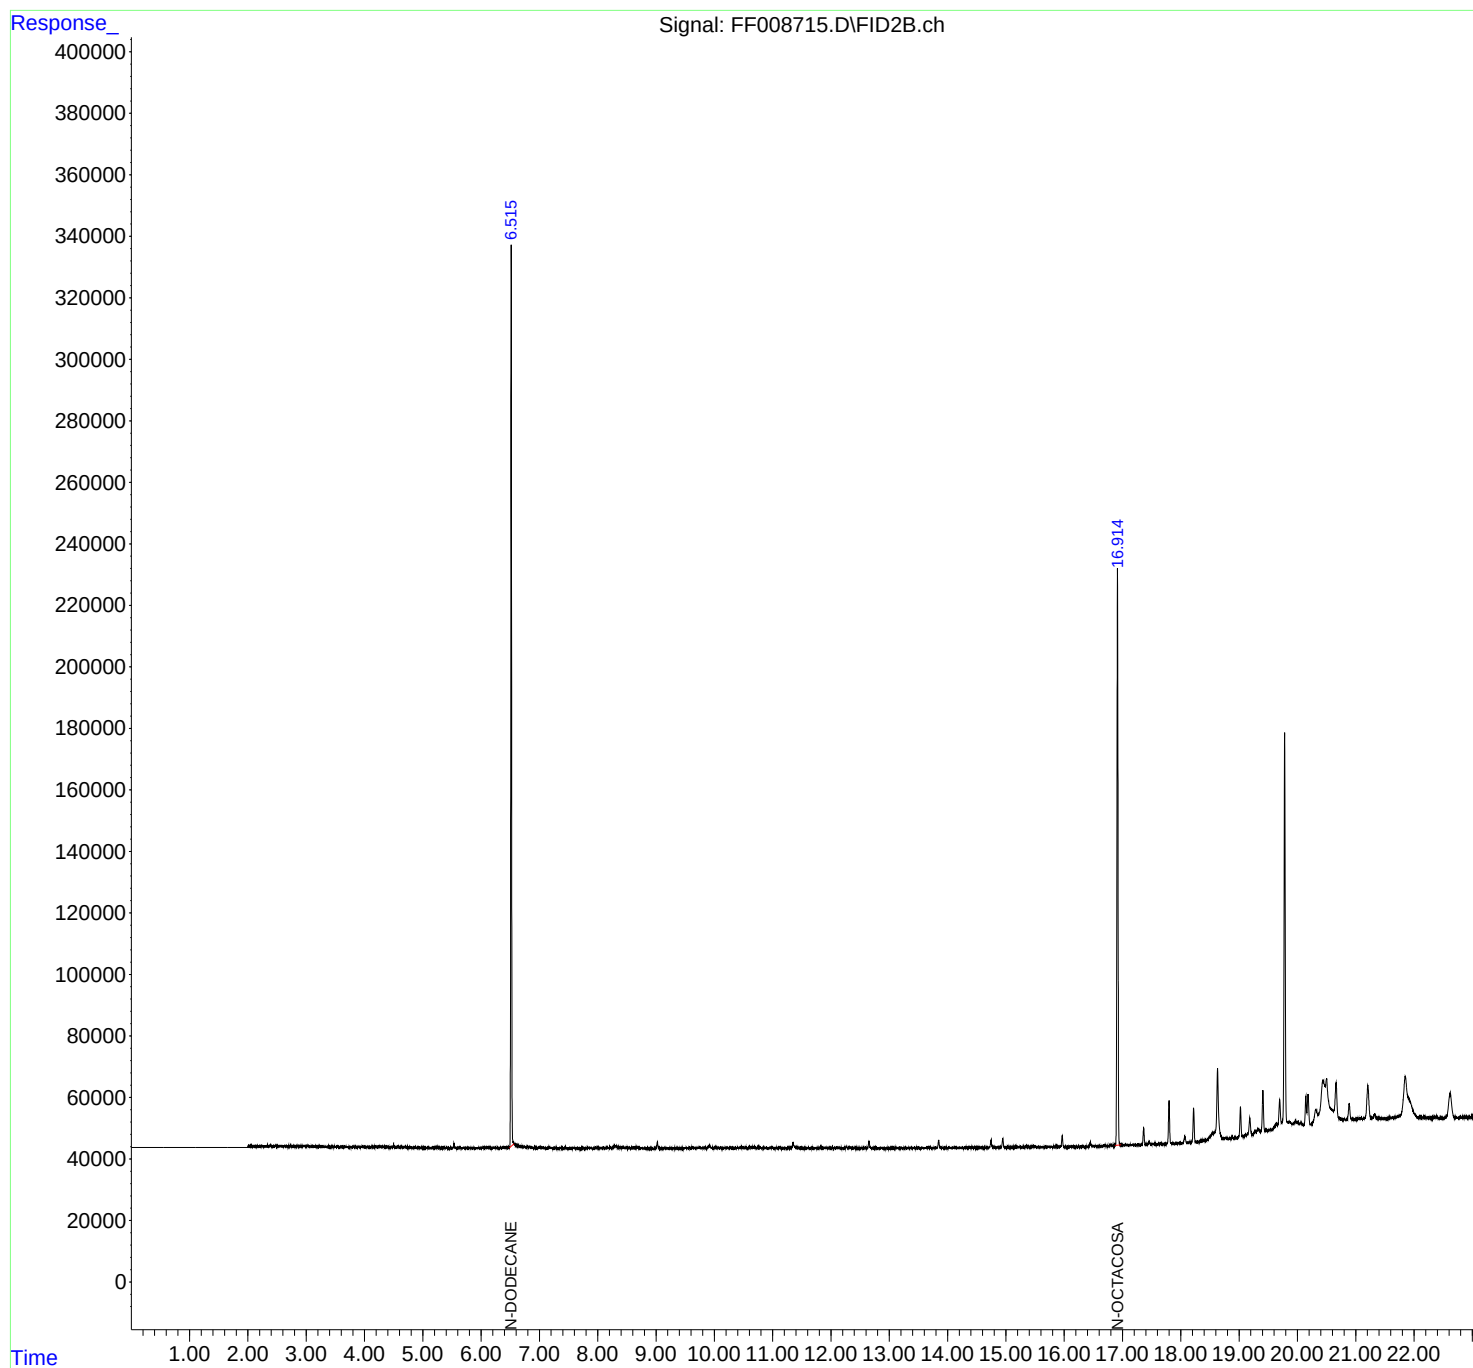


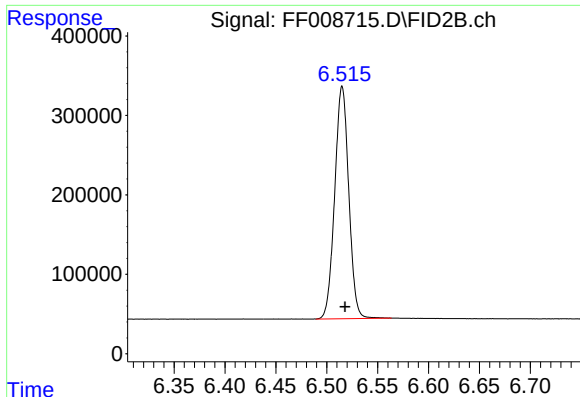

#3 N-DODECANE


R.T.: 6.515 min  
Delta R.T.: -0.003 min  
Response: 2807451  
Conc: 20.64 ug/ml

Instrument :  
FID\_F  
ClientSampleId :  
RT MARKER

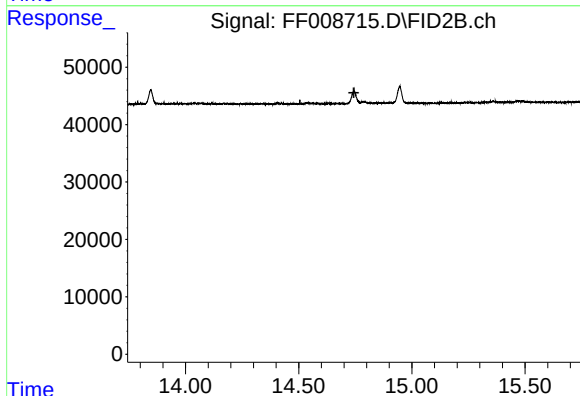

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min  
Exp R.T. : 14.744 min  
Response: 0  
Conc: N.D.

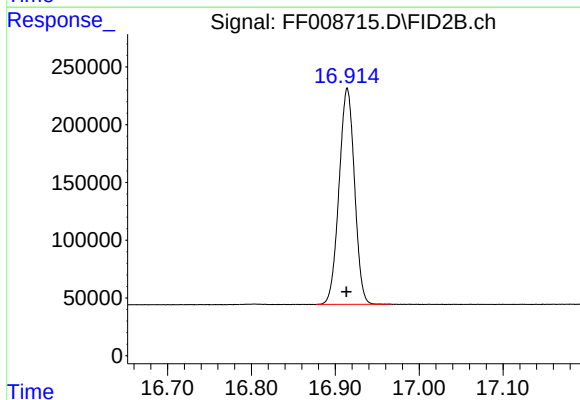

#12 N-OCTACOSANE

R.T.: 16.914 min  
Delta R.T.: 0.001 min  
Response: 2397285  
Conc: 19.38 ug/ml