

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF070222\
 Data File : FF010982.D
 Signal(s) : FID2B.ch
 Acq On : 02 Jul 2022 14:28
 Operator : AJ\MA
 Sample : N3564-29 10X
 Misc :
 ALS Vial : 63 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jul 03 22:12:13 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF063022.M
 Quant Title :
 QLast Update : Fri Jul 01 01:40:42 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.815	113146	1.206 ug/ml
Target Compounds			
7) N-EICOSANE	12.717	102244	0.951 ug/ml
8) N-DOCOSANE	13.915	298129	2.815 ug/ml
10) N-TETRACOSANE	15.017	678243	6.469 ug/ml
11) N-HEXACOSANE	16.037	1012727	9.719 ug/ml
12) N-OCTACOSANE	16.986	937145	8.979 ug/ml
13) N-TRIACONTANE	17.871	632929	6.029 ug/ml
14) N-DOTRIACONTANE	18.702	408934	3.810 ug/ml
15) N-TETRATRIACONTANE	19.483	321168	3.294 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF070222\
Data File : FF010982.D
Signal(s) : FID2B.ch
Acq On : 02 Jul 2022 14:28
Operator : AJ\MA
Sample : N3564-29 10X
Misc :
ALS Vial : 63 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jul 03 22:12:13 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF063022.M
Quant Title :
QLast Update : Fri Jul 01 01:40:42 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

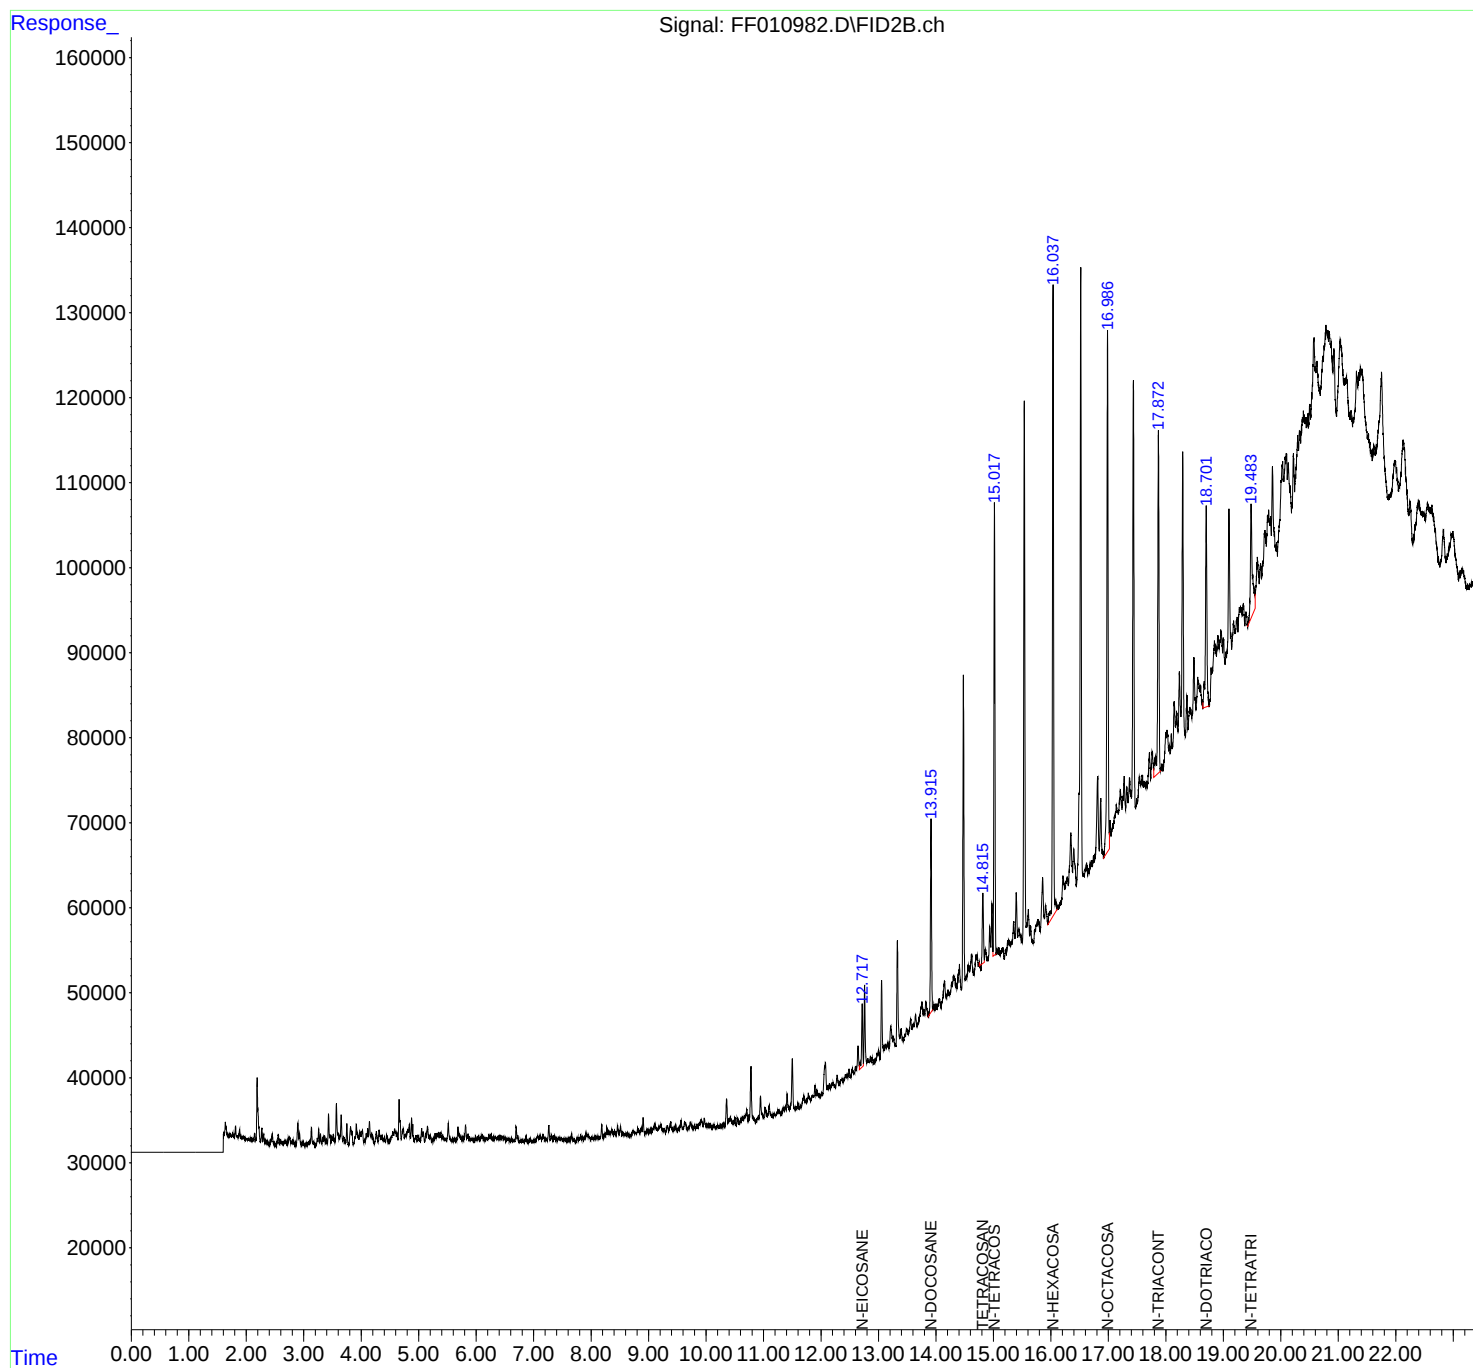


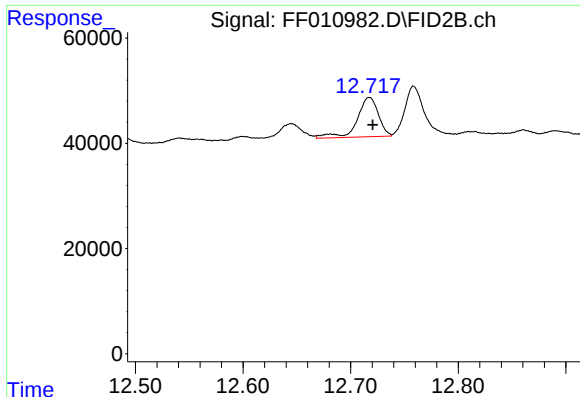

#7 N-EICOSANE


R.T.: 12.717 min
Delta R.T.: -0.003 min
Response: 102244
Conc: 0.95 ug/ml

Instrument :
FID_F
ClientSampleId :

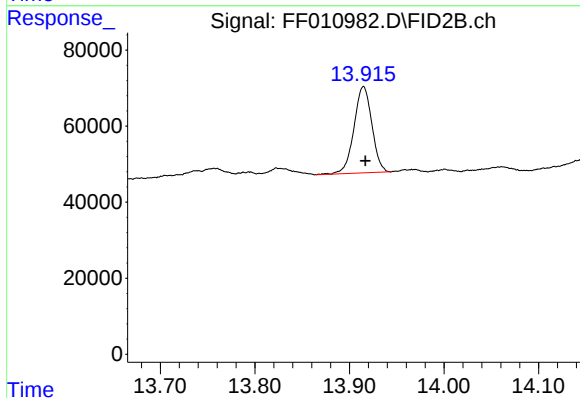


#8 N-DOCOSANE

R.T.: 13.915 min
Delta R.T.: -0.002 min
Response: 298129
Conc: 2.81 ug/ml

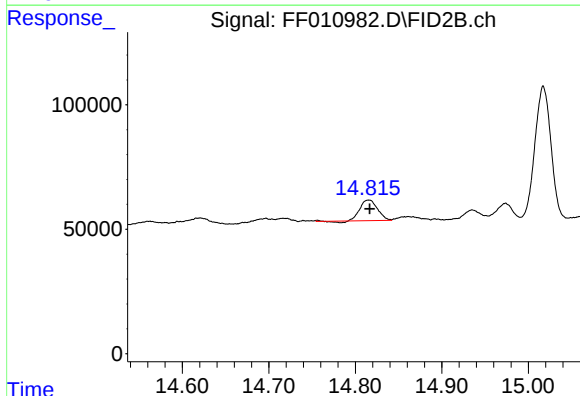


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.815 min
Delta R.T.: -0.002 min
Response: 113146
Conc: 1.21 ug/ml

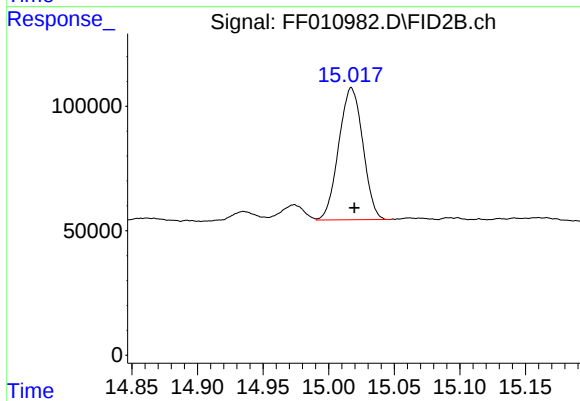

#10 N-TETRACOSANE


R.T.: 15.017 min
Delta R.T.: -0.002 min
Response: 678243
Conc: 6.47 ug/ml

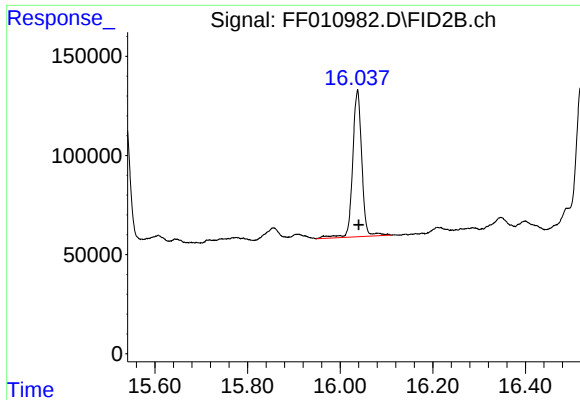

#11 N-HEXACOSANE


R.T.: 16.037 min
Delta R.T.: -0.003 min
Response: 1012727
Conc: 9.72 ug/ml

Instrument :
FID_F
ClientSampleId :

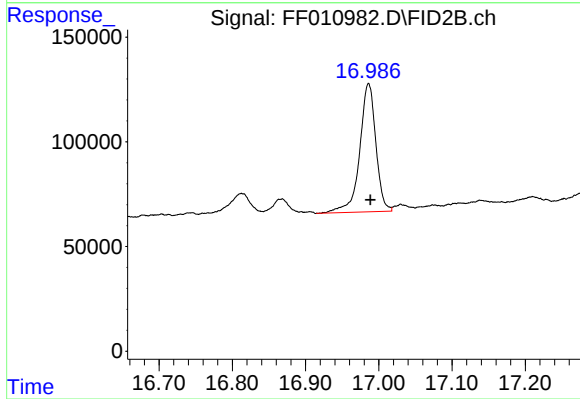


#12 N-OCTACOSANE

R.T.: 16.986 min
Delta R.T.: -0.003 min
Response: 937145
Conc: 8.98 ug/ml

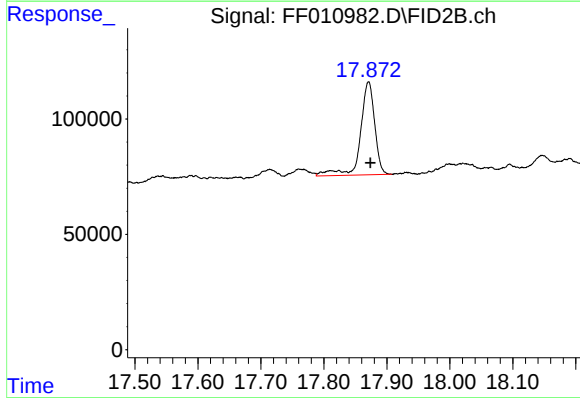


#13 N-TRIACONTANE

R.T.: 17.871 min
Delta R.T.: -0.003 min
Response: 632929
Conc: 6.03 ug/ml

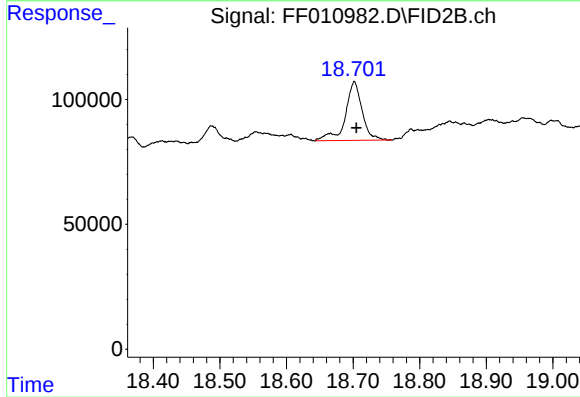

#14 N-DOTRIACONTANE

R.T.: 18.702 min
Delta R.T.: -0.003 min
Response: 408934
Conc: 3.81 ug/ml

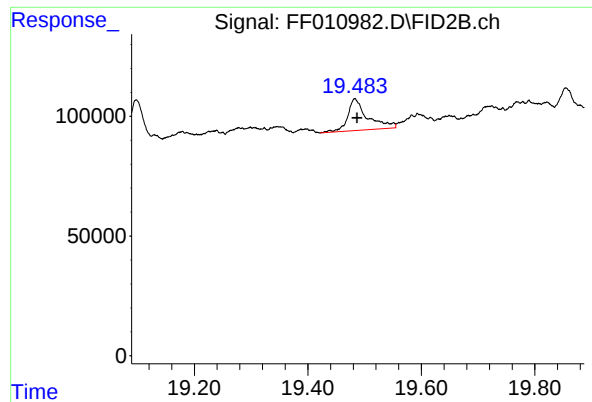

#15 N-TETRATRIACONTANE

R.T.: 19.483 min
Delta R.T.: -0.004 min
Response: 321168
Conc: 3.29 ug/ml

Instrument :

FID_F

ClientSampleId :