

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF070222\
 Data File : FF010981.D
 Signal(s) : FID2B.ch
 Acq On : 02 Jul 2022 13:59
 Operator : AJ\MA
 Sample : N3564-24 10X
 Misc :
 ALS Vial : 62 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :
 WC-16-2-5-GR

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 07/05/2022
 Supervised By :Ankita Jodhani 07/05/2022

Integration File: autoint1.e
 Quant Time: Jul 03 22:12:00 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF063022.M
 Quant Title :
 QLast Update : Fri Jul 01 01:40:42 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.810	85892	0.916 ug/mlm
Target Compounds			

(f)=RT Delta > 1/2 Window

(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF070222\
Data File : FF010981.D
Signal(s) : FID2B.ch
Acq On : 02 Jul 2022 13:59
Operator : AJ\MA
Sample : N3564-24 10X
Misc :
ALS Vial : 62 Sample Multiplier: 1


Instrument :
FID_F
ClientSampleId :
WC-16-2-5-GR


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/05/2022
Supervised By :Ankita Jodhani 07/05/2022

Integration File: autoint1.e
Quant Time: Jul 03 22:12:00 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF063022.M
Quant Title :
QLast Update : Fri Jul 01 01:40:42 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

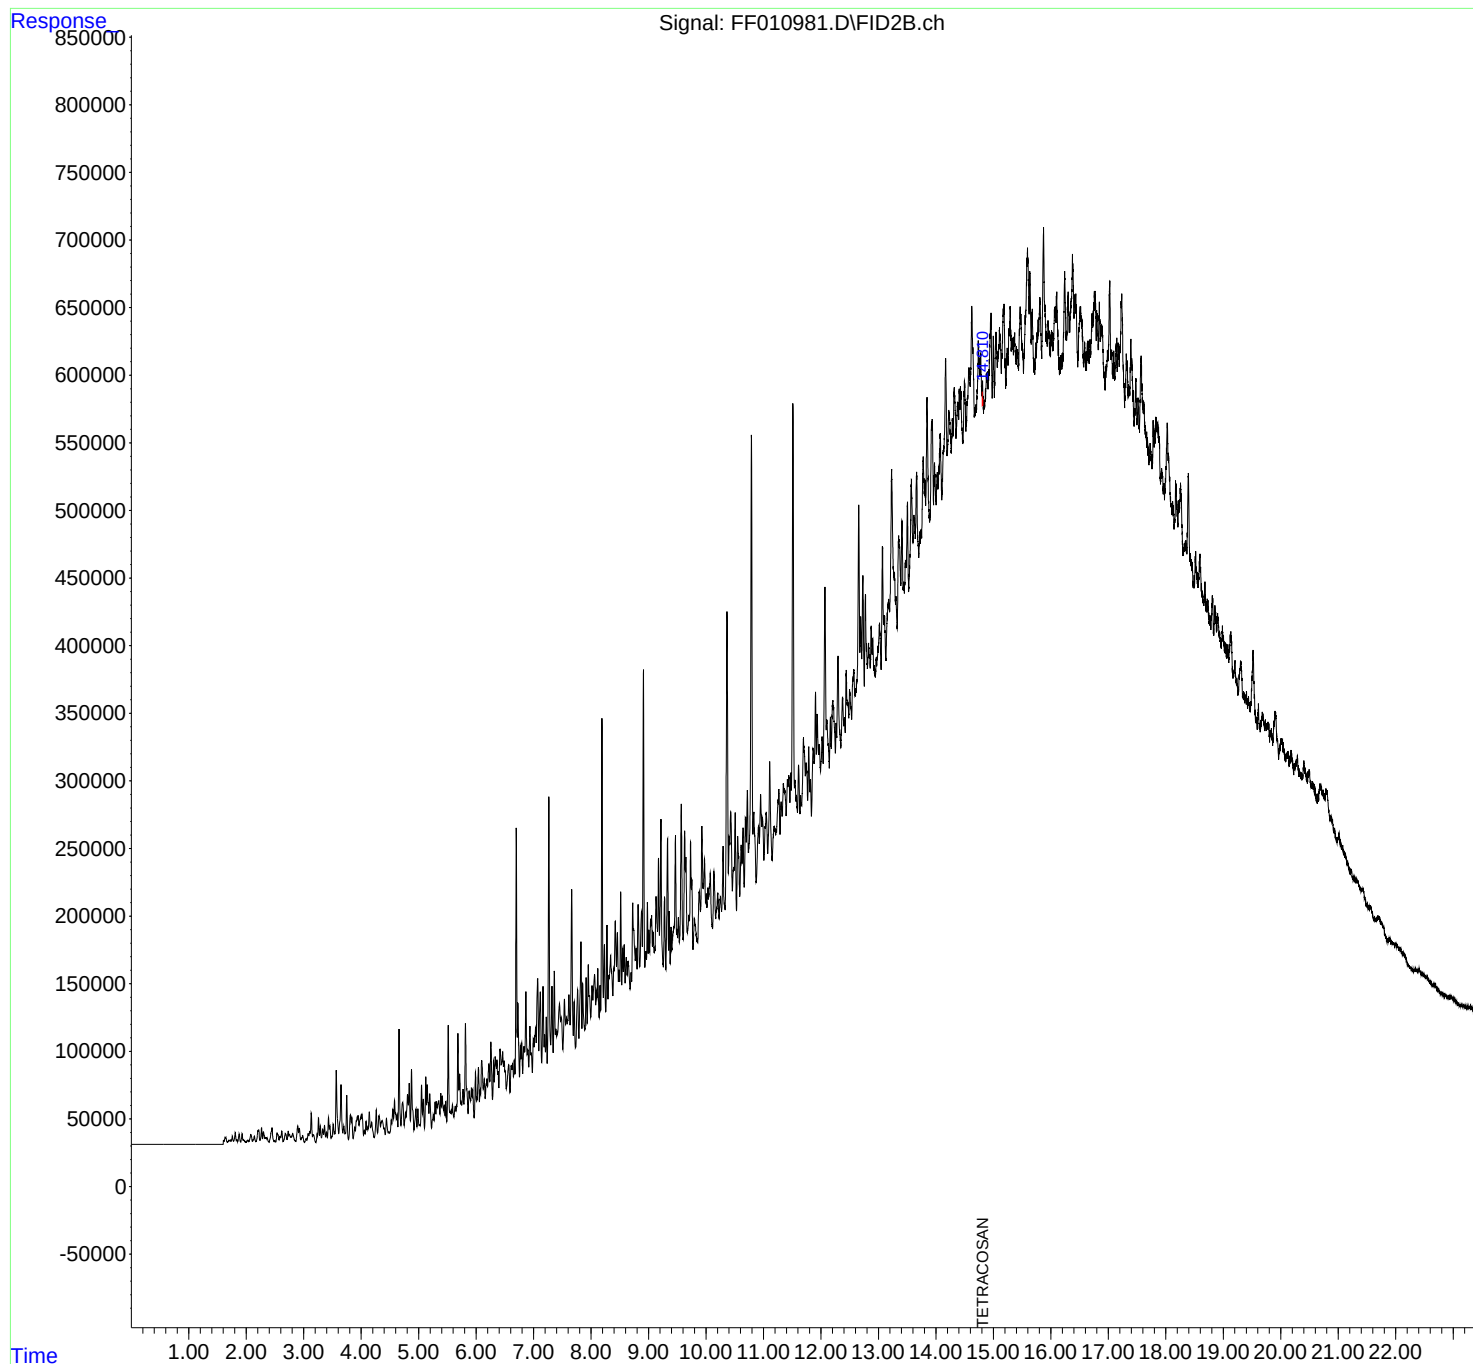

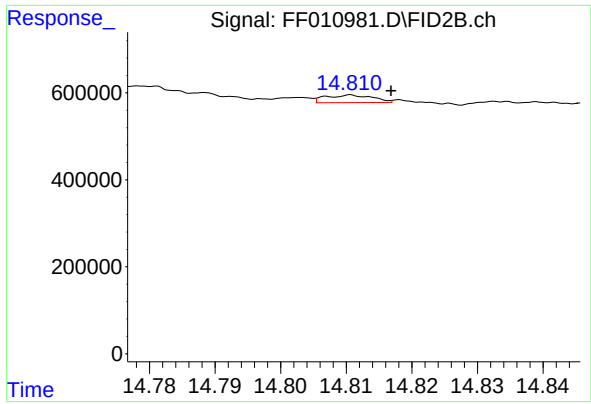

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.810 min
Delta R.T.: -0.006 min
Response: 85892
Conc: 0.92 ug/ml

Instrument :
FID_F
ClientSampleId :
WC-16-2-5-GR

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/05/2022
Supervised By :Ankita Jodhani 07/05/2022