

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF070318\
 Data File : FF001220.D
 Signal(s) : FID2B.ch
 Acq On : 04 Jul 2018 02:51
 Operator : UA\AJ
 Sample : J3826-01
 Misc :
 ALS Vial : 76 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Jul 05 01:23:19 2018
 Quant Method : Z:\PESTPCBSRV\HPCHEM1\FID_F\Method\FF070218.M
 Quant Title :
 QLast Update : Mon Jul 02 13:42:46 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.461	1853294	17.204 ug/ml
Target Compounds			
4) N-TETRADECANE	8.083f	956811	7.608 ug/ml
7) N-EICOSANE	12.411	870624	6.999 ug/ml
8) N-DOCOSANE	13.570	418759	3.396 ug/ml
10) N-TETRACOSANE	14.664	195681	1.605 ug/ml
11) N-HEXACOSANE	15.685	365646	3.017 ug/ml
12) N-OCTACOSANE	16.631	719391	5.971 ug/ml
13) N-TRIACONTANE	17.518	620955	5.166 ug/ml
14) N-DOTRIACONTANE	18.350	527487	4.474 ug/ml
15) N-TETRATRIACONTANE	19.142	704710	5.996 ug/ml
16) N-HEXATRIACONTANE	19.876	858848	7.561 ug/ml
17) N-OCTATRIACONTANE	20.597	443916	4.299 ug/ml
18) N-TETRACONTANE	21.424	296786	2.898 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF070318\
Data File : FF001220.D
Signal(s) : FID2B.ch
Acq On : 04 Jul 2018 02:51
Operator : UA\AJ
Sample : J3826-01
Misc :
ALS Vial : 76 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Jul 05 01:23:19 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\FID_F\Method\FF070218.M
Quant Title :
QLast Update : Mon Jul 02 13:42:46 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

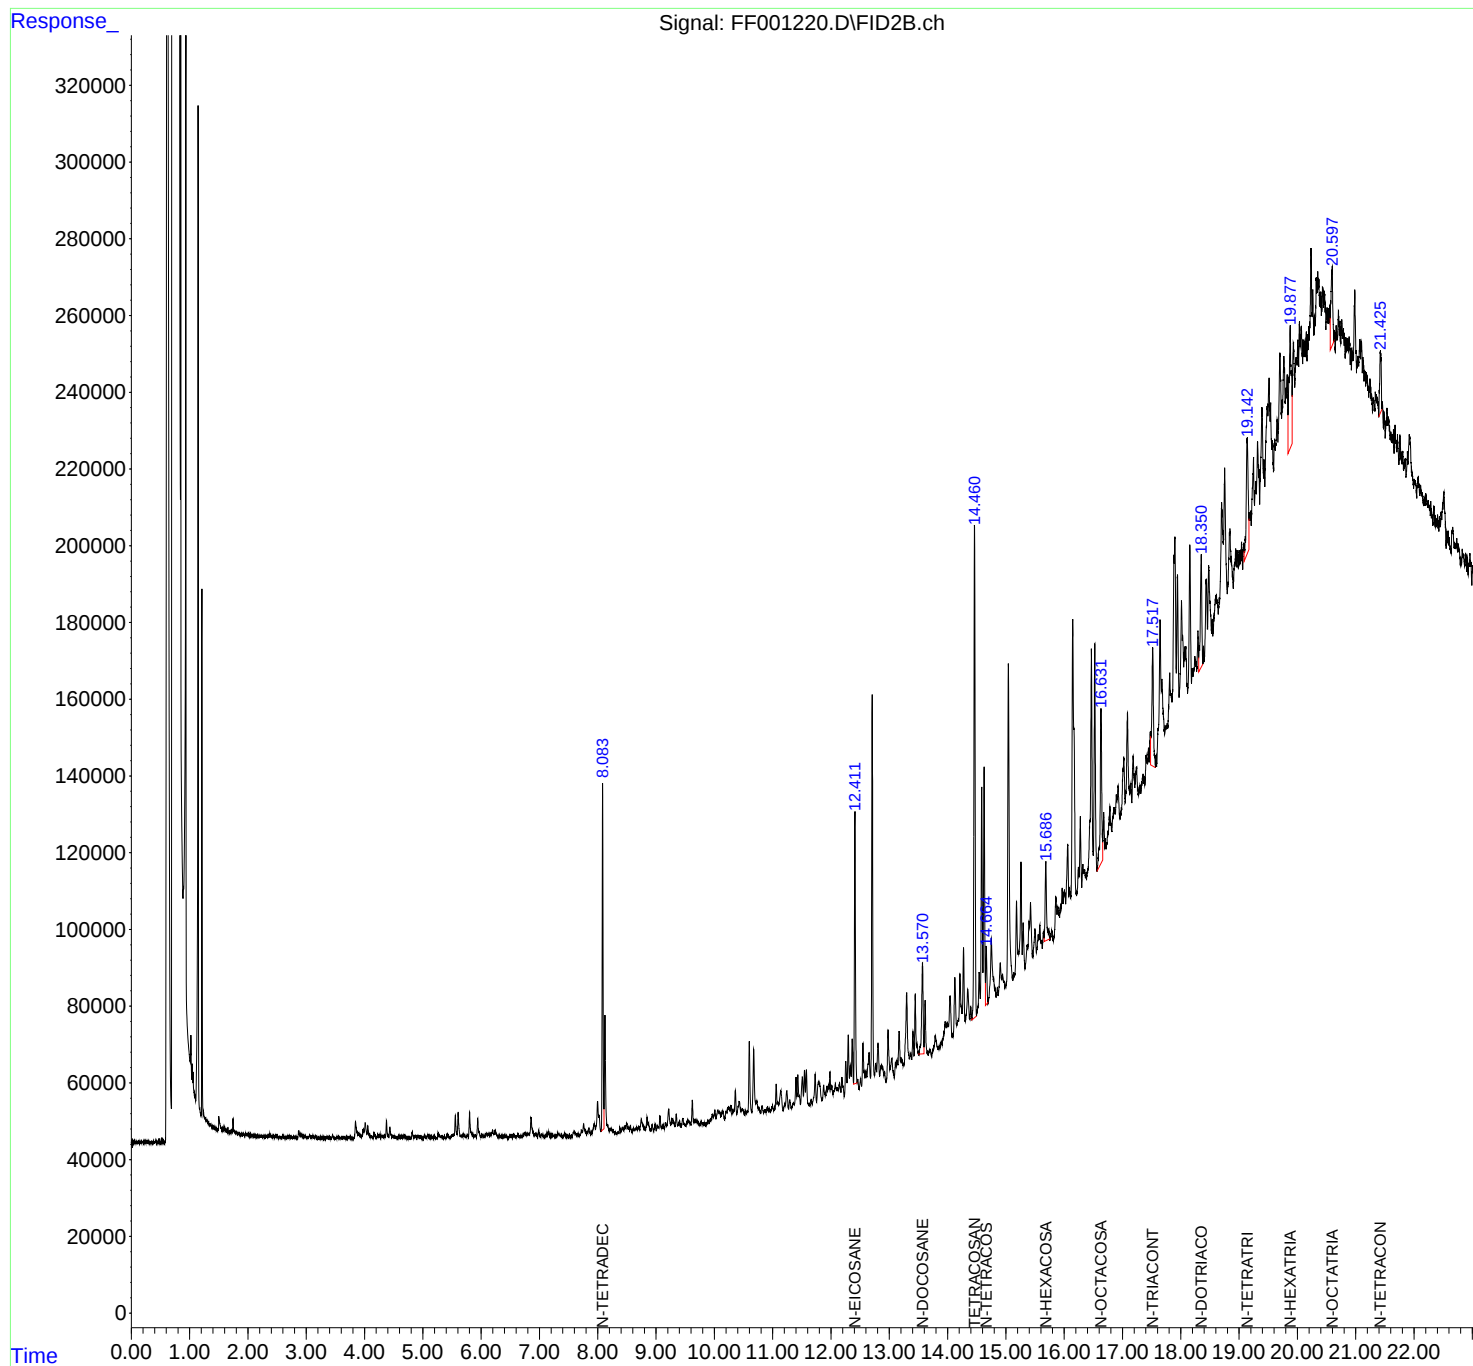

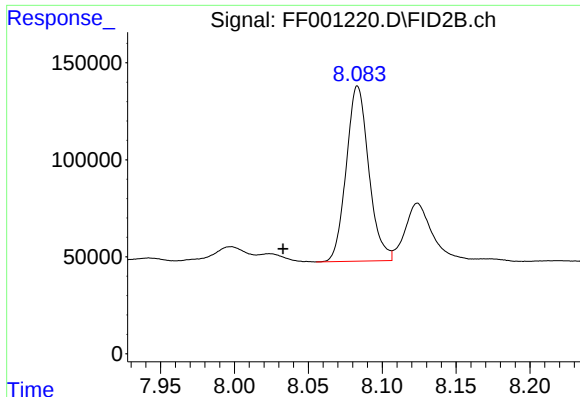


#4 N-TETRADECANE

R.T.: 8.083 min
Delta R.T.: 0.051 min
Response: 956811
Conc: 7.61 ug/ml

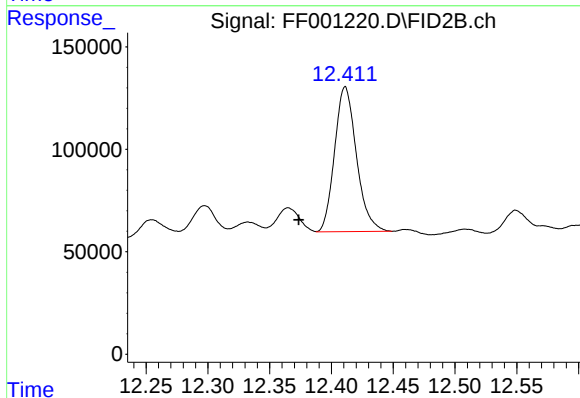


#7 N-EICOSANE

R.T.: 12.411 min
Delta R.T.: 0.038 min
Response: 870624
Conc: 7.00 ug/ml

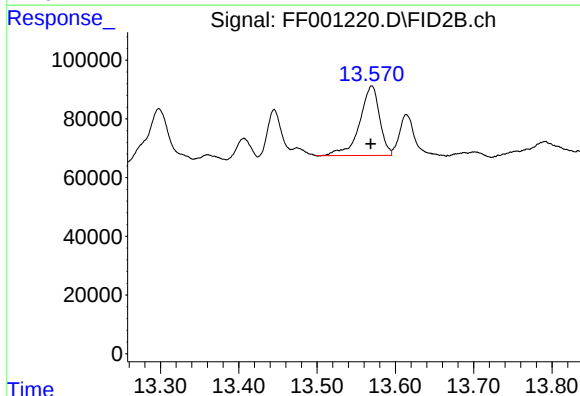


#8 N-DOCOSANE

R.T.: 13.570 min
Delta R.T.: 0.001 min
Response: 418759
Conc: 3.40 ug/ml

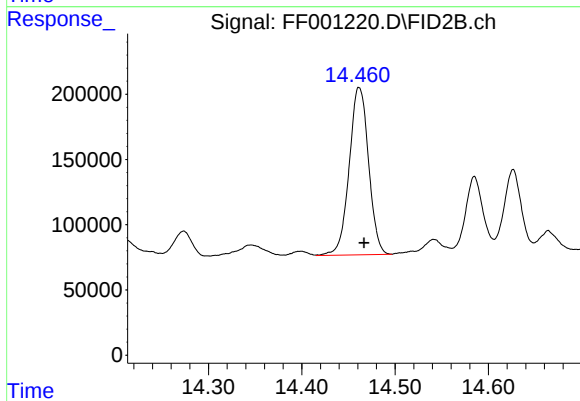


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.461 min
Delta R.T.: -0.005 min
Response: 1853294
Conc: 17.20 ug/ml

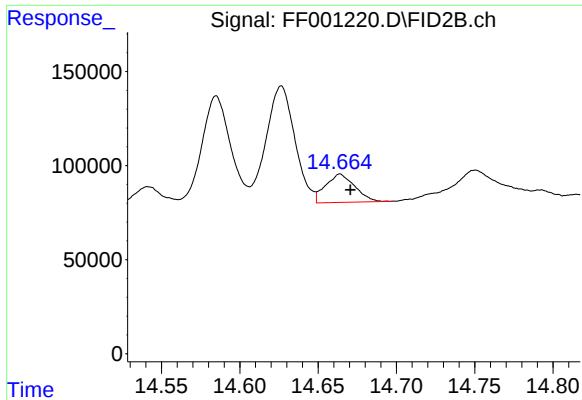


#10 N-TETRACOSANE

R.T.: 14.664 min
Delta R.T.: -0.007 min
Response: 195681
Conc: 1.61 ug/ml

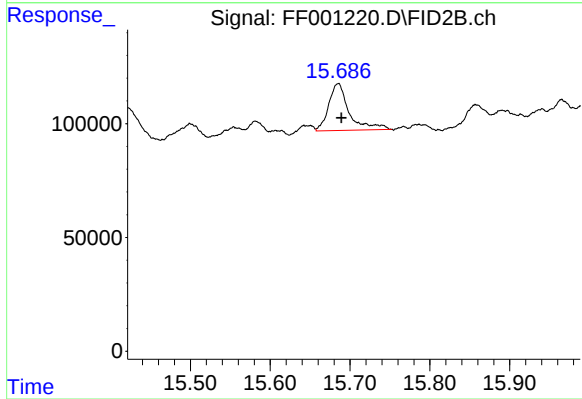


#11 N-HEXACOSANE

R.T.: 15.685 min
Delta R.T.: -0.004 min
Response: 365646
Conc: 3.02 ug/ml

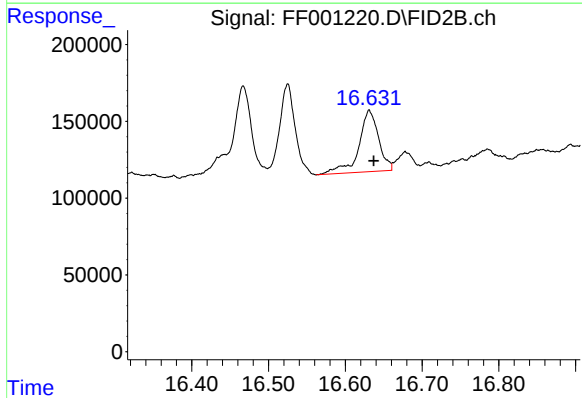


#12 N-OCTACOSANE

R.T.: 16.631 min
Delta R.T.: -0.006 min
Response: 719391
Conc: 5.97 ug/ml

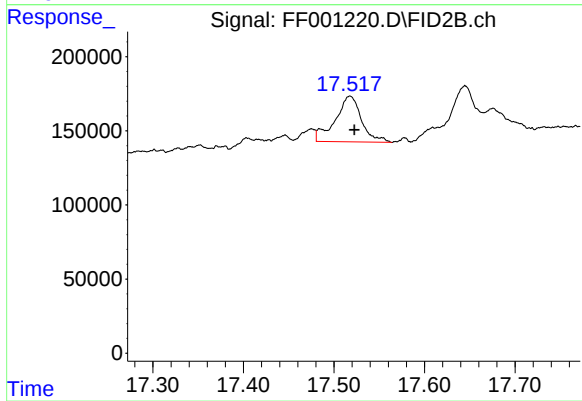


#13 N-TRIACONTANE

R.T.: 17.518 min
Delta R.T.: -0.005 min
Response: 620955
Conc: 5.17 ug/ml

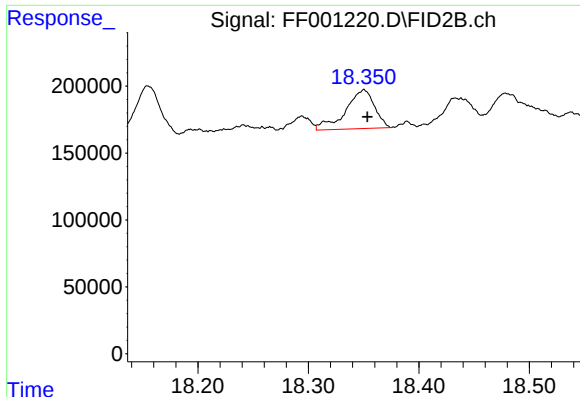


#14 N-DOTRIACONTANE

R.T.: 18.350 min
Delta R.T.: -0.003 min
Response: 527487
Conc: 4.47 ug/ml

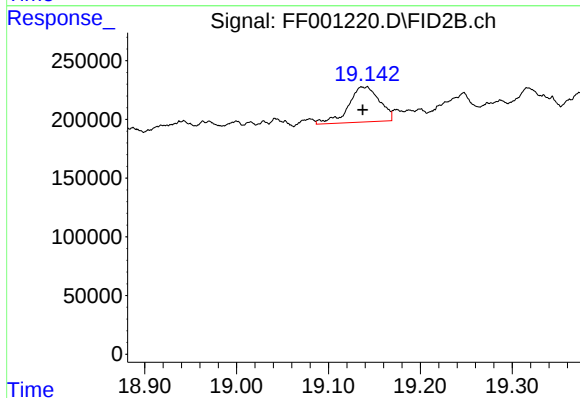


#15 N-TETRATRIACONTANE

R.T.: 19.142 min
Delta R.T.: 0.005 min
Response: 704710
Conc: 6.00 ug/ml

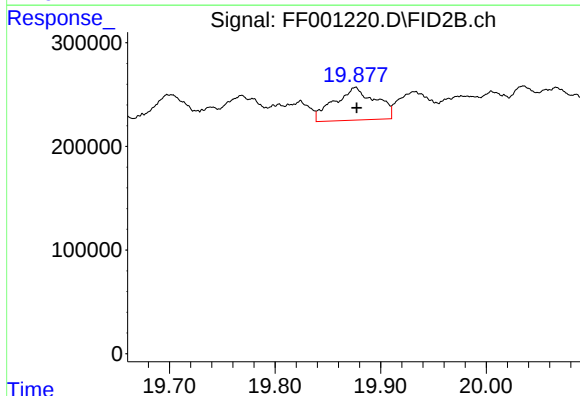


#16 N-HEXATRIACONTANE

R.T.: 19.876 min
Delta R.T.: -0.001 min
Response: 858848
Conc: 7.56 ug/ml

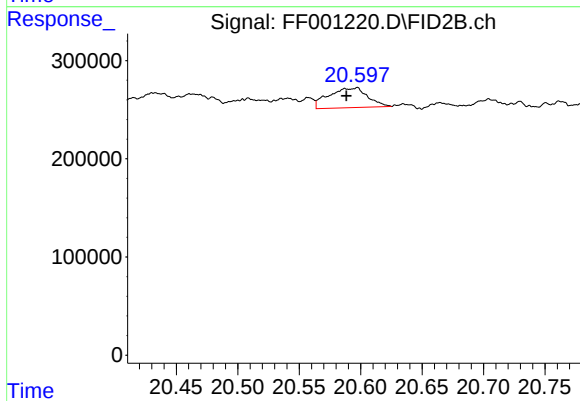

#17 N-OCTATRIACONTANE

R.T.: 20.597 min
Delta R.T.: 0.008 min
Response: 443916
Conc: 4.30 ug/ml

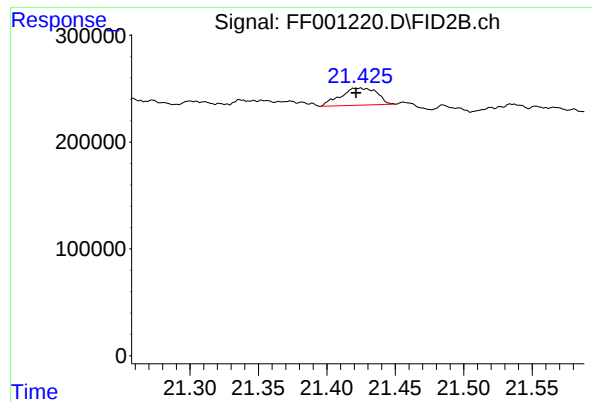

#18 N-TETRACONTANE

R.T.: 21.424 min
Delta R.T.: 0.003 min
Response: 296786
Conc: 2.90 ug/ml