

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF070318\
 Data File : FF001223.D
 Signal(s) : FID2B.ch
 Acq On : 04 Jul 2018 04:22
 Operator : UA\AJ
 Sample : J3245-17 2X
 Misc :
 ALS Vial : 79 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Jul 05 01:24:25 2018
 Quant Method : Z:\PESTPCBSRV\HPCHEM1\FID_F\Method\FF070218.M
 Quant Title :
 QLast Update : Mon Jul 02 13:42:46 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.465	982729	9.123 ug/ml
Target Compounds			
4) N-TETRADECANE	8.086f	331837	2.638 ug/ml
7) N-EICOSANE	12.417	1787734	14.372 ug/ml
8) N-DOCOSANE	13.577	283057	2.295 ug/ml
10) N-TETRACOSANE	14.631	920045	7.547 ug/ml
11) N-HEXACOSANE	15.688	217647	1.796 ug/ml
12) N-OCTACOSANE	16.636	619410	5.142 ug/ml
13) N-TRIACONTANE	17.519	753330	6.267 ug/ml
14) N-DOTRIACONTANE	18.352	351717	2.983 ug/ml
15) N-TETRATRIACONTANE	19.148	271997	2.314 ug/ml
16) N-HEXATRIACONTANE	19.880	112564	0.991 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF070318\
Data File : FF001223.D
Signal(s) : FID2B.ch
Acq On : 04 Jul 2018 04:22
Operator : UA\AJ
Sample : J3245-17 2X
Misc :
ALS Vial : 79 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Jul 05 01:24:25 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\FID_F\Method\FF070218.M
Quant Title :
QLast Update : Mon Jul 02 13:42:46 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

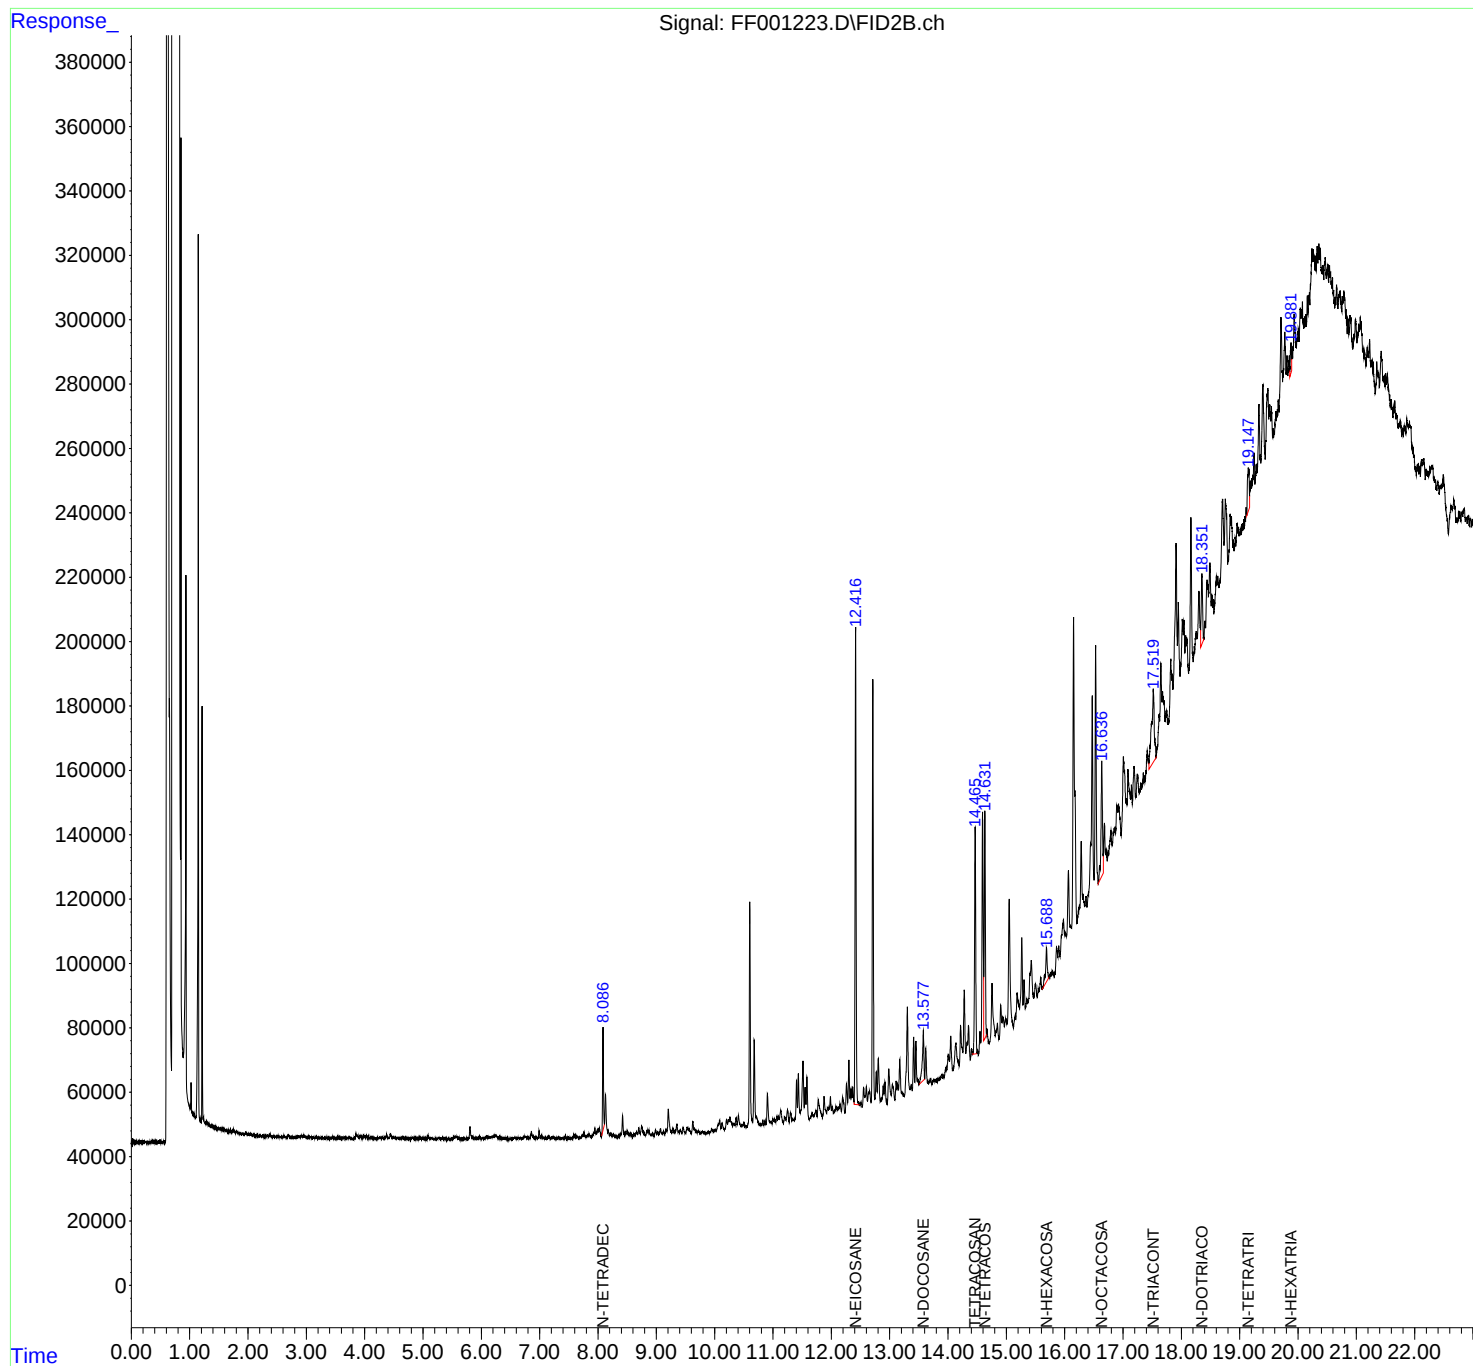

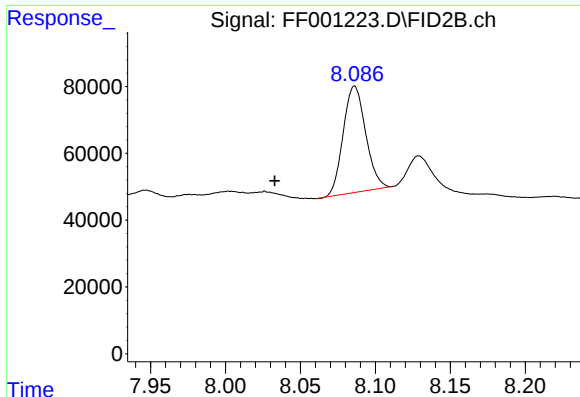


#4 N-TETRADECANE

R.T.: 8.086 min
Delta R.T.: 0.053 min
Response: 331837
Conc: 2.64 ug/ml

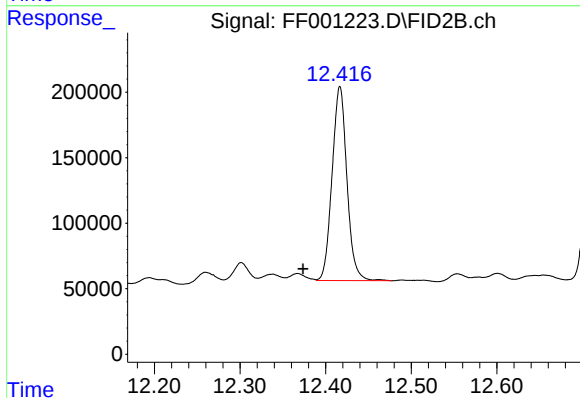


#7 N-EICOSANE

R.T.: 12.417 min
Delta R.T.: 0.043 min
Response: 1787734
Conc: 14.37 ug/ml

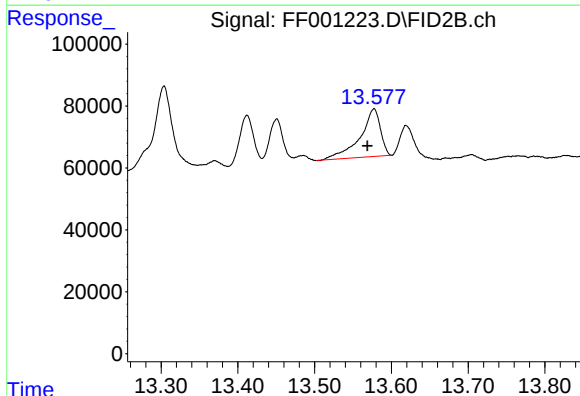


#8 N-DOCOSANE

R.T.: 13.577 min
Delta R.T.: 0.009 min
Response: 283057
Conc: 2.30 ug/ml

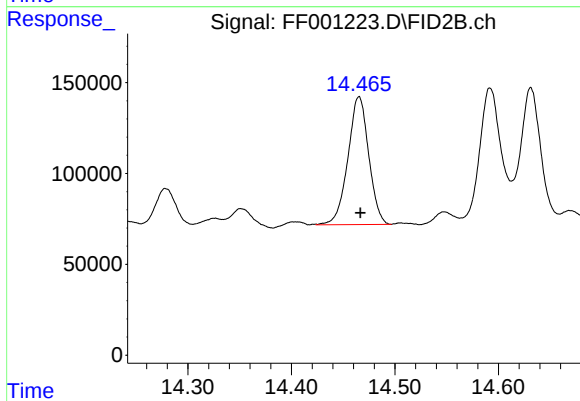


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.465 min
Delta R.T.: -0.001 min
Response: 982729
Conc: 9.12 ug/ml

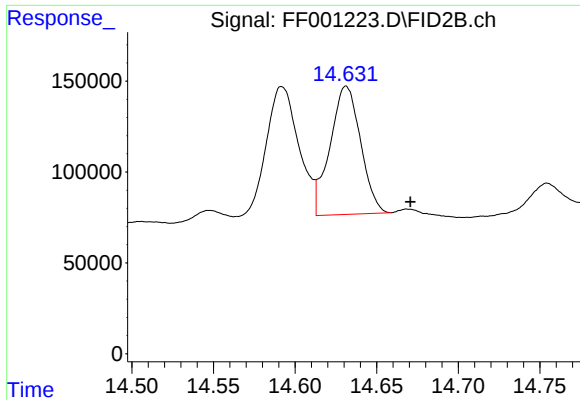


#10 N-TETRACOSANE

R.T.: 14.631 min
Delta R.T.: -0.039 min
Response: 920045
Conc: 7.55 ug/ml

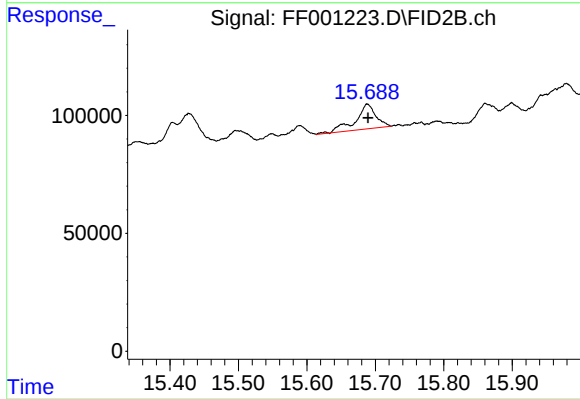


#11 N-HEXACOSANE

R.T.: 15.688 min
Delta R.T.: -0.001 min
Response: 217647
Conc: 1.80 ug/ml

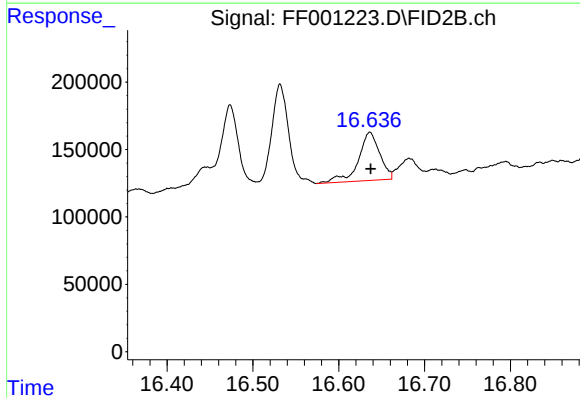


#12 N-OCTACOSANE

R.T.: 16.636 min
Delta R.T.: 0.000 min
Response: 619410
Conc: 5.14 ug/ml

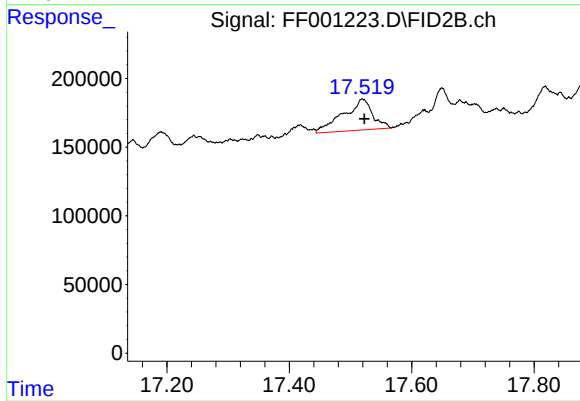


#13 N-TRIACONTANE

R.T.: 17.519 min
Delta R.T.: -0.004 min
Response: 753330
Conc: 6.27 ug/ml

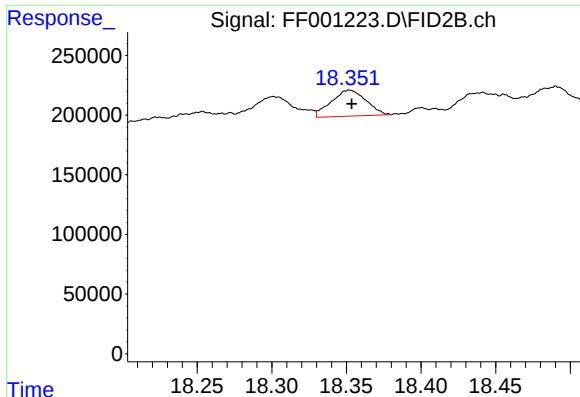


#14 N-DOTRIACONTANE

R.T.: 18.352 min
Delta R.T.: -0.001 min
Response: 351717
Conc: 2.98 ug/ml

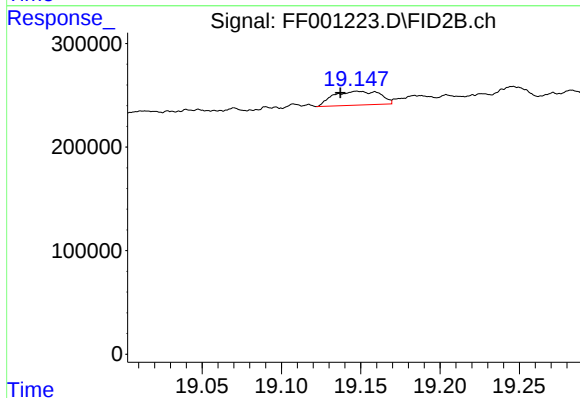

#15 N-TETRATRIACONTANE

R.T.: 19.148 min
Delta R.T.: 0.010 min
Response: 271997
Conc: 2.31 ug/ml

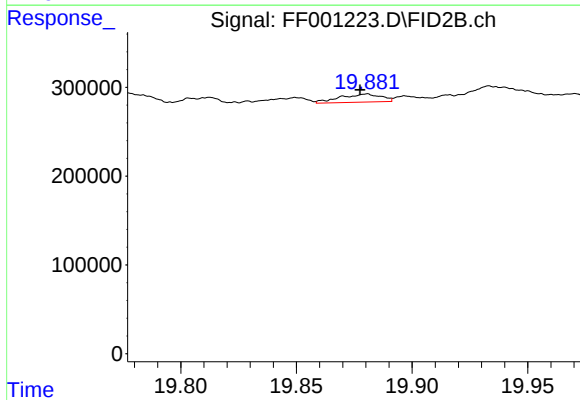

#16 N-HEXATRIACONTANE

R.T.: 19.880 min
Delta R.T.: 0.003 min
Response: 112564
Conc: 0.99 ug/ml