

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF070519\
 Data File : FF004984.D
 Signal(s) : FID2B.ch
 Acq On : 05 Jul 2019 18:11
 Operator : DD\AJ
 Sample : K3624-07 2X
 Misc :
 ALS Vial : 66 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Jul 05 22:38:55 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF062619.M
 Quant Title :
 QLast Update : Wed Jun 26 14:27:24 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.686	1087598	11.183 ug/ml
Target Compounds			
4) N-TETRADECANE	8.275f	446556	3.569 ug/ml
7) N-EICOSANE	12.639f	602757	5.195 ug/ml
10) N-TETRACOSANE	14.868	497125	4.466 ug/ml
11) N-HEXACOSANE	15.920	151357	1.368 ug/ml
12) N-OCTACOSANE	16.875	577040	5.173 ug/ml
13) N-TRIACONTANE	17.767	869806	7.743 ug/ml
14) N-DOTRIACONTANE	18.605	352281	3.093 ug/ml
15) N-TETRATRIACONTANE	19.396	108220	0.997 ug/ml
16) N-HEXATRIACONTANE	20.148	498855	4.817 ug/ml
17) N-OCTATRIACONTANE	20.831f	667789	7.002 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF070519\
Data File : FF004984.D
Signal(s) : FID2B.ch
Acq On : 05 Jul 2019 18:11
Operator : DD\AJ
Sample : K3624-07 2X
Misc :
ALS Vial : 66 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Jul 05 22:38:55 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF062619.M
Quant Title :
QLast Update : Wed Jun 26 14:27:24 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

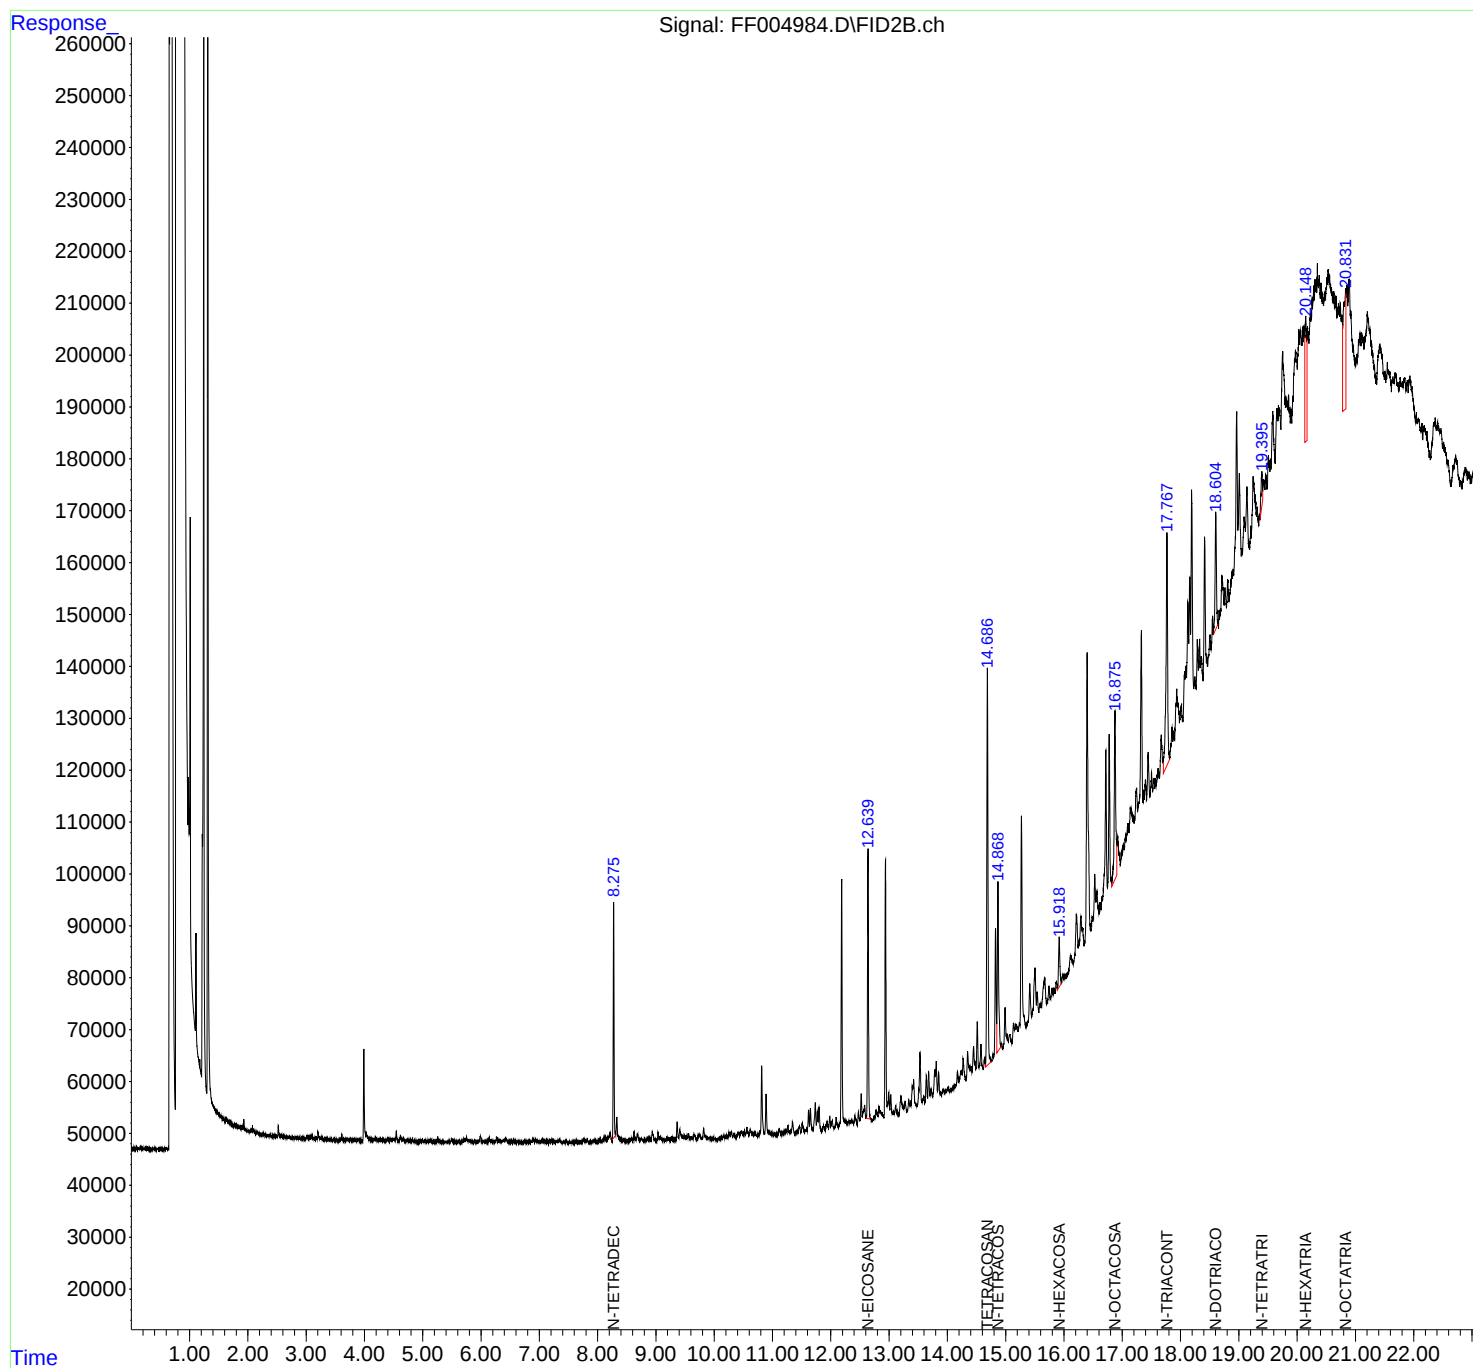

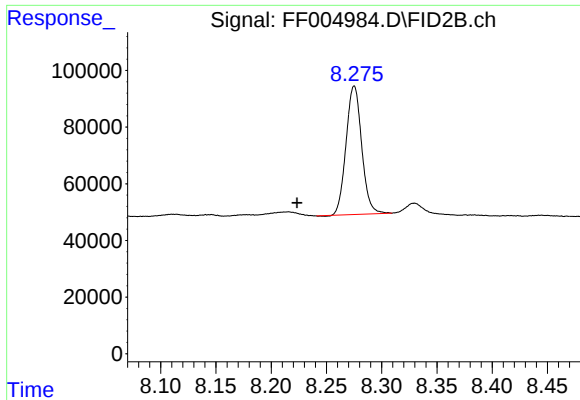


#4 N-TETRADECANE

R.T.: 8.275 min
Delta R.T.: 0.052 min
Response: 446556
Conc: 3.57 ug/ml

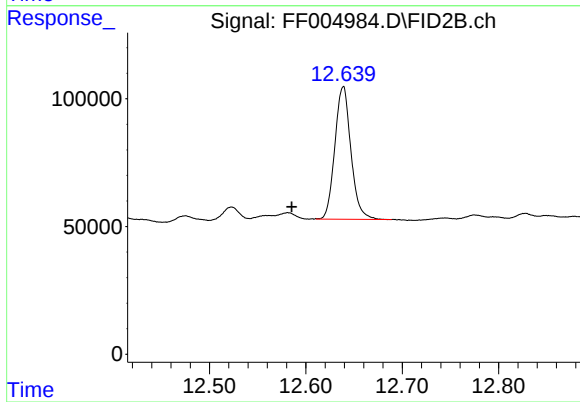


#7 N-EICOSANE

R.T.: 12.639 min
Delta R.T.: 0.053 min
Response: 602757
Conc: 5.20 ug/ml

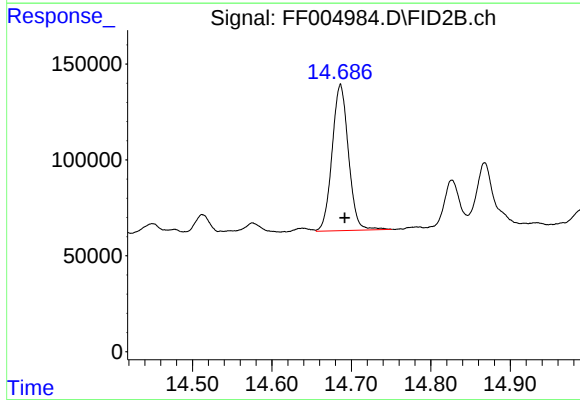


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.686 min
Delta R.T.: -0.005 min
Response: 1087598
Conc: 11.18 ug/ml

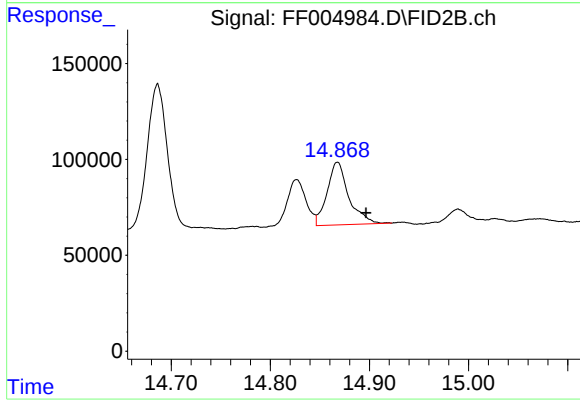


#10 N-TETRACOSANE

R.T.: 14.868 min
Delta R.T.: -0.029 min
Response: 497125
Conc: 4.47 ug/ml

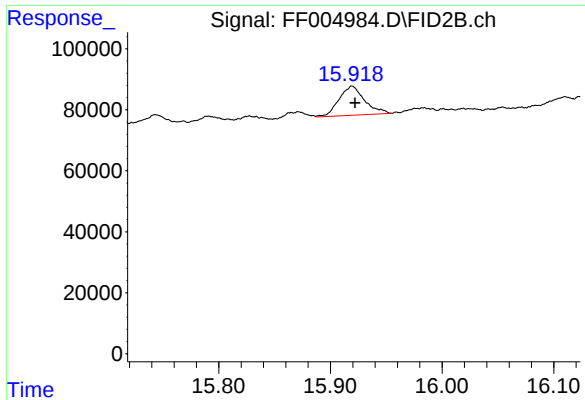


#11 N-HEXACOSANE

R.T.: 15.920 min
Delta R.T.: -0.003 min
Response: 151357
Conc: 1.37 ug/ml

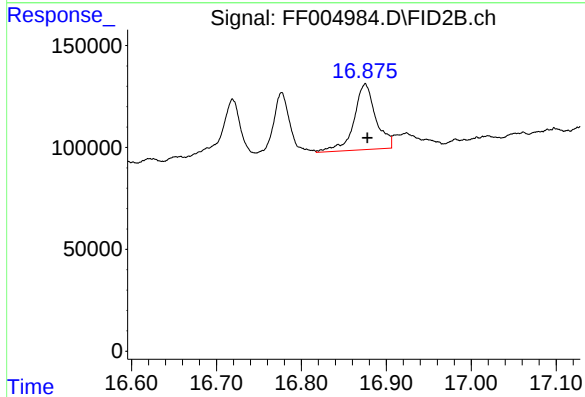


#12 N-OCTACOSANE

R.T.: 16.875 min
Delta R.T.: -0.003 min
Response: 577040
Conc: 5.17 ug/ml

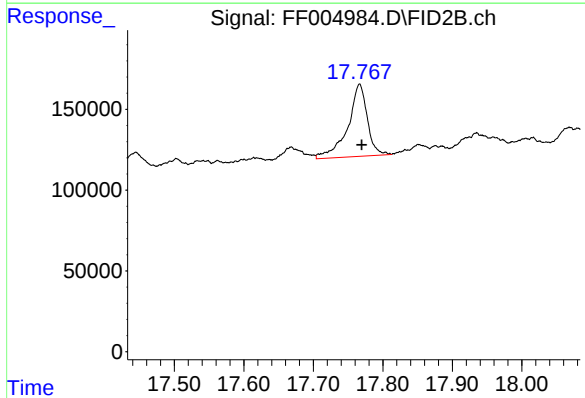


#13 N-TRIACONTANE

R.T.: 17.767 min
Delta R.T.: -0.003 min
Response: 869806
Conc: 7.74 ug/ml

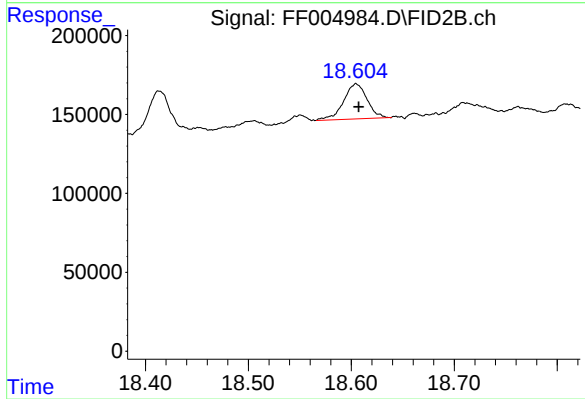

#14 N-DOTRIACONTANE

R.T.: 18.605 min
Delta R.T.: -0.003 min
Response: 352281
Conc: 3.09 ug/ml

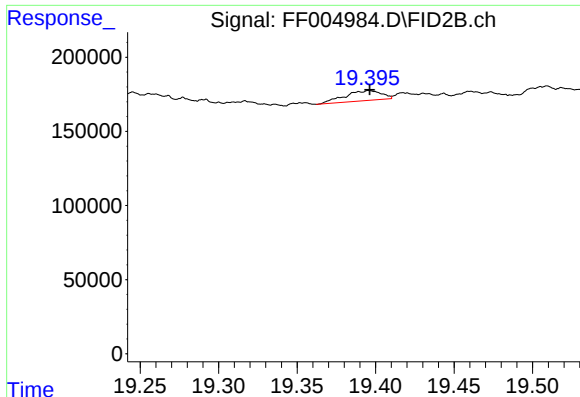


#15 N-TETRATRIACONTANE

R.T.: 19.396 min

Delta R.T.: 0.000 min

Response: 108220

Conc: 1.00 ug/ml

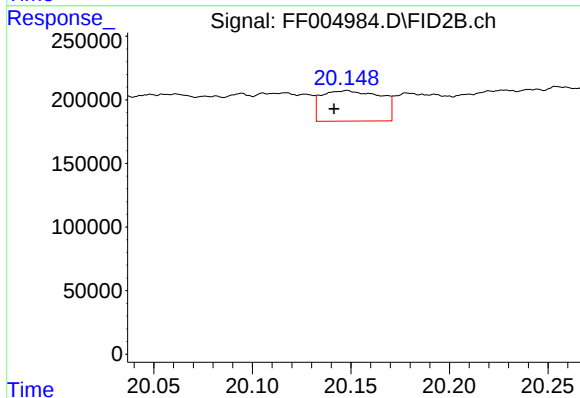


#16 N-HEXATRIACONTANE

R.T.: 20.148 min

Delta R.T.: 0.006 min

Response: 498855

Conc: 4.82 ug/ml

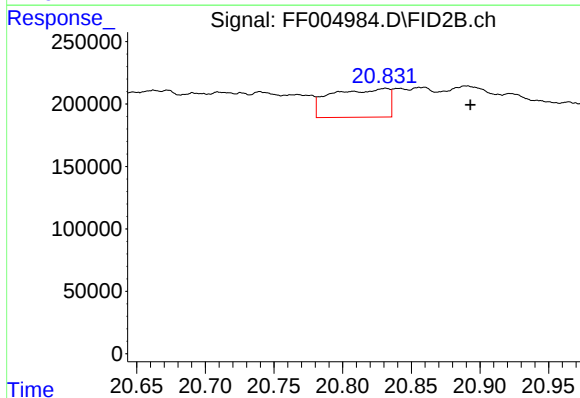

#17 N-OCTATRIACONTANE

R.T.: 20.831 min

Delta R.T.: -0.062 min

Response: 667789

Conc: 7.00 ug/ml