

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF070519\
 Data File : FF004985.D
 Signal(s) : FID2B.ch
 Acq On : 05 Jul 2019 18:41
 Operator : DD\AJ
 Sample : K3624-01
 Misc :
 ALS Vial : 67 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Jul 05 22:39:11 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF062619.M
 Quant Title :
 QLast Update : Wed Jun 26 14:27:24 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.688	1561018	16.050 ug/ml
Target Compounds			
4) N-TETRADECANE	8.276f	558597	4.464 ug/ml
7) N-EICOSANE	12.641f	1629593	14.045 ug/ml
8) N-DOCOSANE	13.786	139413	1.239 ug/ml
10) N-TETRACOSANE	14.869	1222956	10.986 ug/ml
11) N-HEXACOSANE	15.920	232375	2.101 ug/ml
12) N-OCTACOSANE	16.879	855778	7.672 ug/ml
13) N-TRIACONTANE	17.768	956420	8.514 ug/ml
14) N-DOTRIACONTANE	18.604	331157	2.908 ug/ml
15) N-TETRATRIACONTANE	19.396	57011	0.525 ug/ml
16) N-HEXATRIACONTANE	20.139	41583	0.402 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF070519\
Data File : FF004985.D
Signal(s) : FID2B.ch
Acq On : 05 Jul 2019 18:41
Operator : DD\AJ
Sample : K3624-01
Misc :
ALS Vial : 67 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Jul 05 22:39:11 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF062619.M
Quant Title :
QLast Update : Wed Jun 26 14:27:24 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

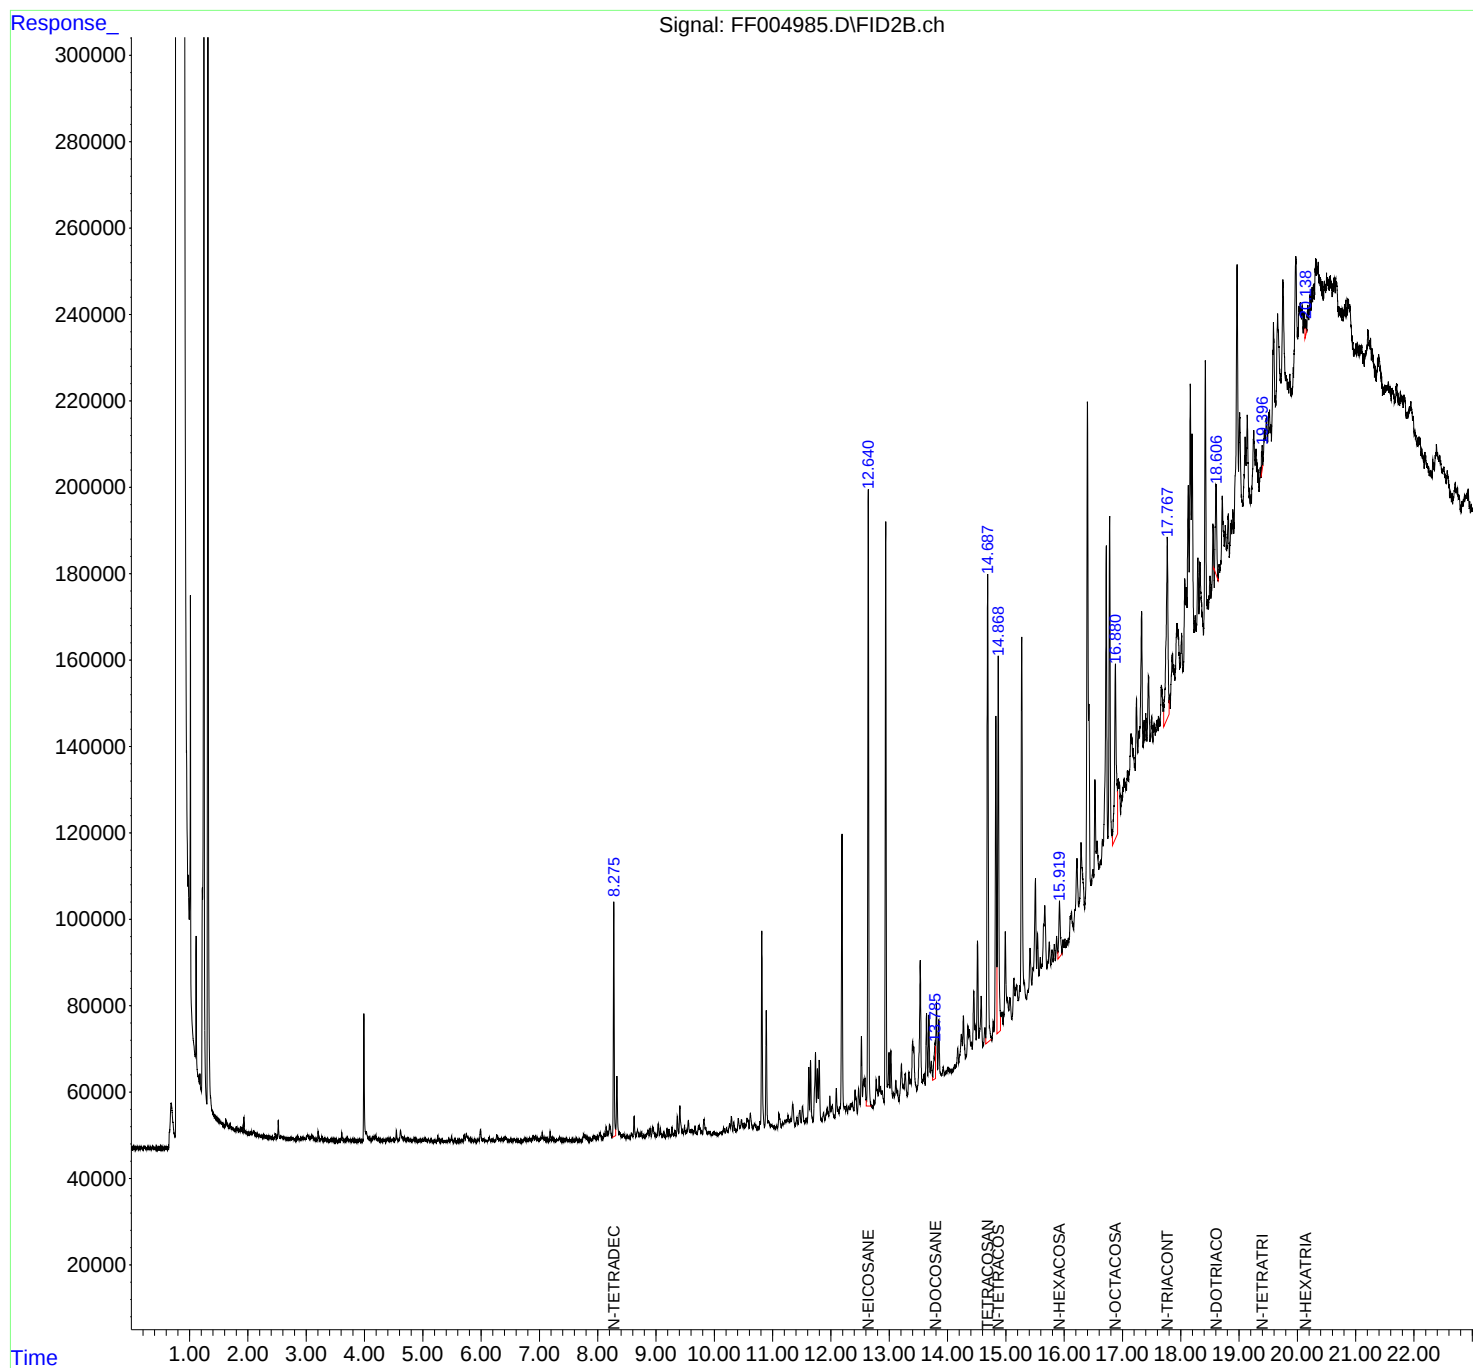

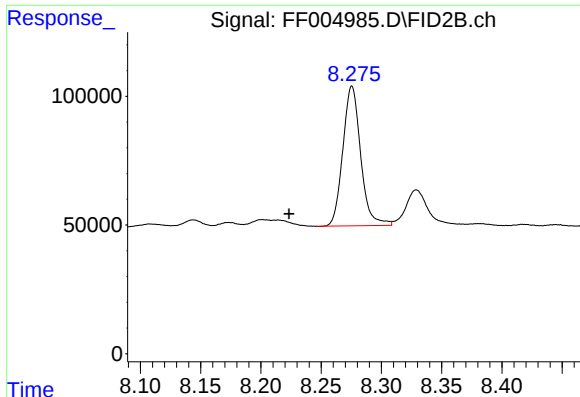


#4 N-TETRADECANE

R.T.: 8.276 min
Delta R.T.: 0.052 min
Response: 558597
Conc: 4.46 ug/ml

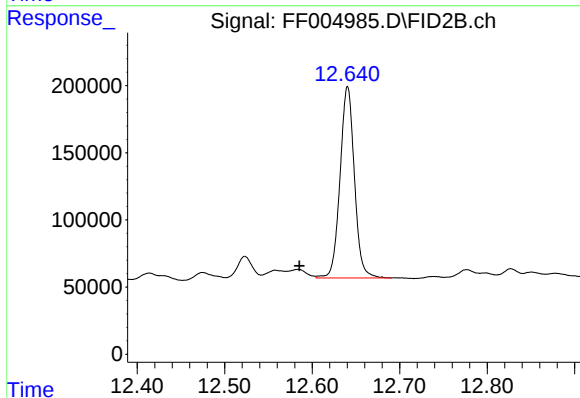


#7 N-EICOSANE

R.T.: 12.641 min
Delta R.T.: 0.055 min
Response: 1629593
Conc: 14.05 ug/ml

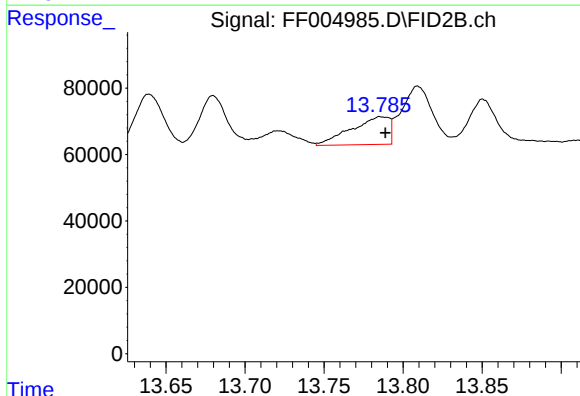


#8 N-DOCOSANE

R.T.: 13.786 min
Delta R.T.: -0.003 min
Response: 139413
Conc: 1.24 ug/ml

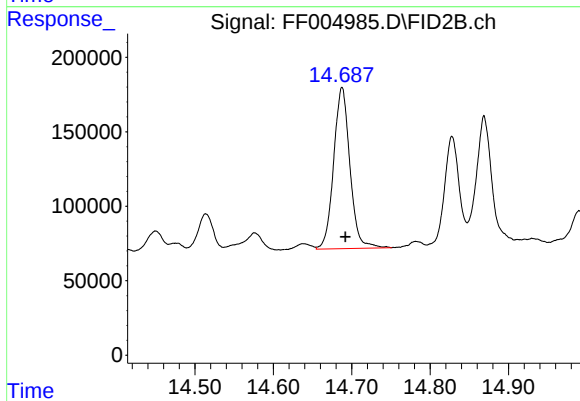


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.688 min
Delta R.T.: -0.004 min
Response: 1561018
Conc: 16.05 ug/ml

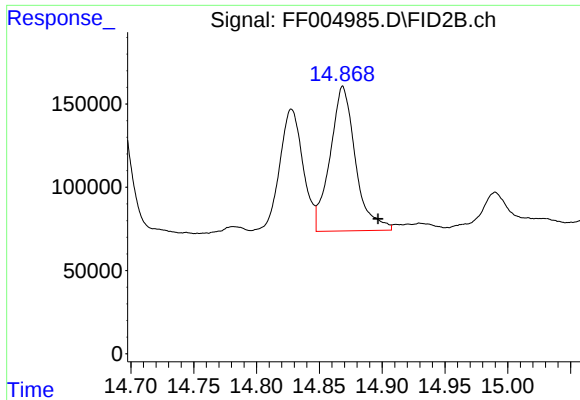


#10 N-TETRACOSANE

R.T.: 14.869 min
Delta R.T.: -0.028 min
Response: 1222956
Conc: 10.99 ug/ml

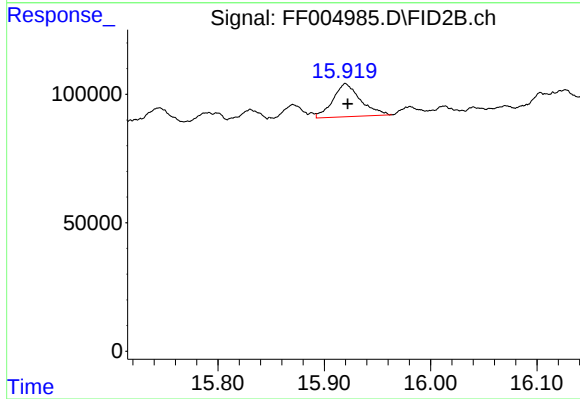


#11 N-HEXACOSANE

R.T.: 15.920 min
Delta R.T.: -0.002 min
Response: 232375
Conc: 2.10 ug/ml

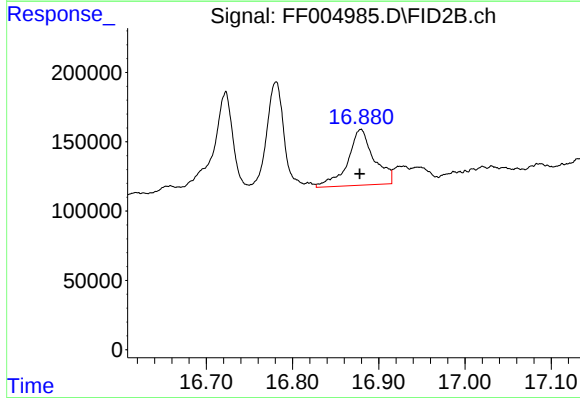


#12 N-OCTACOSANE

R.T.: 16.879 min
Delta R.T.: 0.001 min
Response: 855778
Conc: 7.67 ug/ml

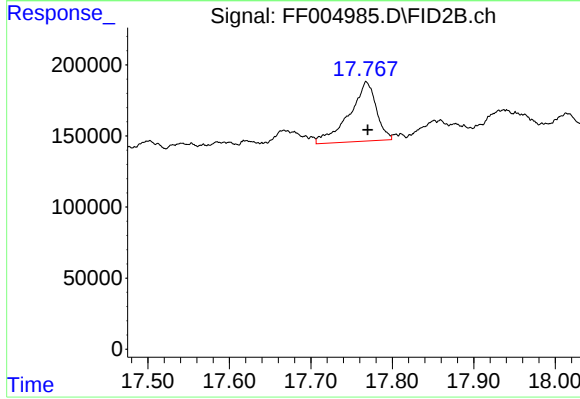


#13 N-TRIACONTANE

R.T.: 17.768 min
Delta R.T.: -0.002 min
Response: 956420
Conc: 8.51 ug/ml

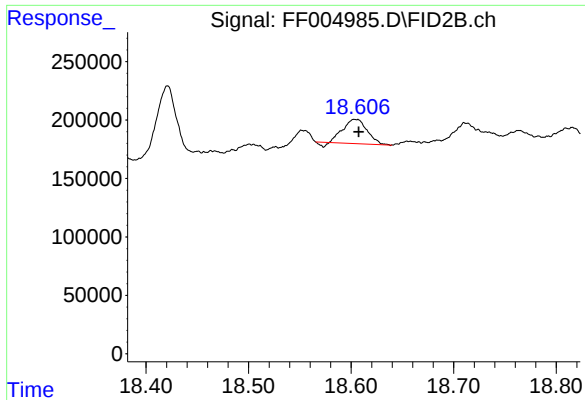


#14 N-DOTRIACONTANE

R.T.: 18.604 min
Delta R.T.: -0.003 min
Response: 331157
Conc: 2.91 ug/ml

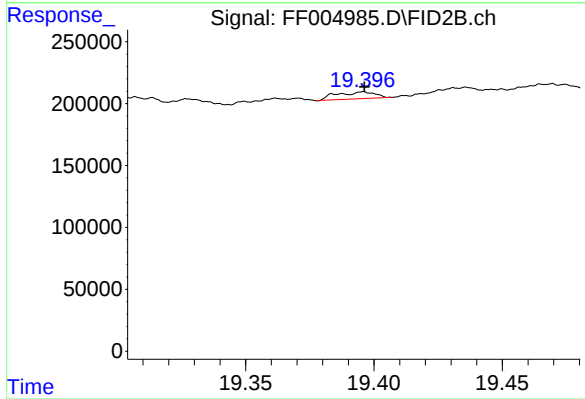

#15 N-TETRATRIACONTANE

R.T.: 19.396 min
Delta R.T.: 0.000 min
Response: 57011
Conc: 0.53 ug/ml

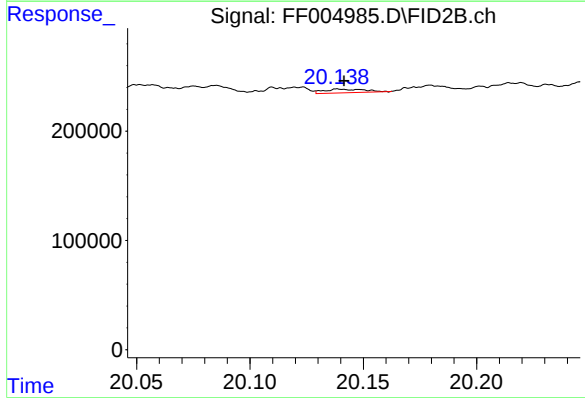

#16 N-HEXATRIACONTANE

R.T.: 20.139 min
Delta R.T.: -0.002 min
Response: 41583
Conc: 0.40 ug/ml