

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF070621\
Data File : FF008730.D
Signal(s) : FID2B.ch
Acq On : 06 Jul 2021 10:05
Operator : DD\AJ
Sample : MECL2
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jul 06 22:41:31 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF062321.M
Quant Title :
QLast Update : Thu Jun 24 08:07:11 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
Target Compounds				
14)	N-DOTRIACONTANE	18.638	751162	6.412 ug/ml
16)	N-HEXATRIACONTANE	20.184	306172	3.260 ug/ml
18)	N-TETRACONTANE	21.858	451203	4.875 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF070621\
Data File : FF008730.D
Signal(s) : FID2B.ch
Acq On : 06 Jul 2021 10:05
Operator : DD\AJ
Sample : MECL2
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jul 06 22:41:31 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF062321.M
Quant Title :
QLast Update : Thu Jun 24 08:07:11 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

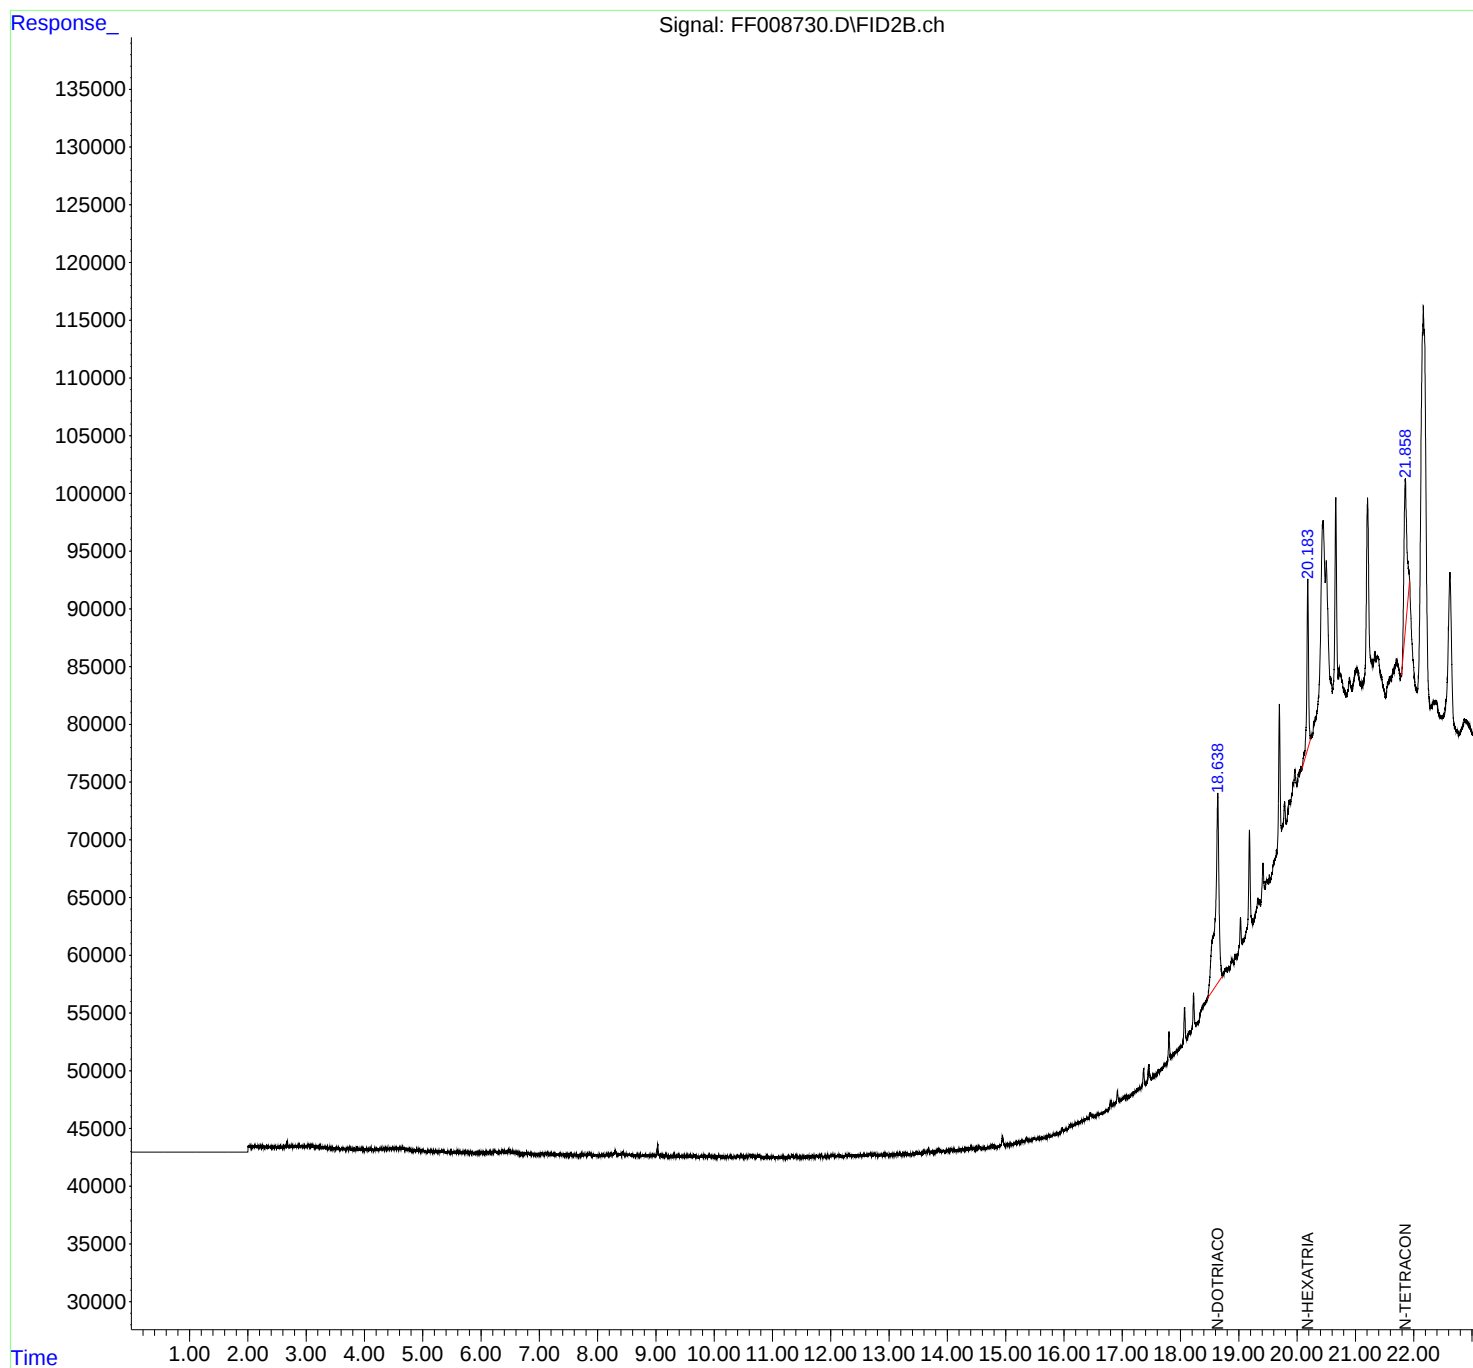


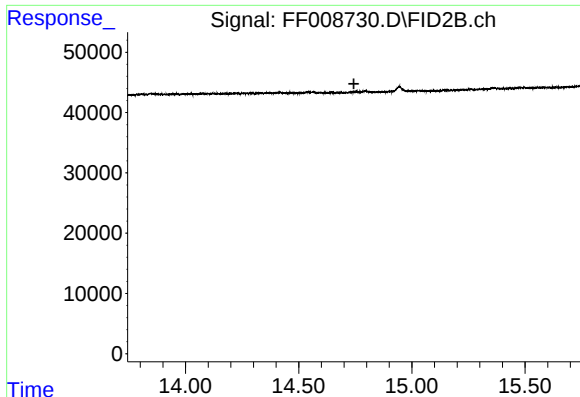

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 0.000 min
Exp R.T.: 14.744 min
Response: 0
Conc: N.D.

Instrument :
FID_F
ClientSampleId :

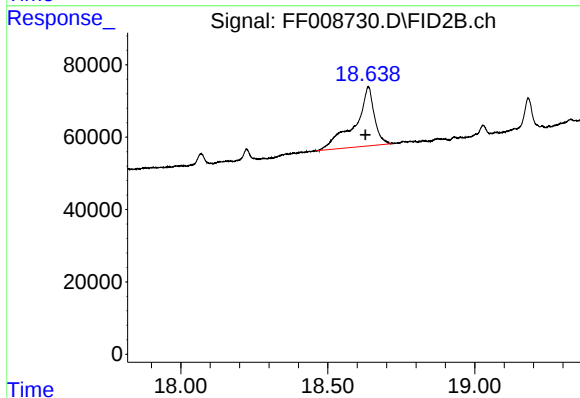


#14 N-DOTRIACONTANE

R.T.: 18.638 min
Delta R.T.: 0.009 min
Response: 751162
Conc: 6.41 ug/ml

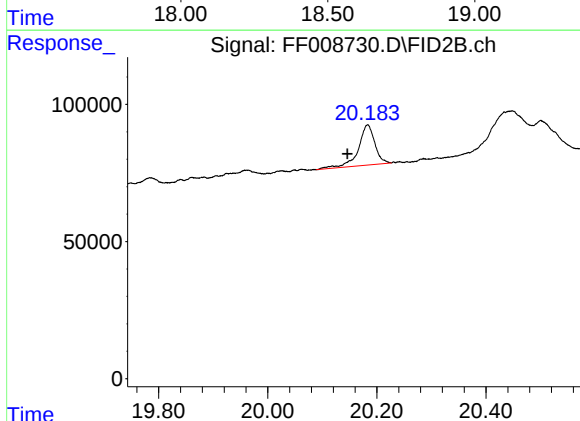

#16 N-HEXATRIACONTANE

R.T.: 20.184 min
Delta R.T.: 0.038 min
Response: 306172
Conc: 3.26 ug/ml

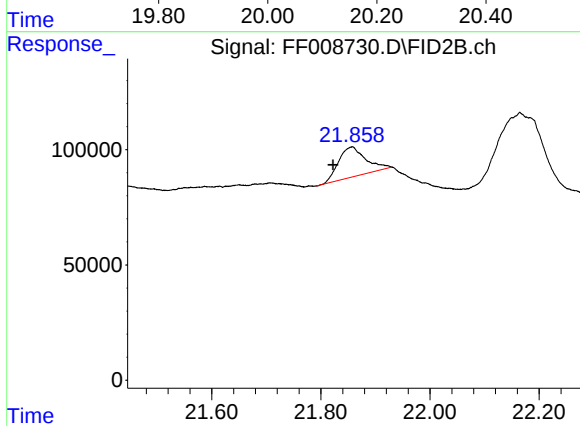

#18 N-TETRACONTANE

R.T.: 21.858 min
Delta R.T.: 0.036 min
Response: 451203
Conc: 4.88 ug/ml