

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF070621\
Data File : FF008733.D
Signal(s) : FID2B.ch
Acq On : 06 Jul 2021 13:33
Operator : DD\AJ
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jul 06 22:41:58 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF062321.M
Quant Title :
QLast Update : Thu Jun 24 08:07:11 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds

3)	N-DODECANE	6.520	2768464	20.356 ug/ml
12)	N-OCTACOSANE	16.919	2372544	19.182 ug/ml
13)	N-TRIACONTANE	17.803	174848	1.459 ug/ml
14)	N-DOTRIACONTANE	18.633	280776	2.397 ug/ml
15)	N-TETRATRIACONTANE	19.414	174870	1.673 ug/ml
16)	N-HEXATRIACONTANE	20.151	92924	0.989 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF070621\
Data File : FF008733.D
Signal(s) : FID2B.ch
Acq On : 06 Jul 2021 13:33
Operator : DD\AJ
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jul 06 22:41:58 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF062321.M
Quant Title :
QLast Update : Thu Jun 24 08:07:11 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

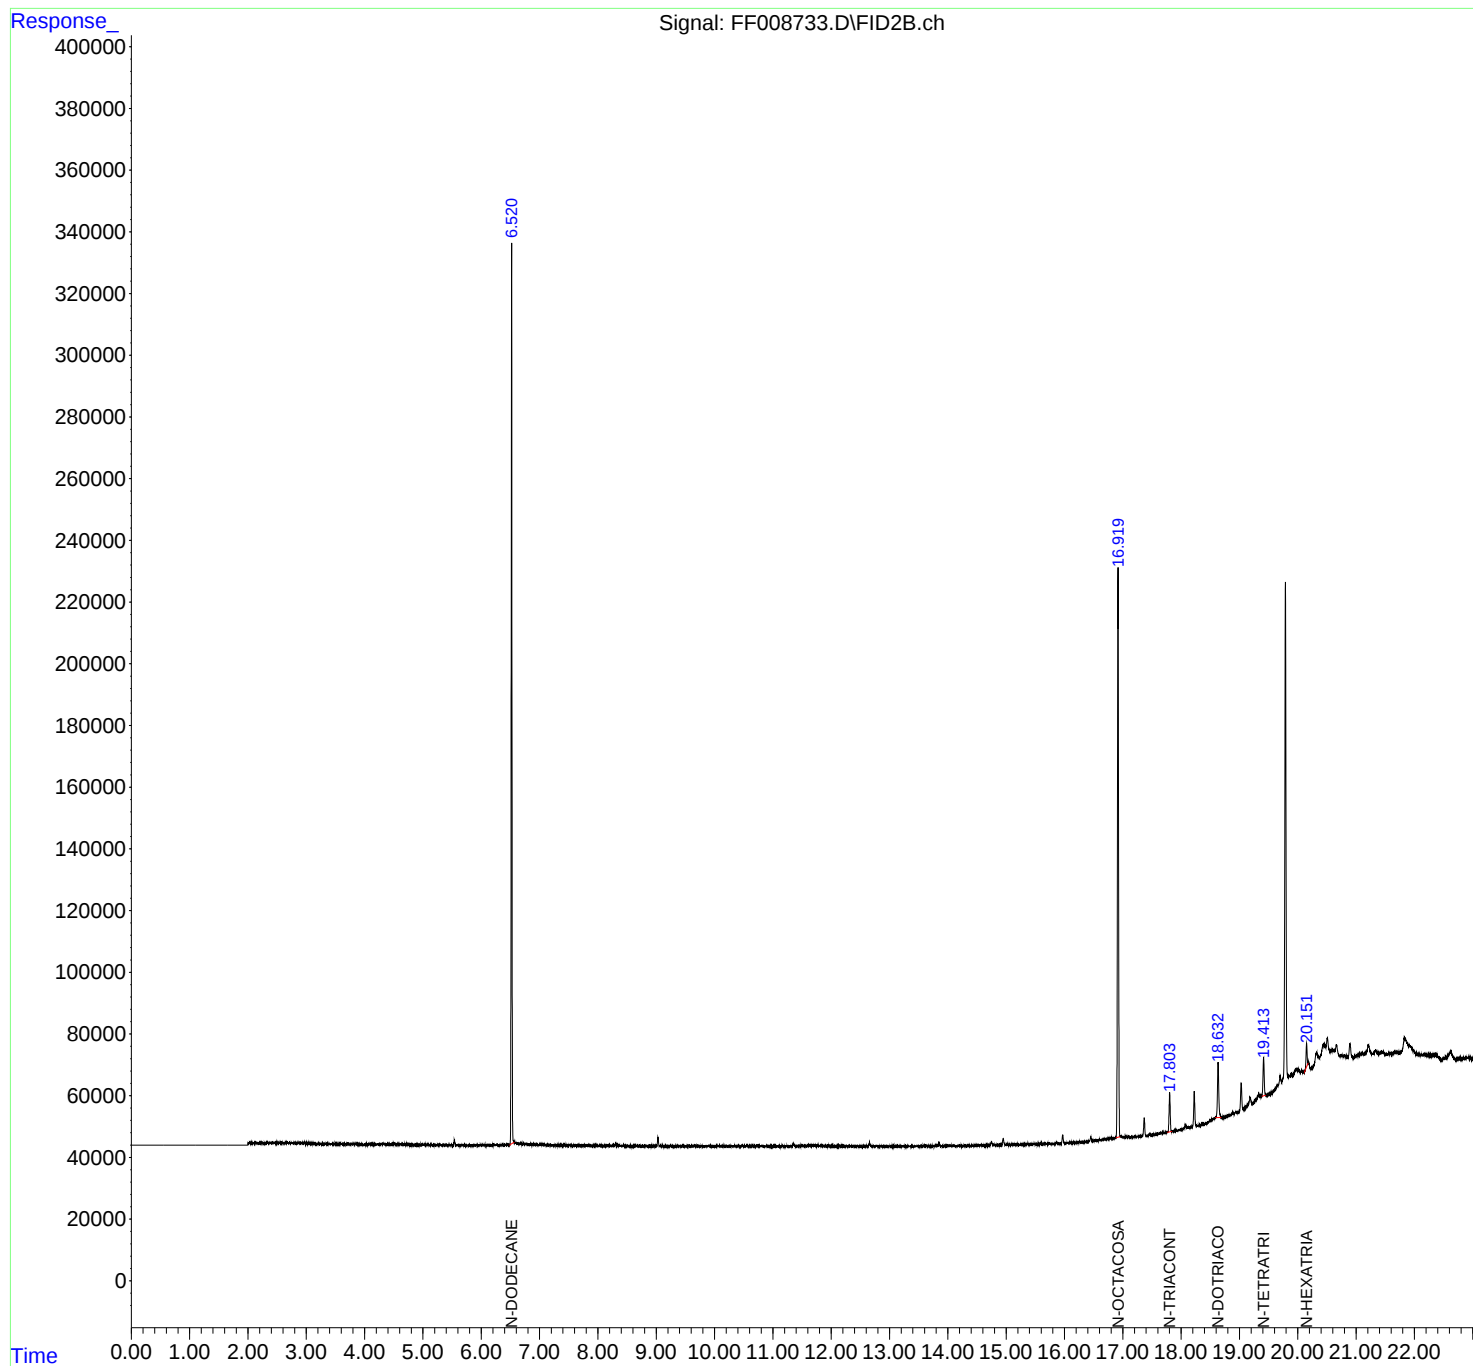


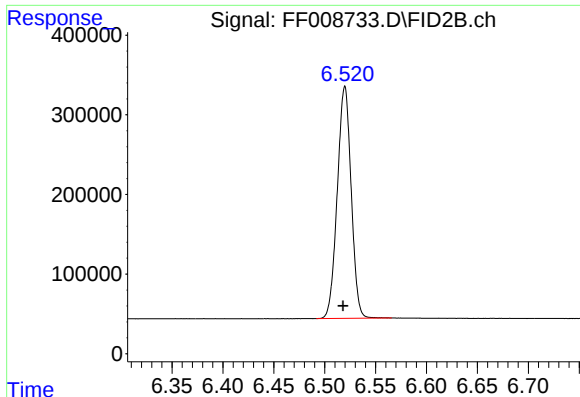

#3 N-DODECANE


R.T.: 6.520 min
Delta R.T.: 0.002 min
Response: 2768464
Conc: 20.36 ug/ml

Instrument :
FID_F
ClientSampleId :

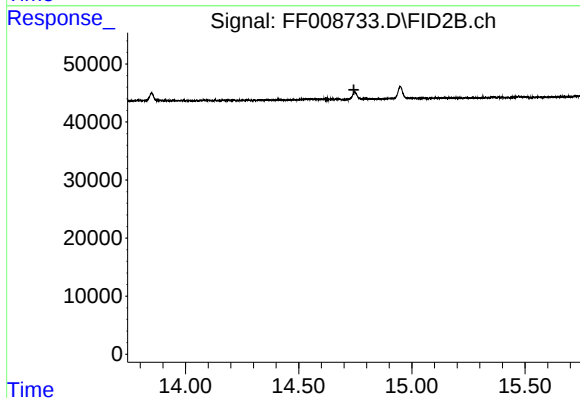


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.744 min
Response: 0
Conc: N.D.

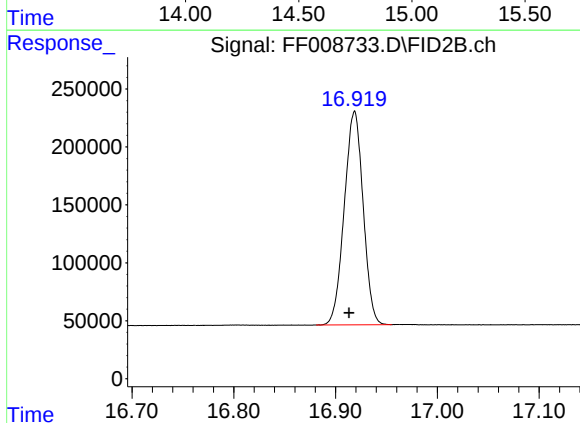


#12 N-OCTACOSANE

R.T.: 16.919 min
Delta R.T.: 0.006 min
Response: 2372544
Conc: 19.18 ug/ml

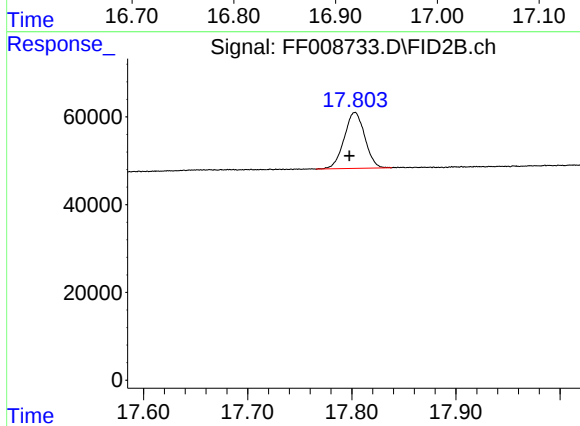

#13 N-TRIACONTANE


R.T.: 17.803 min
Delta R.T.: 0.005 min
Response: 174848
Conc: 1.46 ug/ml

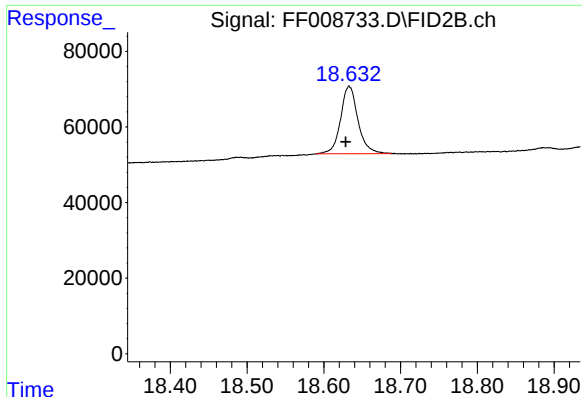

#14 N-DOTRIACONTANE


R.T.: 18.633 min
Delta R.T.: 0.004 min
Response: 280776
Conc: 2.40 ug/ml

Instrument :
FID_F
ClientSampleId :

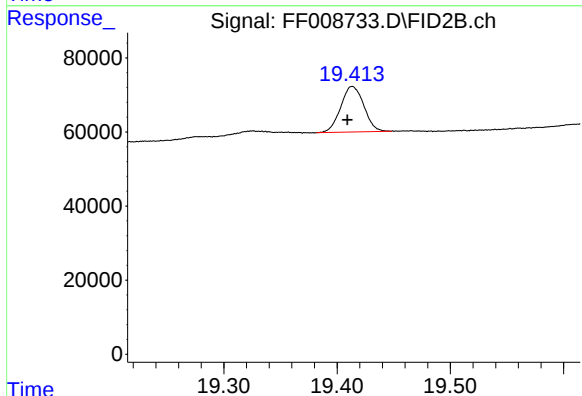

#15 N-TETRATRIACONTANE

R.T.: 19.414 min
Delta R.T.: 0.004 min
Response: 174870
Conc: 1.67 ug/ml

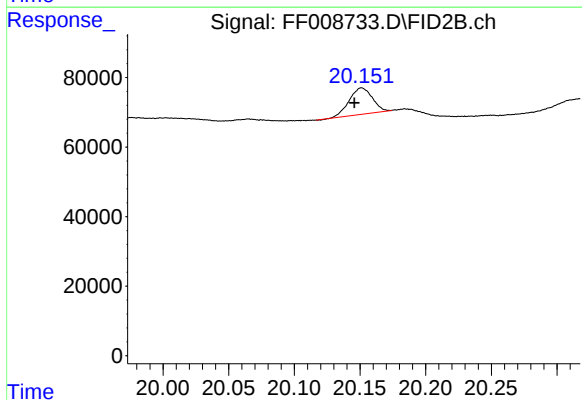

#16 N-HEXATRIACONTANE

R.T.: 20.151 min
Delta R.T.: 0.006 min
Response: 92924
Conc: 0.99 ug/ml