

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF070623\
 Data File : FF013052.D
 Signal(s) : FID2B.ch
 Acq On : 06 Jul 2023 08:54
 Operator : YP\AJ
 Sample : MECL2
 Misc :
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jul 06 13:33:01 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF070623.M
 Quant Title :
 QLast Update : Thu Jul 06 13:26:17 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.991f	67358	0.567 ug/ml
Target Compounds			
14) N-DOTRIACONTANE	18.827	56955	0.495 ug/ml
15) N-TETRATRIACONTANE	19.607	65387	0.652 ug/ml
16) N-HEXATRIACONTANE	20.347	57761	0.672 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF070623\
Data File : FF013052.D
Signal(s) : FID2B.ch
Acq On : 06 Jul 2023 08:54
Operator : YP\AJ
Sample : MECL2
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jul 06 13:33:01 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF070623.M
Quant Title :
QLast Update : Thu Jul 06 13:26:17 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

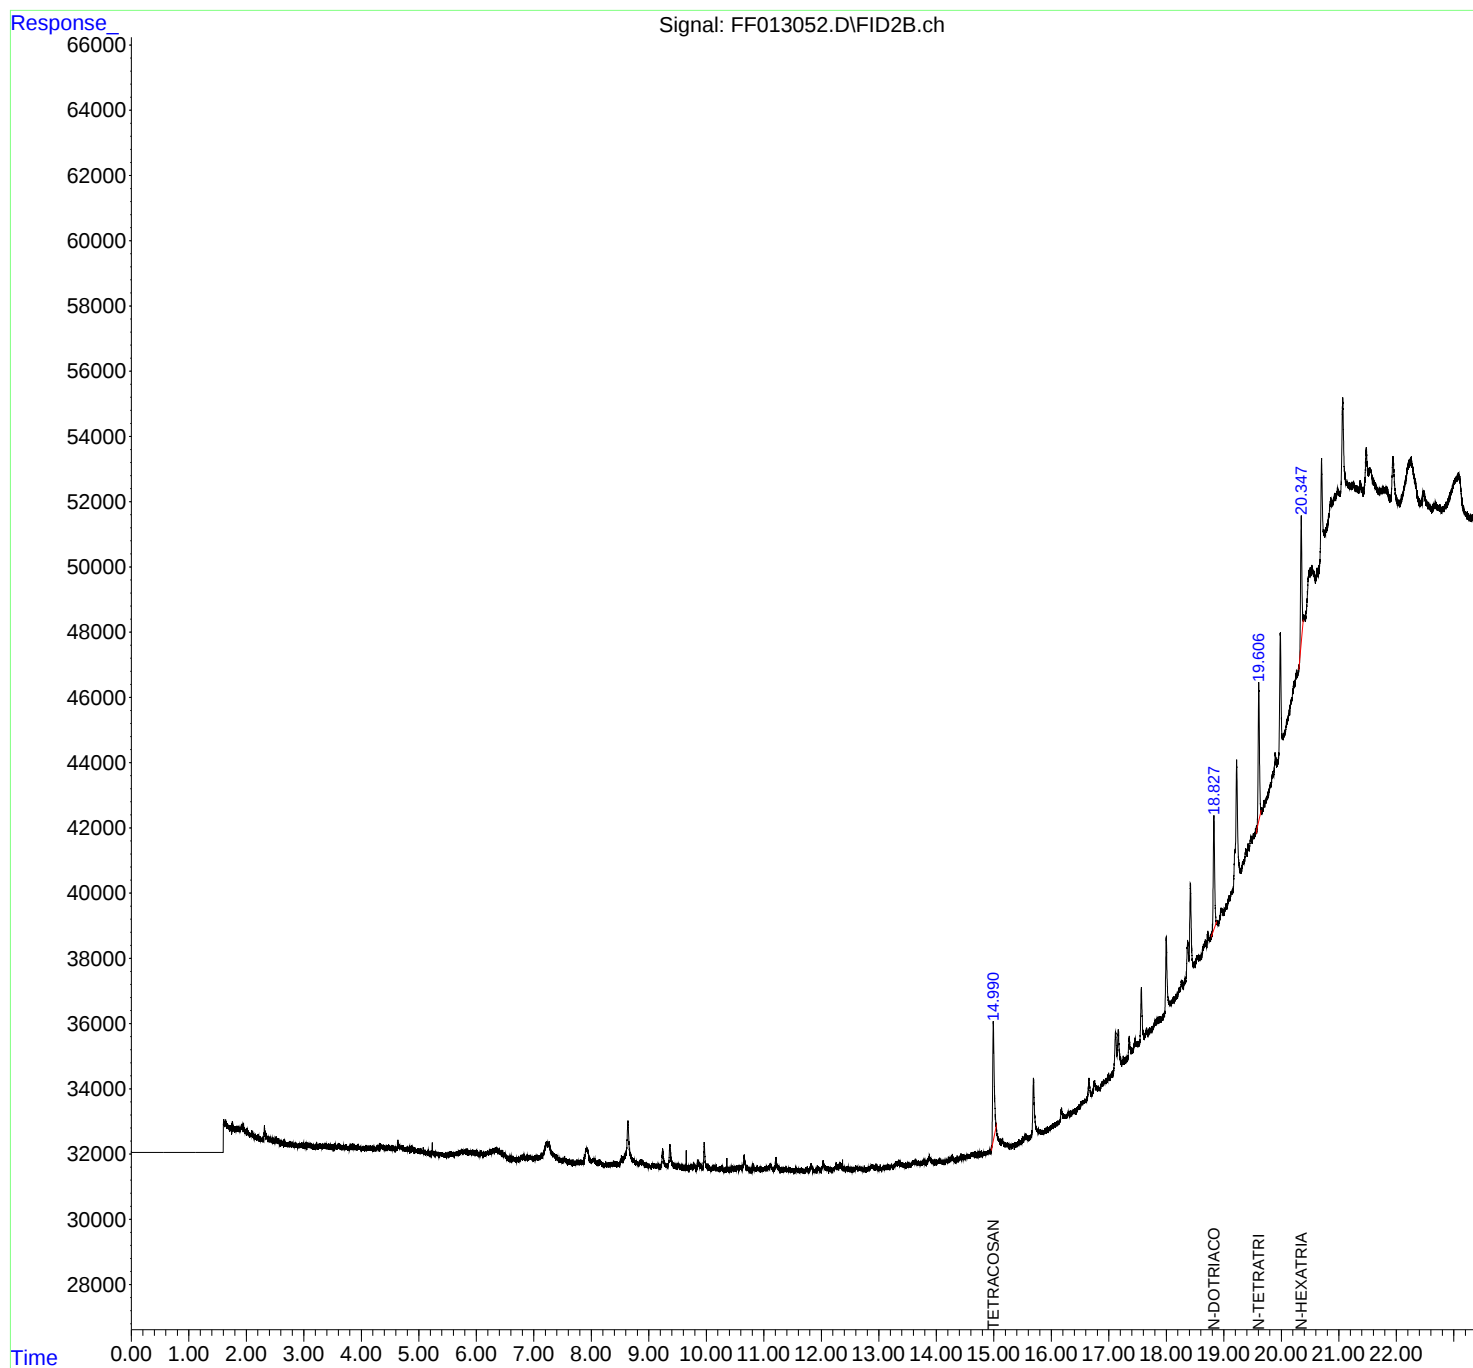


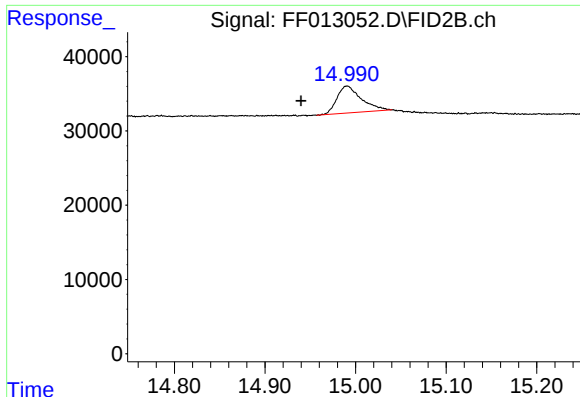

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.991 min
Delta R.T.: 0.051 min
Response: 67358
Conc: 0.57 ug/ml

Instrument :
FID_F
ClientSampleId :

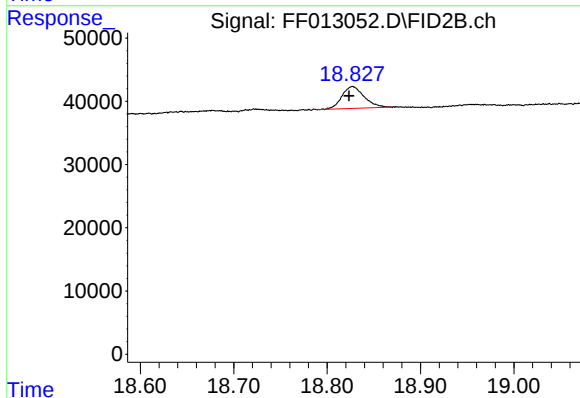


#14 N-DOTRIACONTANE

R.T.: 18.827 min
Delta R.T.: 0.004 min
Response: 56955
Conc: 0.50 ug/ml

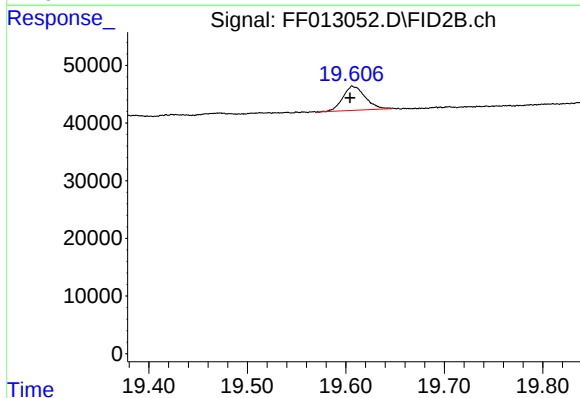

#15 N-TETRATRIACONTANE

R.T.: 19.607 min
Delta R.T.: 0.003 min
Response: 65387
Conc: 0.65 ug/ml

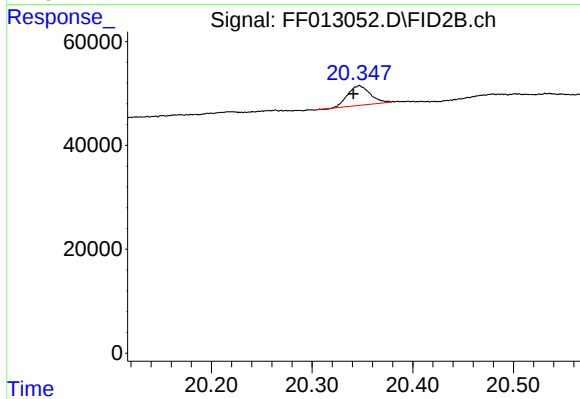

#16 N-HEXATRIACONTANE

R.T.: 20.347 min
Delta R.T.: 0.006 min
Response: 57761
Conc: 0.67 ug/ml