

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF070721\
Data File : FF008740.D
Signal(s) : FID2B.ch
Acq On : 07 Jul 2021 11:11
Operator : DD\AJ
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jul 08 01:47:35 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF062321.M
Quant Title :
QLast Update : Thu Jun 24 08:07:11 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds

3)	N-DODECANE	6.517	3189151	23.449 ug/ml
12)	N-OCTACOSANE	16.919	2779974	22.476 ug/ml
13)	N-TRIACONTANE	17.800	322299	2.689 ug/ml
14)	N-DOTRIACONTANE	18.634	479260	4.091 ug/ml
15)	N-TETRATRIACONTANE	19.413	323479	3.094 ug/ml
16)	N-HEXATRIACONTANE	20.152	194137	2.067 ug/ml
17)	N-OCTATRIACONTANE	20.895	147150	1.785 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF070721\
Data File : FF008740.D
Signal(s) : FID2B.ch
Acq On : 07 Jul 2021 11:11
Operator : DD\AJ
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jul 08 01:47:35 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF062321.M
Quant Title :
QLast Update : Thu Jun 24 08:07:11 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

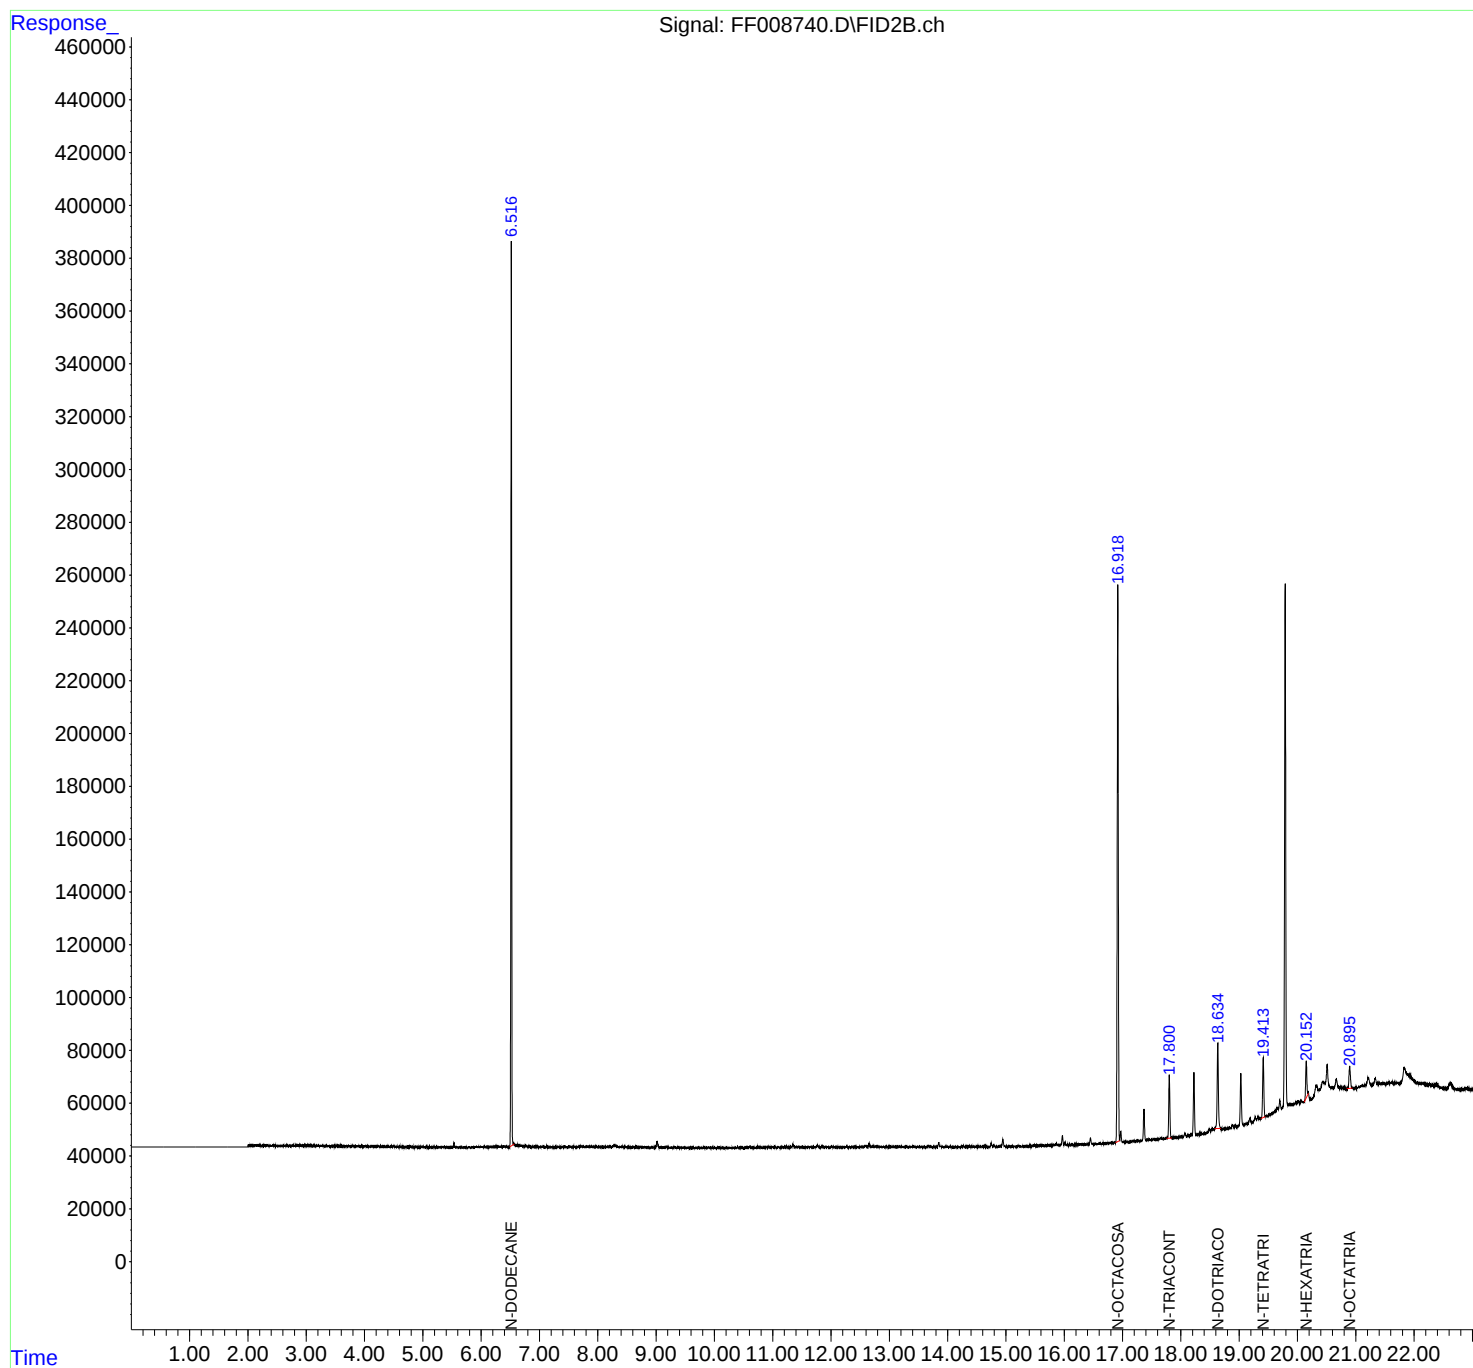


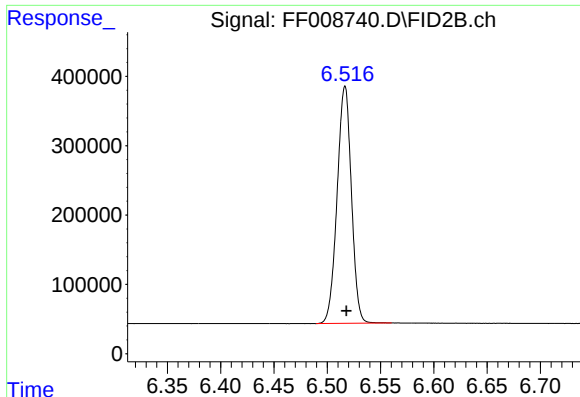

#3 N-DODECANE


R.T.: 6.517 min
Delta R.T.: -0.001 min
Response: 3189151
Conc: 23.45 ug/ml

Instrument :
FID_F
ClientSampleId :

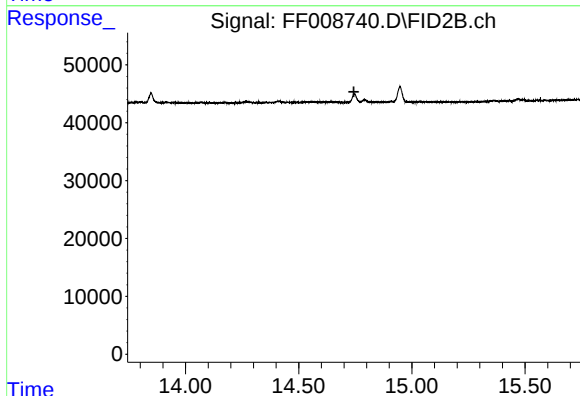


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.744 min
Response: 0
Conc: N.D.

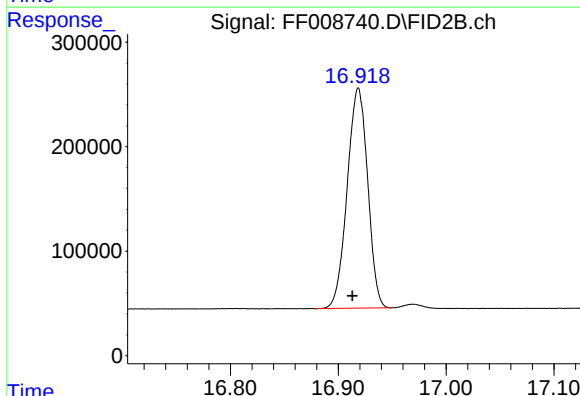


#12 N-OCTACOSANE

R.T.: 16.919 min
Delta R.T.: 0.006 min
Response: 2779974
Conc: 22.48 ug/ml

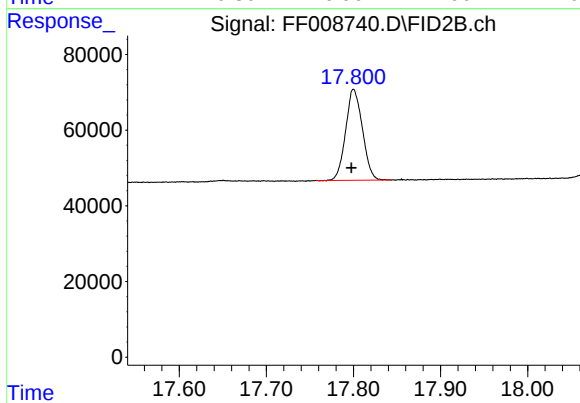

#13 N-TRIACONTANE


R.T.: 17.800 min
Delta R.T.: 0.002 min
Response: 322299
Conc: 2.69 ug/ml

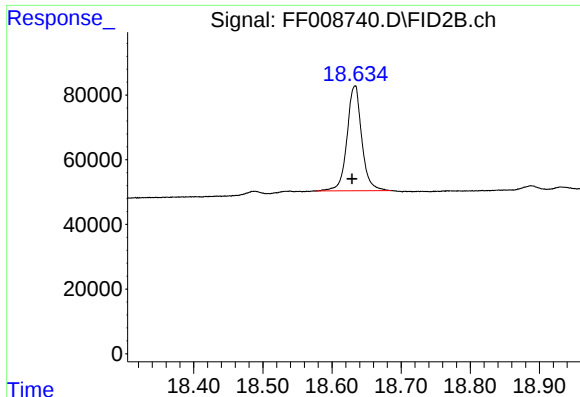

#14 N-DOTRIACONTANE


R.T.: 18.634 min
Delta R.T.: 0.005 min
Response: 479260
Conc: 4.09 ug/ml

Instrument :
FID_F
ClientSampleId :

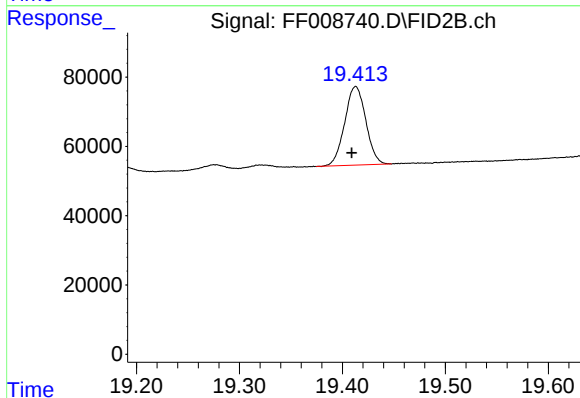


#15 N-TETRATRIACONTANE

R.T.: 19.413 min
Delta R.T.: 0.004 min
Response: 323479
Conc: 3.09 ug/ml

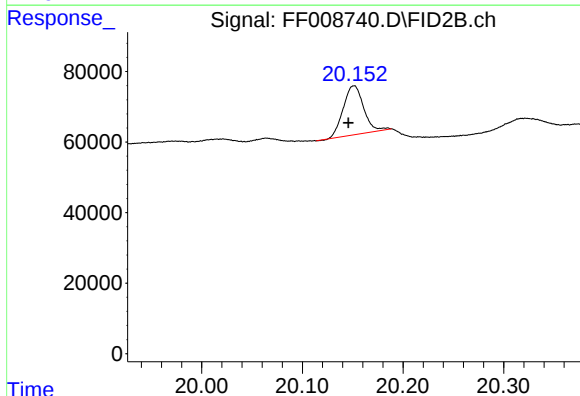

#16 N-HEXATRIACONTANE

R.T.: 20.152 min
Delta R.T.: 0.006 min
Response: 194137
Conc: 2.07 ug/ml

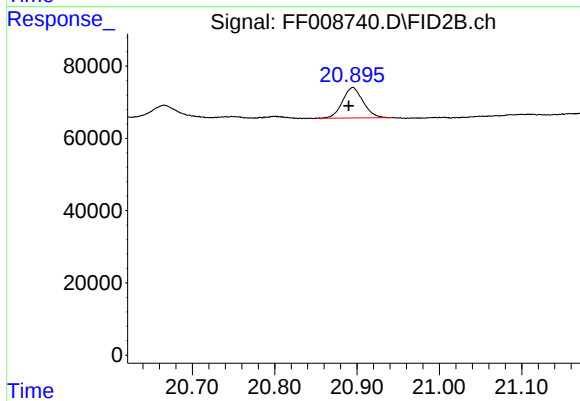

#17 N-OCTATRIACONTANE

R.T.: 20.895 min
Delta R.T.: 0.005 min
Response: 147150
Conc: 1.79 ug/ml